

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
 Data File : BN013674.D
 Acq On : 18 Feb 2021 16:28
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Feb 18 16:59:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 18 10:50:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.547	152	5743	0.40	ng	0.00
7) Naphthalene-d8	10.302	136	23191	0.40	ng	0.00
13) Acenaphthene-d10	14.181	164	13033	0.40	ng	0.00
19) Phenanthrene-d10	16.934	188	27820	0.40	ng	# 0.00
29) Chrysene-d12	21.133	240	26918	0.40	ng	# 0.00
36) Perylene-d12	23.301	264	25269	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.180	112	5573	0.45	ng	0.00
5) Phenol-d6	6.726	99	7030	0.45	ng	0.00
8) Nitrobenzene-d5	8.680	82	4977	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	11.902	152	14237	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.678	330	1477	0.40	ng	0.00
15) 2-Fluorobiphenyl	12.798	172	19066	0.39	ng	0.00
27) Fluoranthene-d10	18.970	212	29321	0.39	ng	0.00
31) Terphenyl-d14	19.581	244	23828	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.182	88	2473	0.38	ng	94
3) n-Nitrosodimethylamine	3.497	42	1863	0.40	ng	91
6) bis(2-Chloroethyl)ether	6.984	93	5726	0.41	ng	98
9) Naphthalene	10.353	128	22611	0.40	ng	99
10) Hexachlorobutadiene	10.644	225	3718	0.39	ng	# 99
12) 2-Methylnaphthalene	11.978	142	15483	0.40	ng	99
16) Acenaphthylene	13.890	152	18625	0.37	ng	100
17) Acenaphthene	14.245	154	14262	0.40	ng	99
18) Fluorene	15.234	166	17623	0.39	ng	100
20) 4,6-Dinitro-2-methylph...	15.323	198	904	0.38	ng	# 83
21) 4-Bromophenyl-phenylether	16.131	248	5157	0.37	ng	95
22) Hexachlorobenzene	16.240	284	5841	0.38	ng	100
23) Atrazine	16.410	200	3231	0.37	ng	100
24) Pentachlorophenol	16.581	266	1276	0.48	ng	93
25) Phenanthrene	16.970	178	29312	0.39	ng	100
26) Anthracene	17.055	178	23461	0.38	ng	100
28) Fluoranthene	19.000	202	31882	0.38	ng	99
30) Pyrene	19.362	202	32443	0.40	ng	100
32) Benzo(a)anthracene	21.123	228	27671	0.39	ng	99
33) Chrysene	21.165	228	32039	0.39	ng	99
34) Bis(2-ethylhexyl)phtha...	21.070	149	8655	0.41	ng	99
35) Indeno(1,2,3-cd)pyrene	25.444	276	35993	0.42	ng	99
37) Benzo(b)fluoranthene	22.654	252	31719	0.36	ng	97
38) Benzo(k)fluoranthene	22.695	252	34317	0.39	ng	96
39) Benzo(a)pyrene	23.205	252	29374	0.40	ng	99
40) Dibenzo(a,h)anthracene	25.461	278	29837	0.37	ng	97
41) Benzo(g,h,i)perylene	26.098	276	30980	0.37	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
Data File : BN013674.D
Acq On : 18 Feb 2021 16:28
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Feb 18 16:59:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 10:50:10 2021
Response via : Initial Calibration




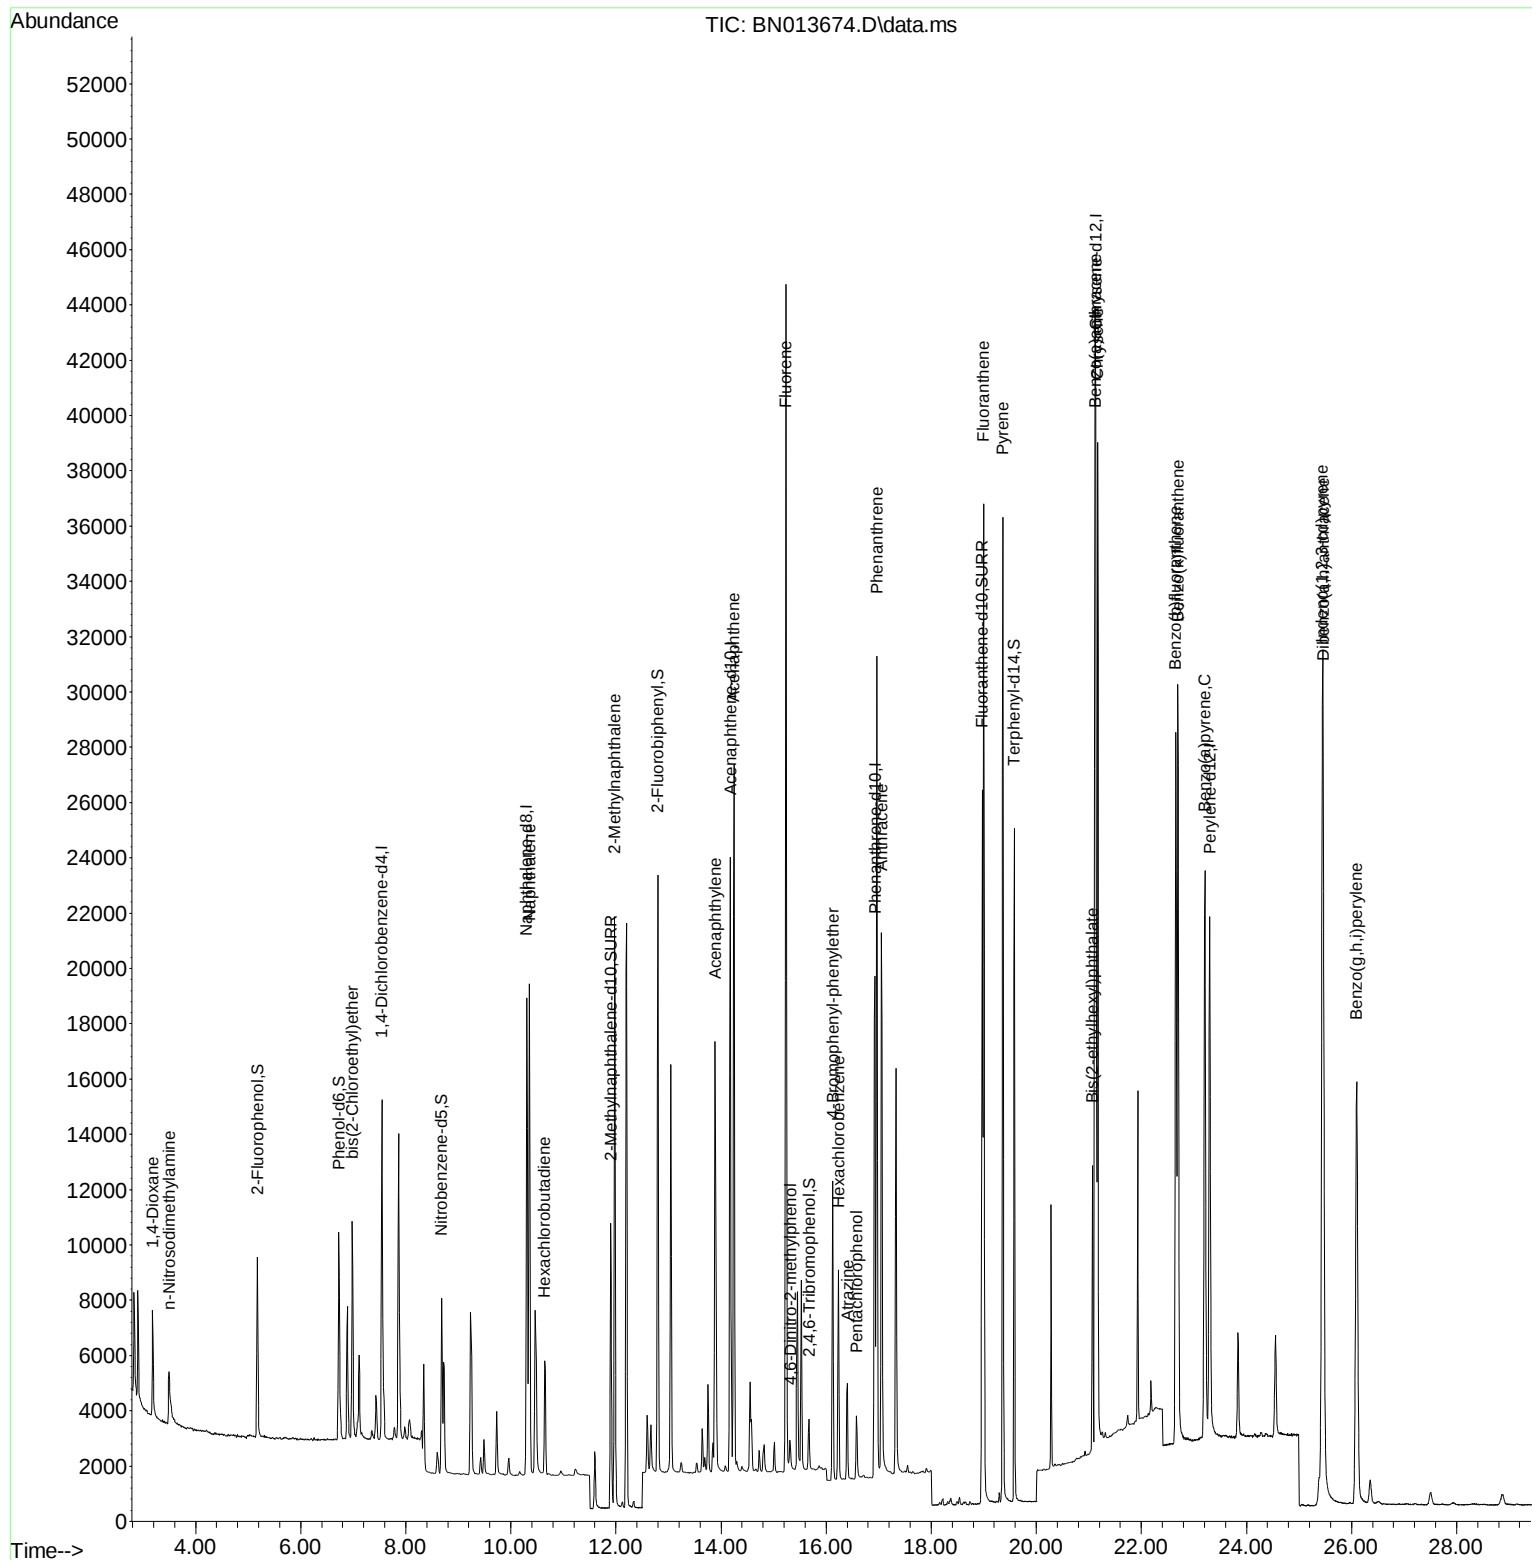


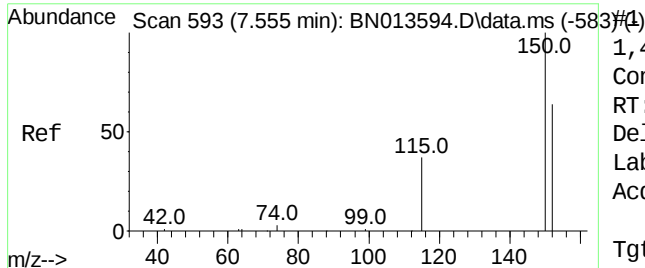

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.547 min Scan# 592
 Delta R.T. 0.000 min
 Lab File: BN013674.D
 Acq: 18 Feb 2021 16:28




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	152	Resp:	5743
Ion	Ratio	Lower	Upper
152	100		
150	158.5	121.8	182.8
115	61.4	46.6	69.8

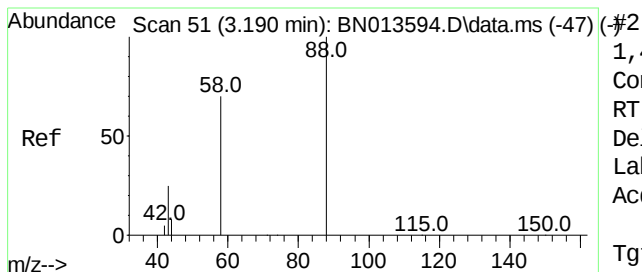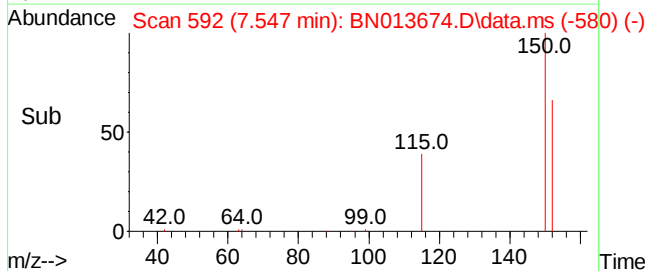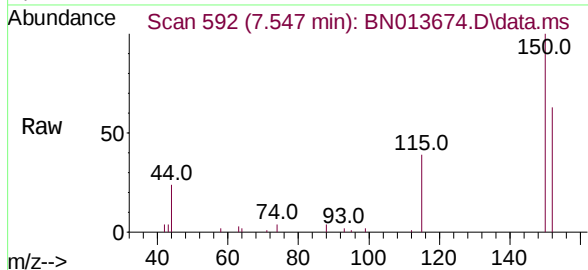

1,4-Dioxane
 Concen: 0.38 ng
 RT: 3.182 min Scan# 50
 Delta R.T. -0.000 min
 Lab File: BN013674.D
 Acq: 18 Feb 2021 16:28

Tgt Ion:	88	Resp:	2473
Ion	Ratio	Lower	Upper
88	100		
58	75.9	64.6	96.8
43	29.6	26.6	40.0

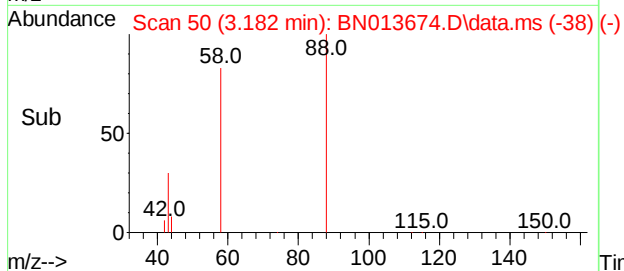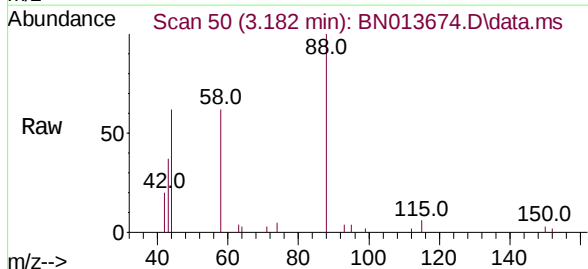




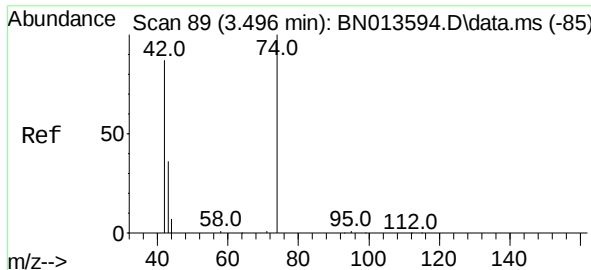


n-Nitrosodimethylamine
Concen: 0.40 ng
RT: 3.497 min Scan# 89
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 42 Resp: 1863




Ion	Ratio	Lower	Upper
42	100		
74	129.3	95.0	142.6
44	6.6	5.8	8.8

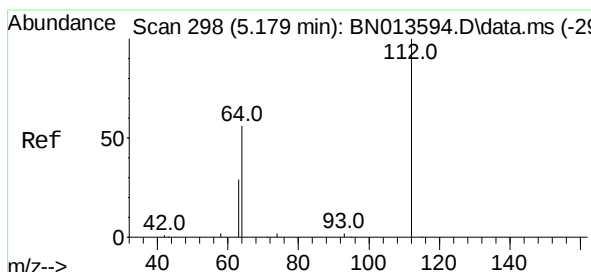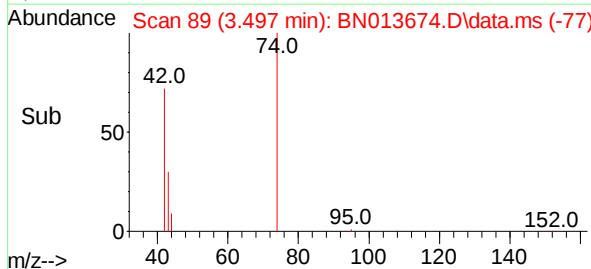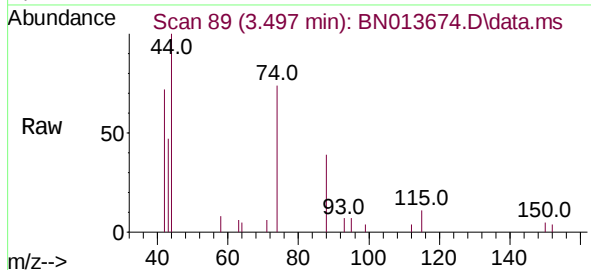


2-Fluorophenol
Concen: 0.45 ng
RT: 5.180 min Scan# 298
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion: 112 Resp: 5573

Ion	Ratio	Lower	Upper
112	100		
64	55.7	44.3	66.5
63	28.2	23.0	34.6


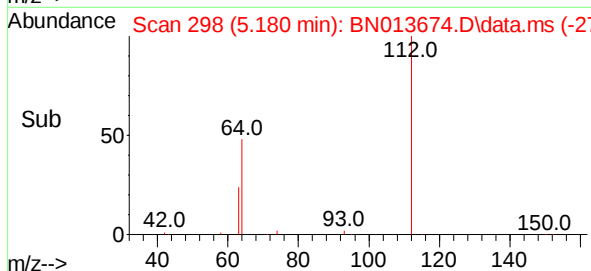

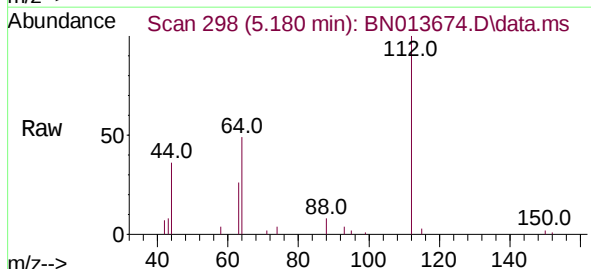


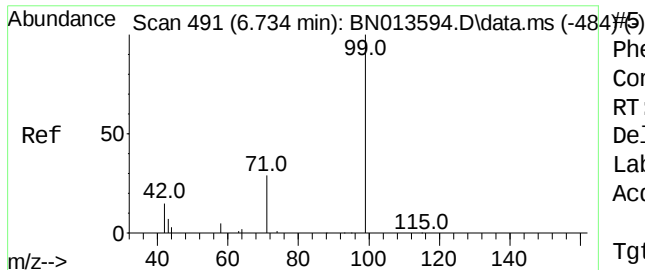

Phenol-d6
Concen: 0.45 ng
RT: 6.726 min Scan# 490
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	99	Resp:	7030
Ion	Ratio	Lower	Upper
99	100		
42	18.6	15.2	22.8
71	30.8	26.1	39.1

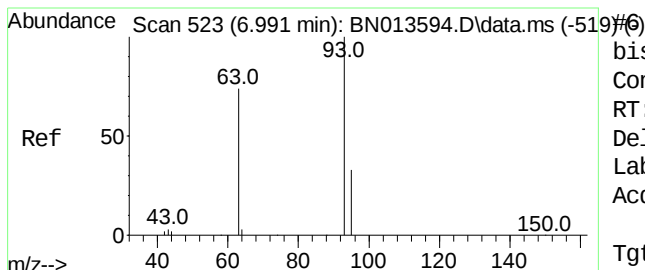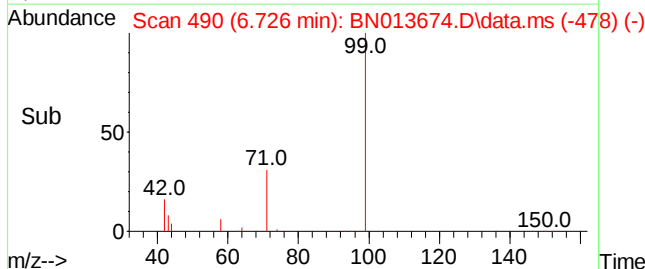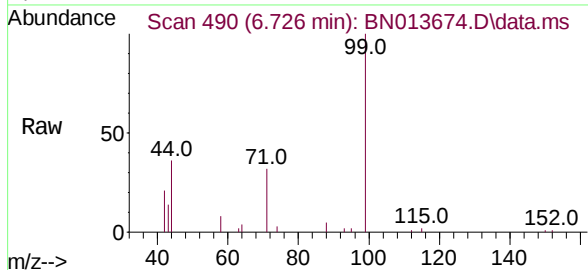


bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 6.984 min Scan# 522
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	93	Resp:	5726
Ion	Ratio	Lower	Upper
93	100		
63	77.6	60.8	91.2
95	33.5	26.0	39.0

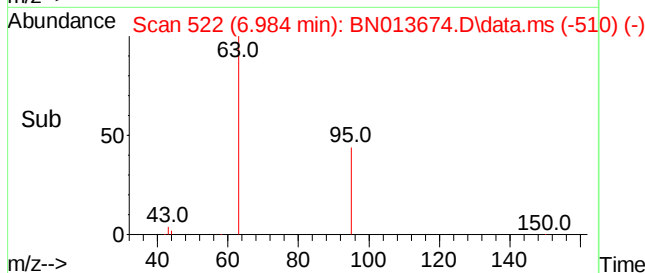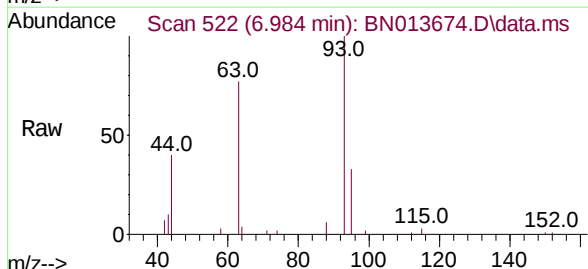



Abundance Scan 845 (10.315 min): BN013594.D\data.ms (-8367-)

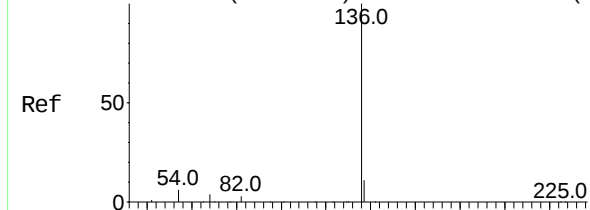


Naphthalene-d8
Concen: 0.40 ng
RT: 10.302 min Scan# 844
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	23191
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.6
54	8.6	6.4	9.6
68	6.4	4.5	6.7

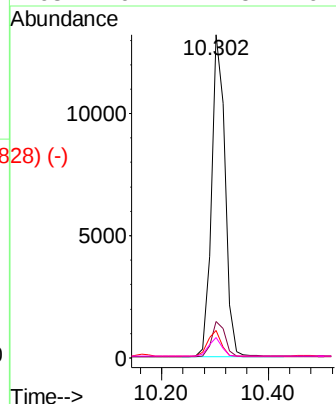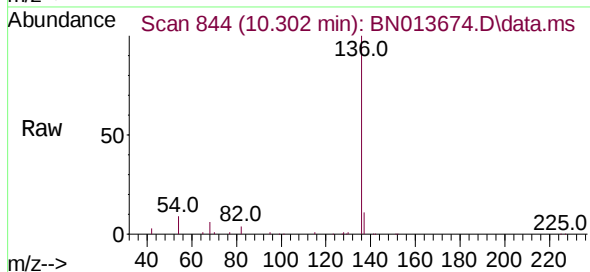

Abundance Scan 844 (10.302 min): BN013674.D\data.ms (-828) (-)


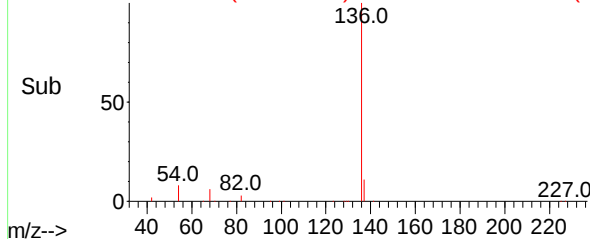


Abundance Scan 717 (8.692 min): BN013594.D\data.ms (-7137-)

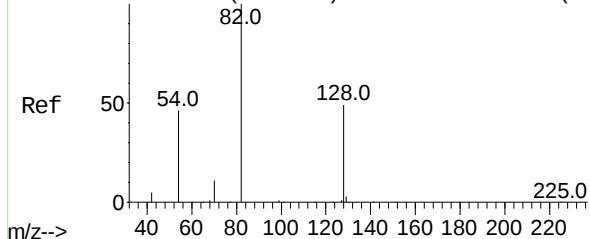


Nitrobenzene-d5
Concen: 0.39 ng
RT: 8.680 min Scan# 716
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion:	82	Resp:	4977
Ion	Ratio	Lower	Upper
82	100		
128	40.8	39.2	58.8
54	53.8	40.1	60.1

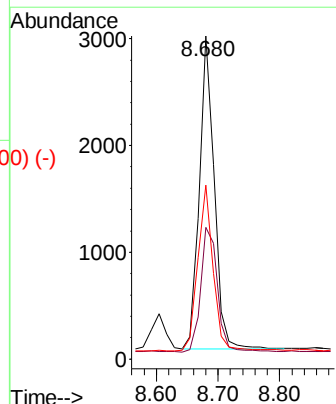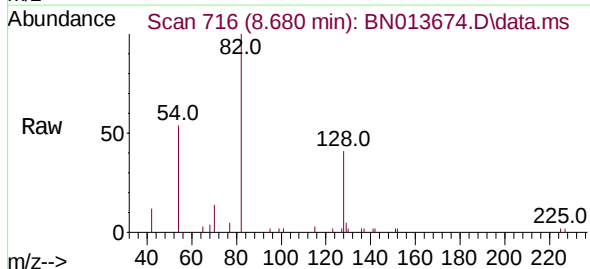

Abundance Scan 716 (8.680 min): BN013674.D\data.ms (-700) (-)

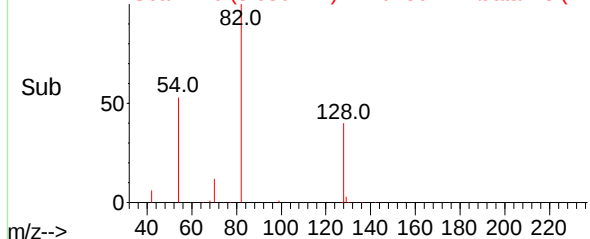




Abundance Scan 849 (10.365 min): BN013594.D\data.ms (-849) (-)




Naphthalene
Concen: 0.40 ng
RT: 10.353 min Scan# 848
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	128	Resp:	22611
Ion Ratio	Lower	Upper	
128	100		
129	11.3	9.0	13.4
127	13.4	10.4	15.6

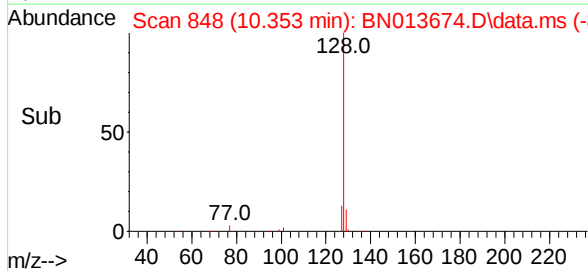
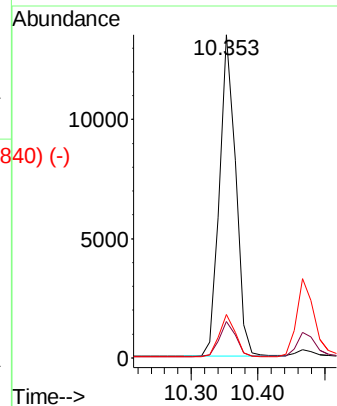
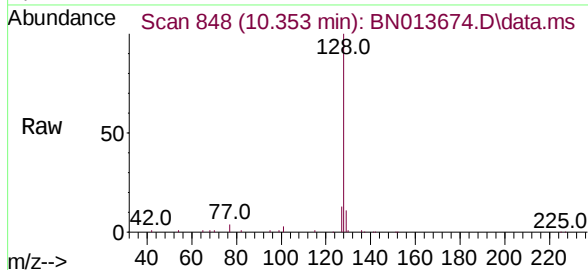


Abundance Scan 872 (10.657 min): BN013594.D\data.ms (-866) (-)




Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.644 min Scan# 871
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	225	Resp:	3718
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.6	51.2	76.8

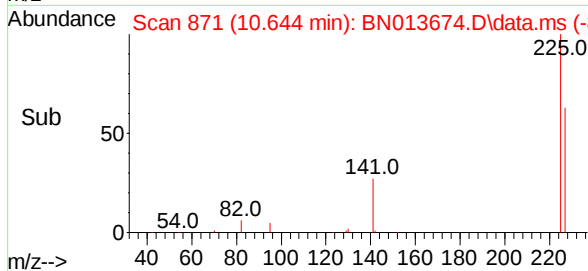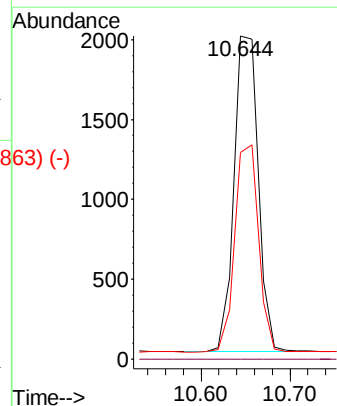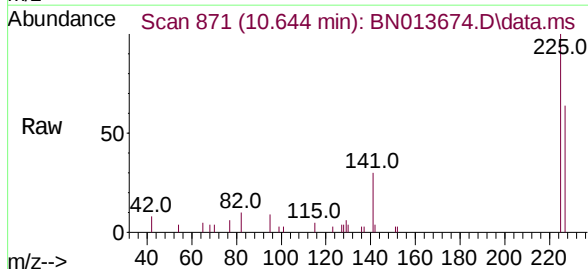



Abundance Scan 1030 (11.911 min): BN013594.D\data.ms (-1011) (-)




2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 11.902 min Scan# 1028
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 14237
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2

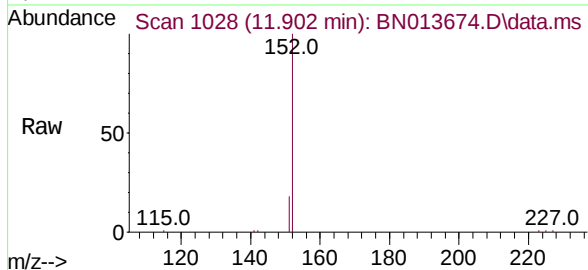

Abundance Scan 1028 (11.902 min): BN013674.D\data.ms (-983) (-)





Abundance Scan 1046 (11.982 min): BN013594.D\data.ms (-1036) (-)




2-Methylnaphthalene
Concen: 0.40 ng
RT: 11.978 min Scan# 1045
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion:142 Resp: 15483
Ion Ratio Lower Upper
142 100
141 87.4 70.5 105.7
115 32.5 27.4 41.0

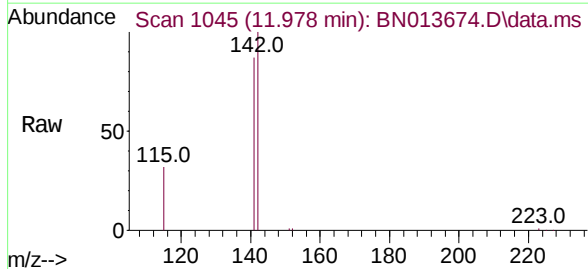

Abundance Scan 1045 (11.978 min): BN013674.D\data.ms (-1023) (-)

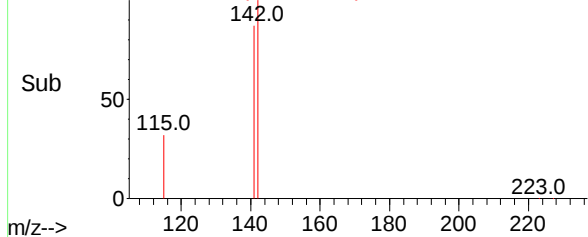



Abundance Scan 1296 (14.181 min): BN013594.D\data.ms (-1280) (-)




Acenaphthene-d10
Concen: 0.40 ng
RT: 14.181 min Scan# 1296
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	164	Resp:	13033
Ion Ratio	Lower	Upper	
164	100		
162	98.1	79.6	119.4
160	43.7	36.0	54.0

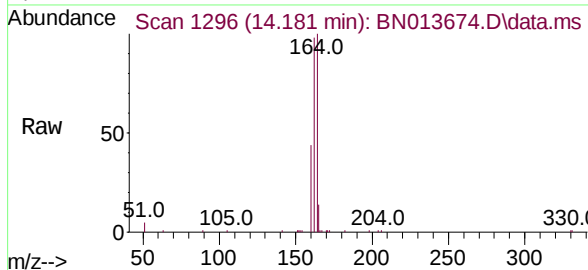

Abundance Scan 1296 (14.181 min): BN013674.D\data.ms (-1280) (-)


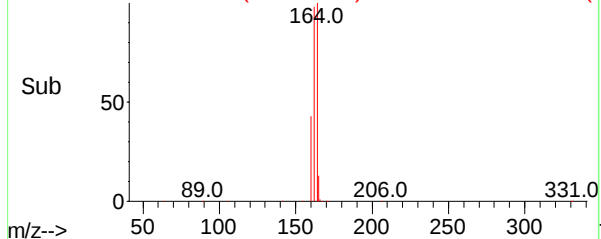


Abundance Scan 1414 (15.678 min): BN013594.D\data.ms (-1406) (-)





2,4,6-Tribromophenol
Concen: 0.40 ng
RT: 15.678 min Scan# 1414
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	330	Resp:	1477
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	36.8	26.8	40.2

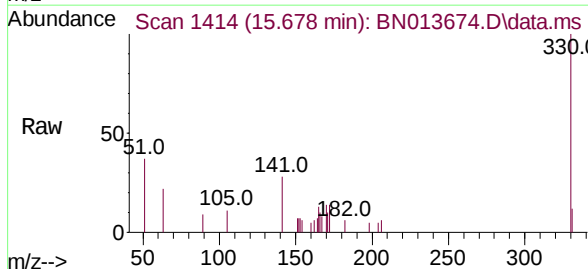

Abundance Scan 1414 (15.678 min): BN013674.D\data.ms (-1406) (-)




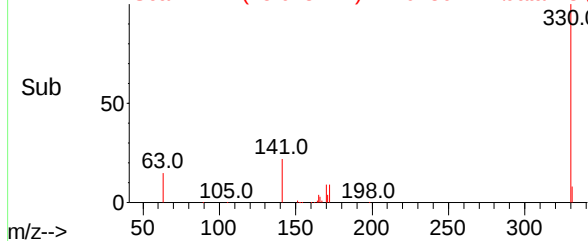


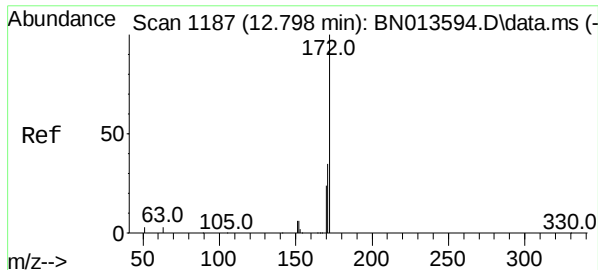

2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.798 min Scan# 1187
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	172	Resp:	19066
Ion	Ratio	Lower	Upper
172	100		
171	34.5	28.6	42.8
170	22.1	18.9	28.3

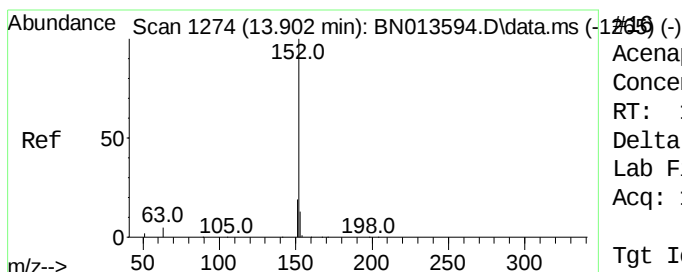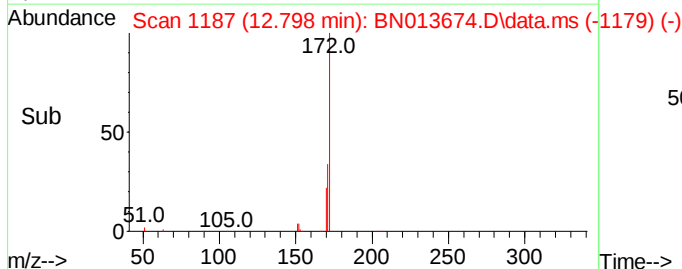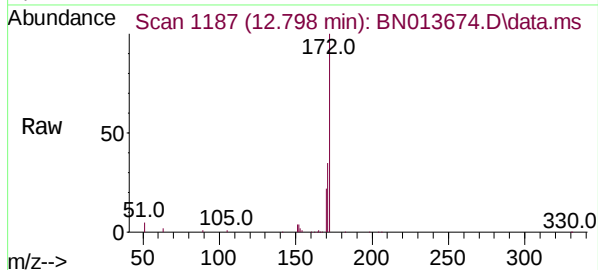

Acenaphthylene
Concen: 0.37 ng
RT: 13.890 min Scan# 1273
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion:	152	Resp:	18625
Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.7	23.5
153	13.0	10.5	15.7

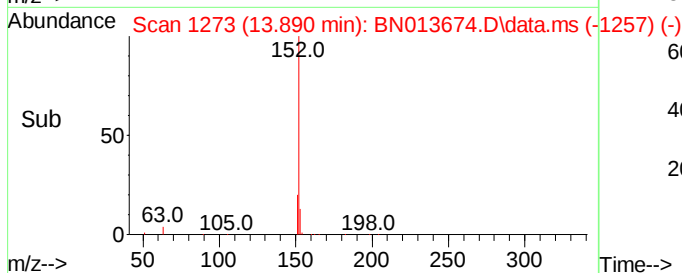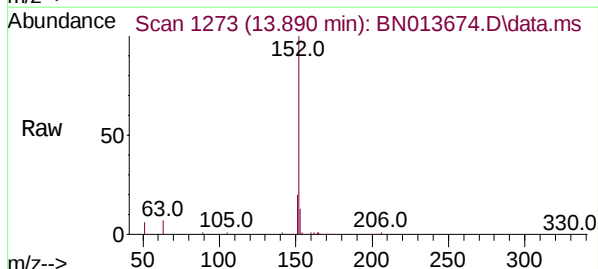




Abundance Scan 1301 (14.245 min): BN013594.D\data.ms (-1295) (-)

Acenaphthene
Concen: 0.40 ng
RT: 14.245 min Scan# 1301
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

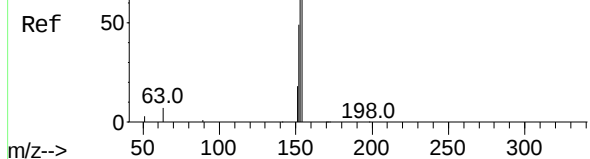


Tgt Ion:	154	Resp:	14262
Ion Ratio	Lower	Upper	
154	100		
153	109.3	88.4	132.6
152	52.5	43.0	64.4

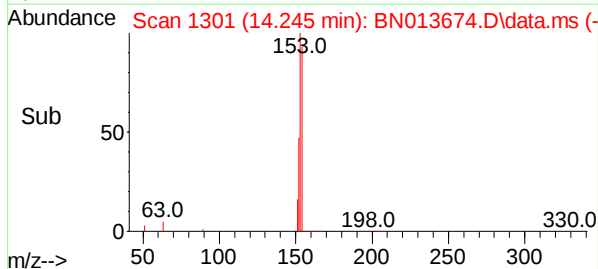

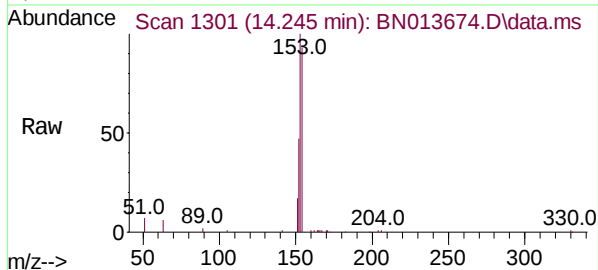



Abundance Scan 1379 (15.234 min): BN013594.D\data.ms (-1313) (-)

Fluorene
Concen: 0.39 ng
RT: 15.234 min Scan# 1379
Delta R.T. -0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

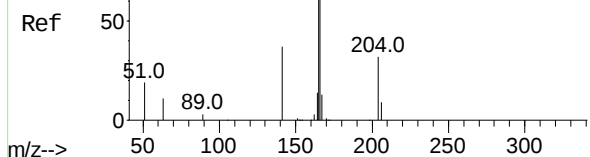

Tgt Ion:	166	Resp:	17623
Ion Ratio	Lower	Upper	
166	100		
165	97.3	77.8	116.8
167	13.5	10.6	16.0


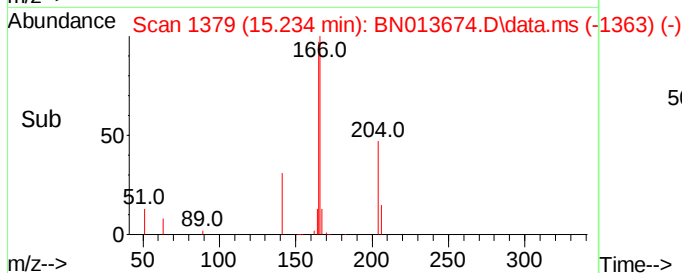

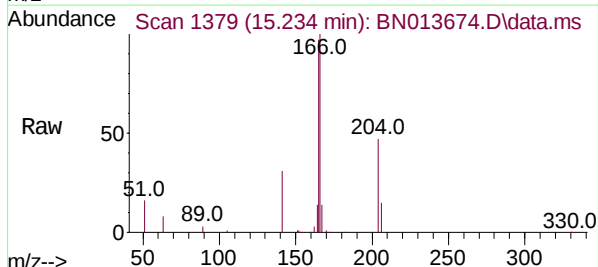


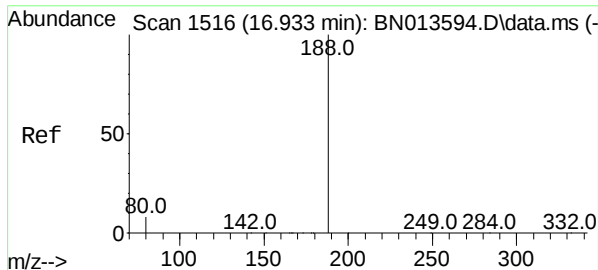

Phenanthrene-d10
 Concen: 0.40 ng
 RT: 16.934 min Scan# 1516
 Delta R.T. 0.001 min
 Lab File: BN013674.D
 Acq: 18 Feb 2021 16:28




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	188	Resp:	27820
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	6.2	9.0	13.6#

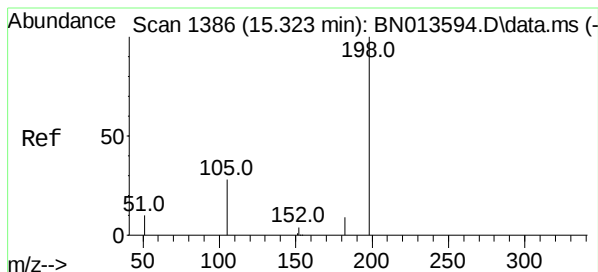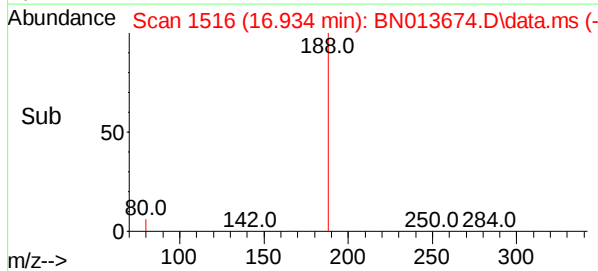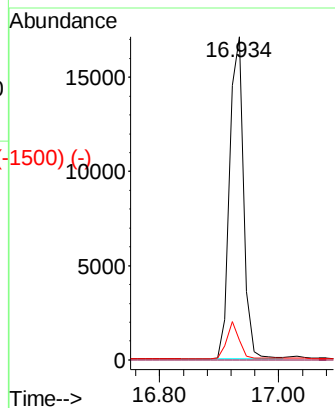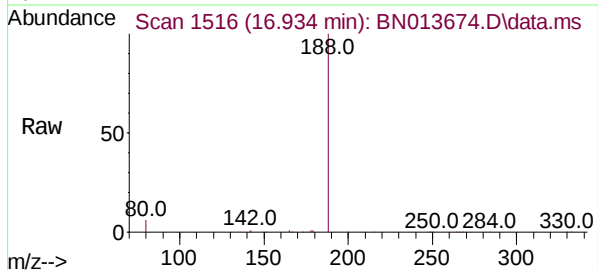


4,6-Dinitro-2-methylphenol
 Concen: 0.38 ng
 RT: 15.323 min Scan# 1386
 Delta R.T. -0.000 min
 Lab File: BN013674.D
 Acq: 18 Feb 2021 16:28

Tgt Ion:	198	Resp:	904
Ion Ratio	Lower	Upper	
198	100		
51	97.8	61.7	92.5#
105	43.4	33.0	49.6

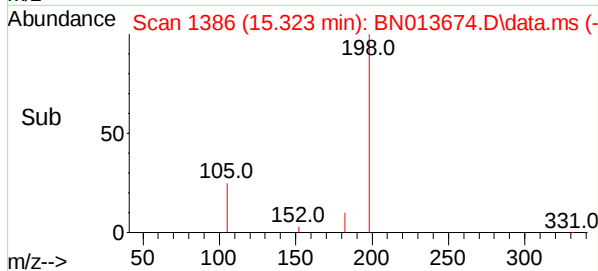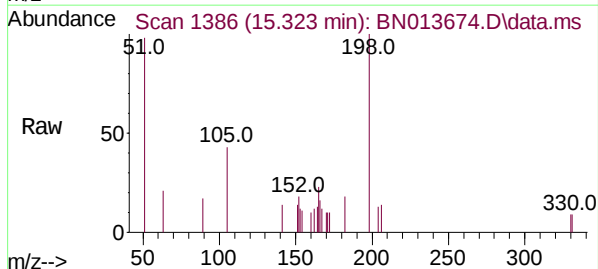



Abundance Scan 1451 (16.142 min): BN013594.D\data.ms (-1425) (-)

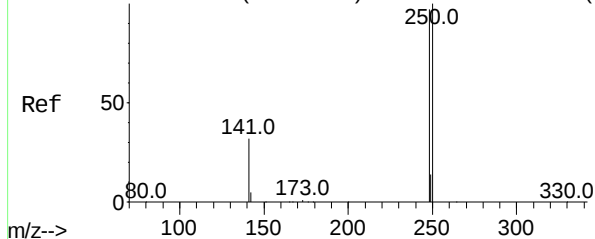


4-Bromophenyl-phenylether
Concen: 0.37 ng
RT: 16.131 min Scan# 1450
Delta R.T. 0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion	Ratio	Lower	Upper
248	100		
250	97.3	75.5	113.3
141	61.6	53.8	80.8

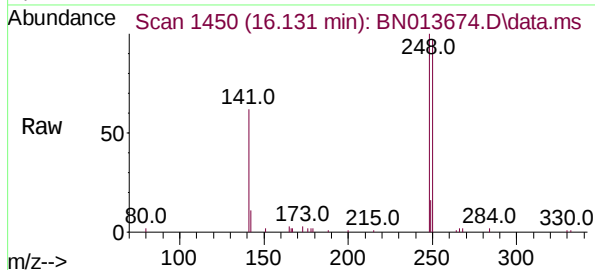

Abundance Scan 1450 (16.131 min): BN013674.D\data.ms (-1442) (-)


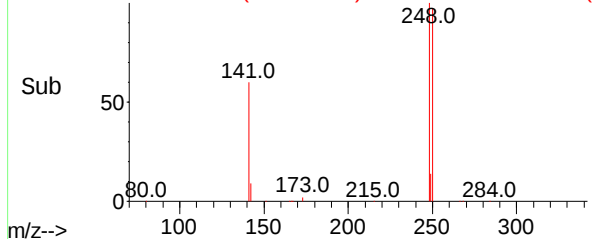


Abundance Scan 1460 (16.252 min): BN013594.D\data.ms (-1425) (-)

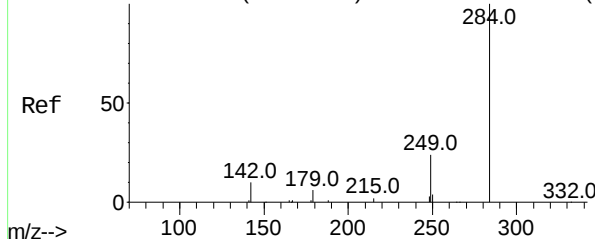


Hexachlorobenzene
Concen: 0.38 ng
RT: 16.240 min Scan# 1459
Delta R.T. 0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion	Ratio	Lower	Upper
284	100		
142	34.8	27.9	41.9
249	29.9	24.2	36.2

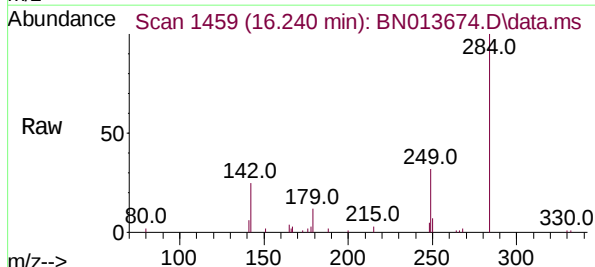


Abundance Scan 1459 (16.240 min): BN013674.D\data.ms (-1451) (-)

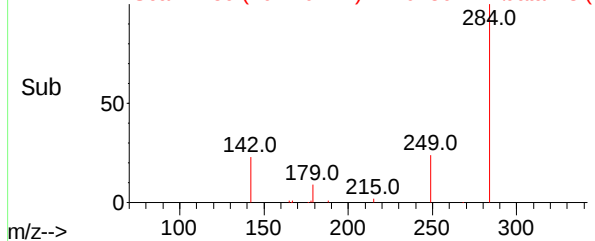



Abundance Scan 1473 (16.410 min): BN013594.D\data.ms (-1432) (-)

Atrazine
Concen: 0.37 ng
RT: 16.410 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

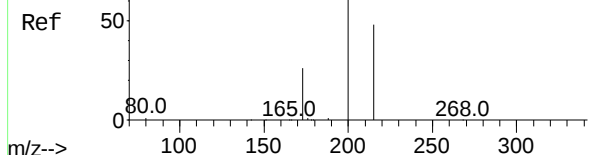

Tgt Ion	Ratio	Lower	Upper
200	100		
173	23.3	18.6	28.0
215	51.4	41.0	61.6

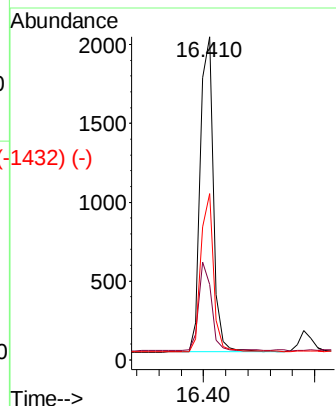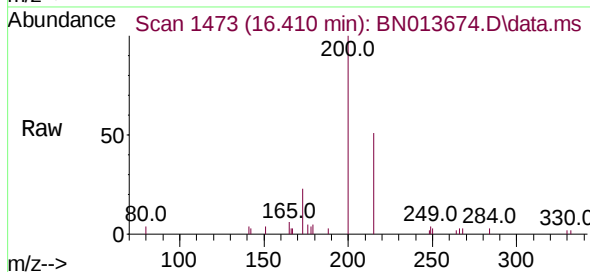




Abundance Scan 1473 (16.410 min): BN013674.D\data.ms (-1432) (-)

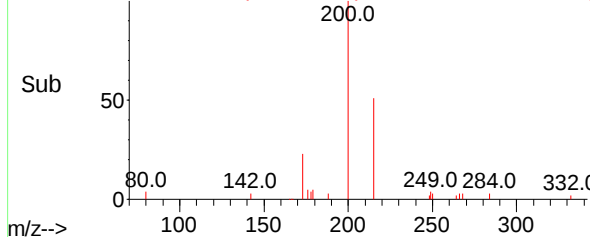


Abundance Scan 1488 (16.592 min): BN013594.D\data.ms (-1424) (-)

Pentachlorophenol
Concen: 0.48 ng
RT: 16.581 min Scan# 1487
Delta R.T. 0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion	Ratio	Lower	Upper
266	100		
264	61.6	51.6	77.4
268	60.7	54.6	82.0

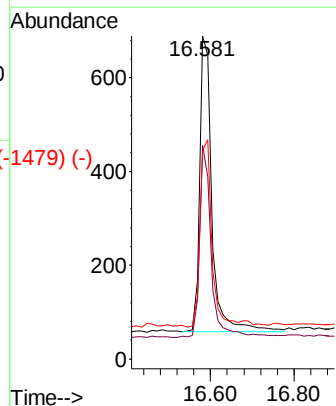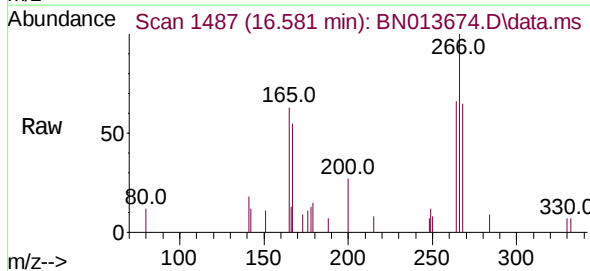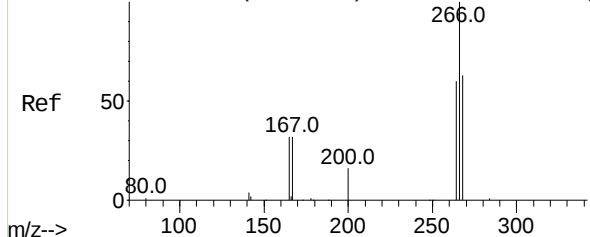


Abundance Scan 1487 (16.581 min): BN013674.D\data.ms (-1479) (-)

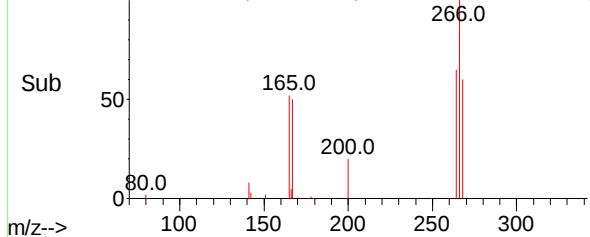



Abundance Scan 1519 (16.970 min): BN013594.D\data.ms (-1525) (-)

Phenanthrene
Concen: 0.39 ng
RT: 16.970 min Scan# 1519
Delta R.T. 0.001 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

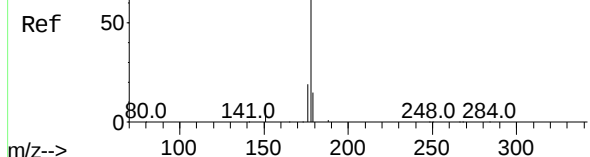

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.7	15.0	22.4
179	15.4	12.3	18.5

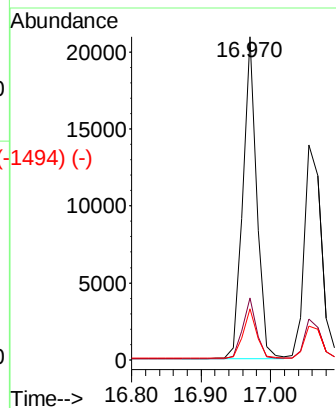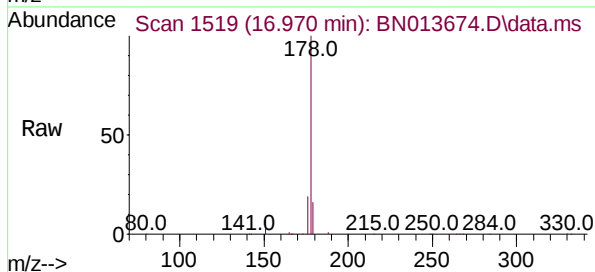




Abundance Scan 1519 (16.970 min): BN013674.D\data.ms (-1494) (-)

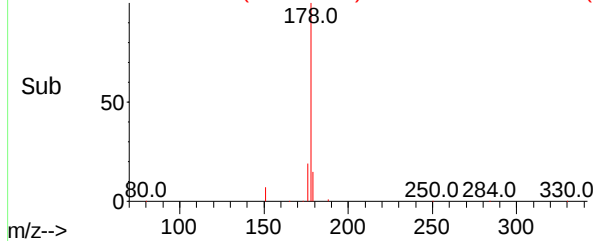


Abundance Scan 1527 (17.067 min): BN013594.D\data.ms (-1526) (-)

Anthracene
Concen: 0.38 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.0	14.6	21.8
179	15.4	12.2	18.2

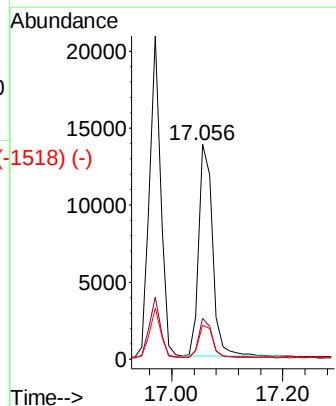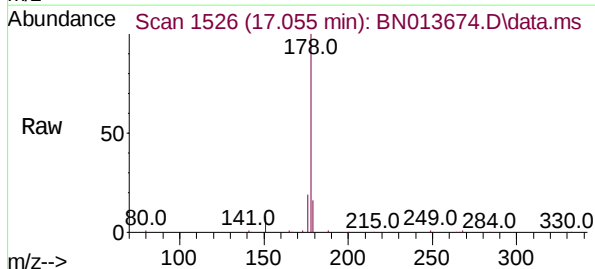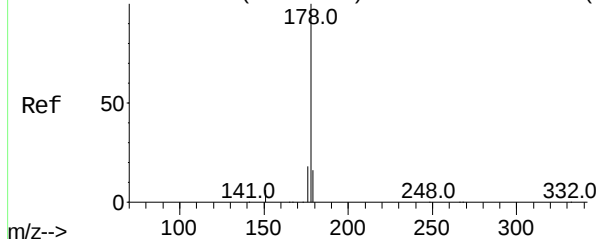


Abundance Scan 1526 (17.055 min): BN013674.D\data.ms (-1518) (-)

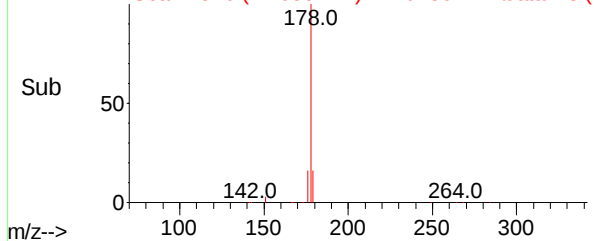



Abundance Scan 1799 (18.972 min): BN013594.D\data.ms (-1729) (-)

Fluoranthene-d10
Concen: 0.39 ng
RT: 18.970 min Scan# 1797
Delta R.T. -0.002 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

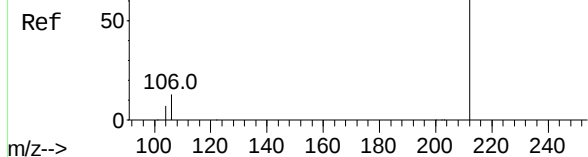

Tgt Ion:	212	Resp:	29321
Ion Ratio	Lower	Upper	
212	100		
106	12.9	9.7	14.5
104	7.3	5.5	8.3

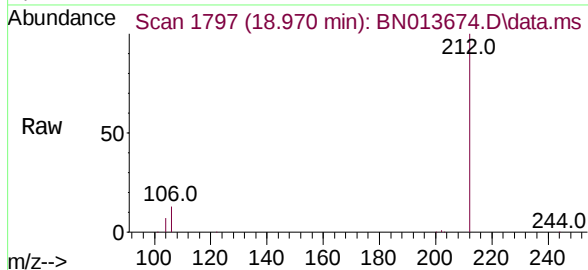


Abundance Scan 1797 (18.970 min): BN013674.D\data.ms (-1757) (-)





Abundance Scan 1806 (19.007 min): BN013594.D\data.ms (-1729) (-)


Fluoranthene
Concen: 0.38 ng
RT: 19.000 min Scan# 1803
Delta R.T. -0.002 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

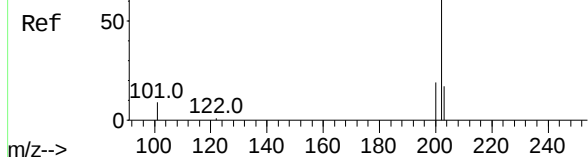

Tgt Ion:	202	Resp:	31882
Ion Ratio	Lower	Upper	
202	100		
101	11.1	8.1	12.1
203	17.3	13.9	20.9

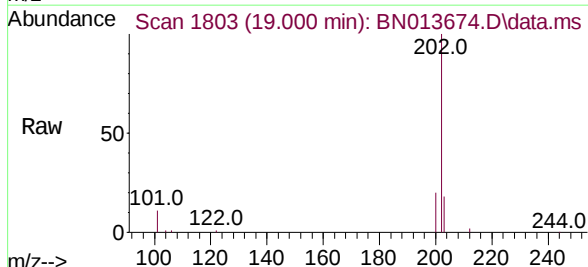


Abundance Scan 1803 (19.000 min): BN013674.D\data.ms (-1763) (-)

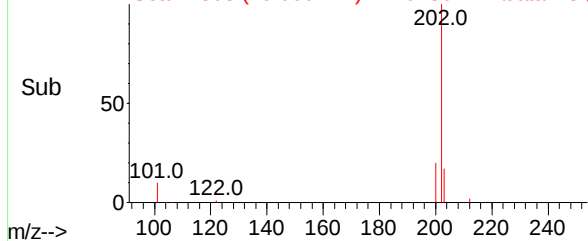




Abundance Scan 2114 (21.141 min): BN013594.D\data.ms (-2129) (-)

Chrysene-d12
Concen: 0.40 ng
RT: 21.133 min Scan# 2112
Delta R.T. 0.003 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

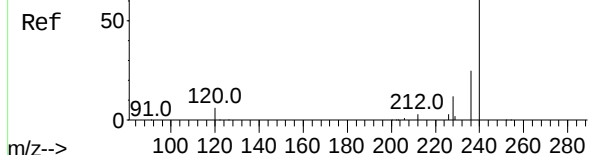





Tgt Ion:	240	Resp:	26918
Ion	Ratio	Lower	Upper
240	100		
120	9.7	10.2	15.4#
236	26.1	21.3	31.9

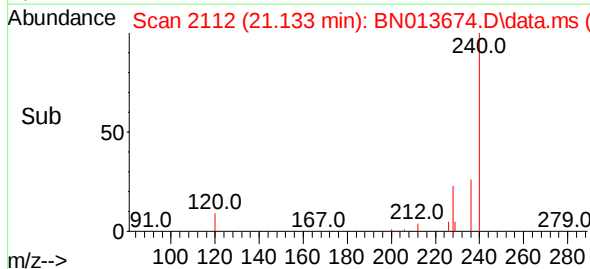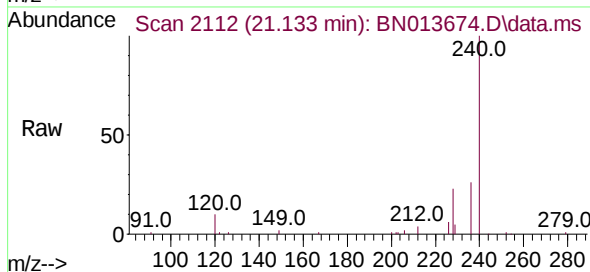


Abundance Scan 1879 (19.369 min): BN013594.D\data.ms (-1836) (-)

Pyrene
Concen: 0.40 ng
RT: 19.362 min Scan# 1876
Delta R.T. -0.002 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	202	Resp:	32443
Ion	Ratio	Lower	Upper
202	100		
200	20.4	16.3	24.5
203	17.3	14.0	21.0

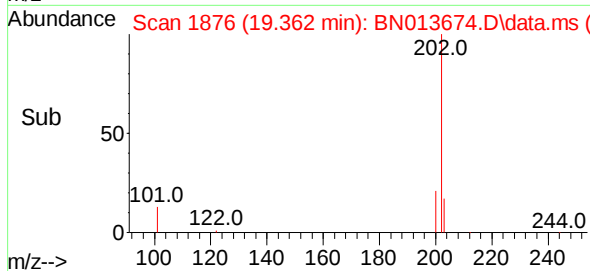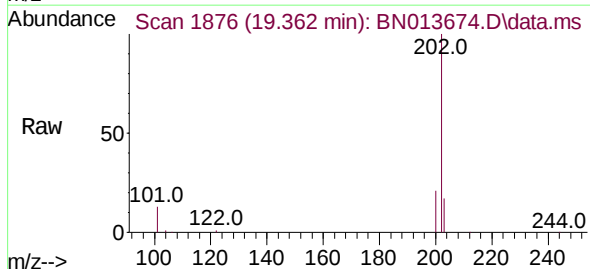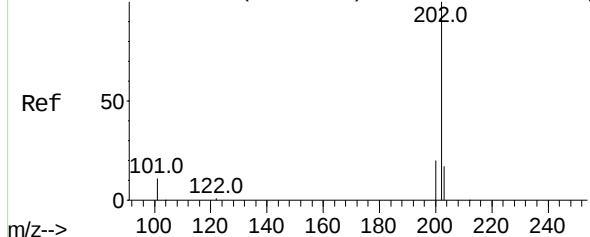



Abundance Scan 1923 (19.588 min): BN013594.D\data.ms (-1890) (-)




Terphenyl-d14
Concen: 0.40 ng
RT: 19.581 min Scan# 1920
Delta R.T. -0.002 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.4	6.1	9.1
122	12.7	9.8	14.8

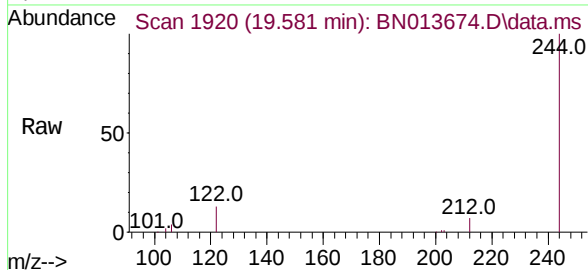

Abundance Scan 1920 (19.581 min): BN013674.D\data.ms (-1890) (-)





Abundance Scan 2112 (21.120 min): BN013594.D\data.ms (-2102) (-)




Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.123 min Scan# 2111
Delta R.T. 0.003 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.7	20.5	30.7
229	19.9	16.2	24.4

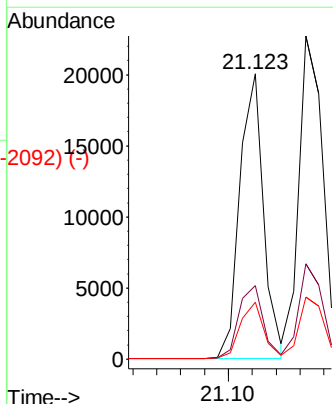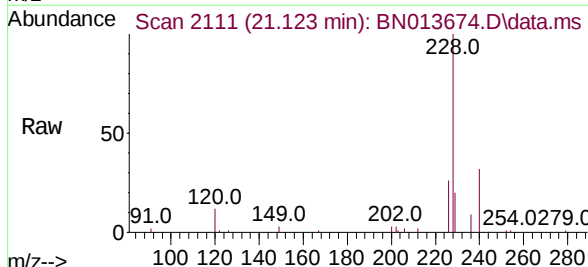

Abundance Scan 2111 (21.123 min): BN013674.D\data.ms (-2092) (-)






Abundance Scan 2117 (21.173 min): BN013594.D\data.ms (-2106) (-)

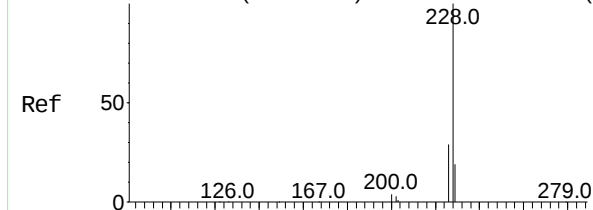


Chrysene
Concen: 0.39 ng
RT: 21.165 min Scan# 2115
Delta R.T. -0.008 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	228	Resp:	32039
Ion	Ratio	Lower	Upper
228	100		
226	29.5	24.3	36.5
229	19.2	15.1	22.7

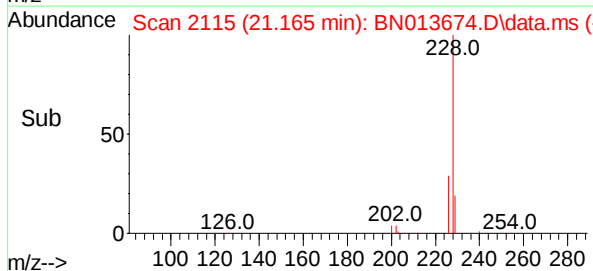

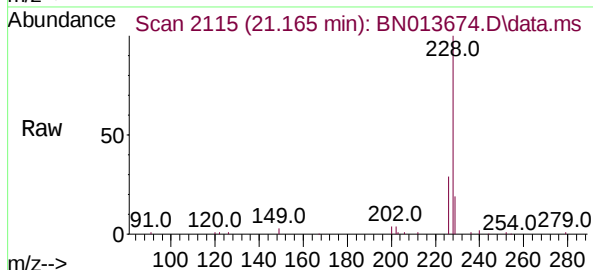


Abundance Scan 2108 (21.077 min): BN013594.D\data.ms (-2106) (-)

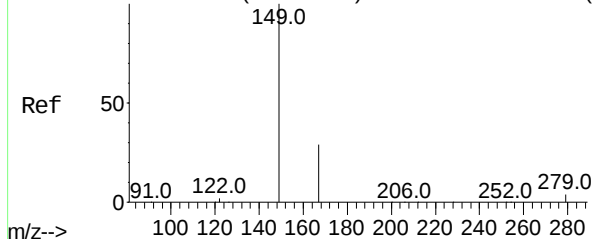


Bis(2-ethylhexyl)phthalate
Concen: 0.41 ng
RT: 21.070 min Scan# 2106
Delta R.T. 0.003 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	149	Resp:	8655
Ion	Ratio	Lower	Upper
149	100		
167	27.1	22.1	33.1
279	4.2	3.5	5.3

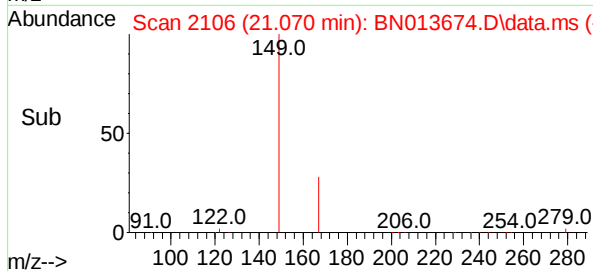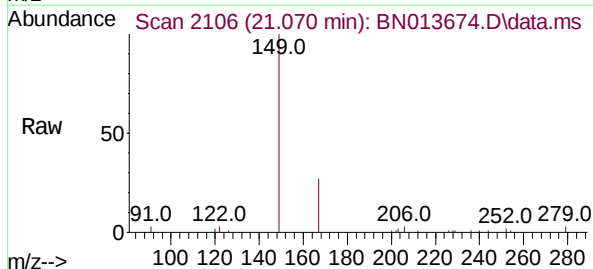



Abundance Scan 3124 (25.454 min): BN013594.D\data.ms (-3095) (-)




Indeno(1,2,3-cd)pyrene
Concen: 0.42 ng
RT: 25.444 min Scan# 3119
Delta R.T. -0.001 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.2	19.8	29.6
277	25.1	19.9	29.9

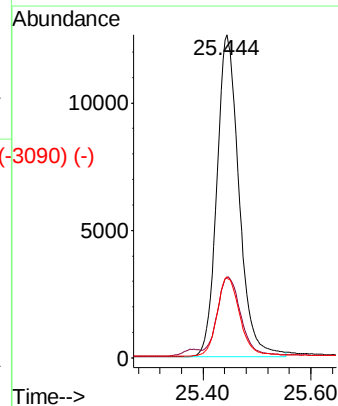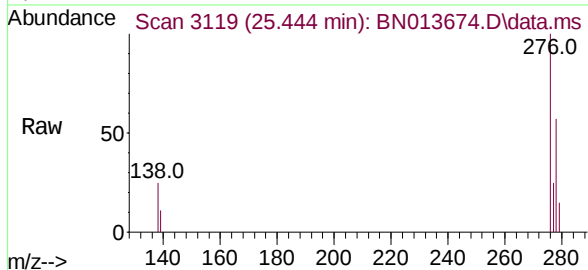

Abundance Scan 3119 (25.444 min): BN013674.D\data.ms (-3090) (-)


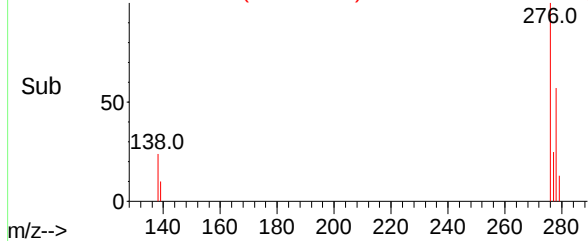


Abundance Scan 2496 (23.305 min): BN013594.D\data.ms (-2486) (-)




Perylene-d12
Concen: 0.40 ng
RT: 23.301 min Scan# 2493
Delta R.T. -0.001 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.3	28.9
265	32.6	66.2	99.4#

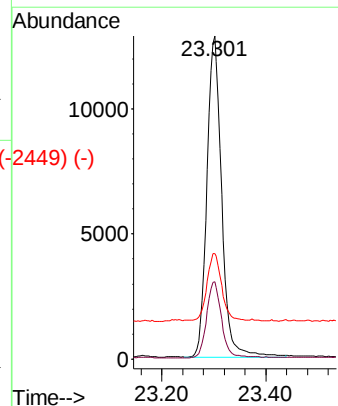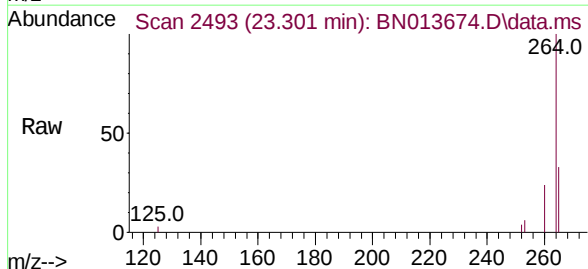

Abundance Scan 2493 (23.301 min): BN013674.D\data.ms (-2449) (-)


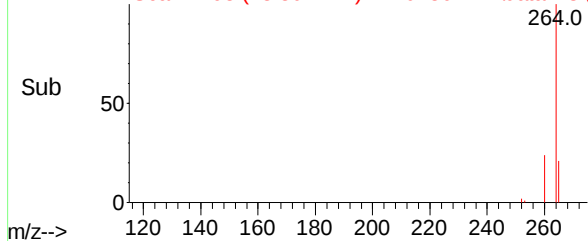


Abundance Scan 2308 (22.661 min): BN013594.D\data.ms (-2307) (-)

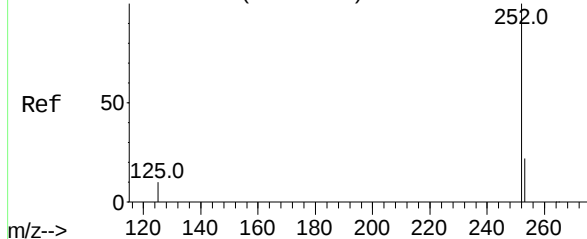


Benzo(b)fluoranthene
Concen: 0.36 ng
RT: 22.654 min Scan# 2304
Delta R.T. -0.004 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion:	252	Resp:	31719
Ion	Ratio	Lower	Upper
252	100		
253	25.0	20.4	30.6
125	11.8	11.6	17.4

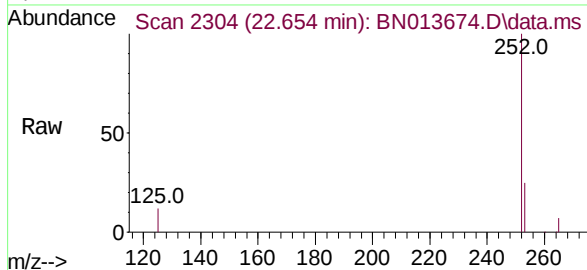

Abundance Scan 2304 (22.654 min): BN013674.D\data.ms (-2247) (-)


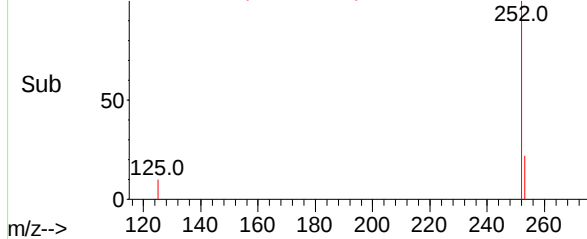


Abundance Scan 2320 (22.702 min): BN013594.D\data.ms (-2319) (-)

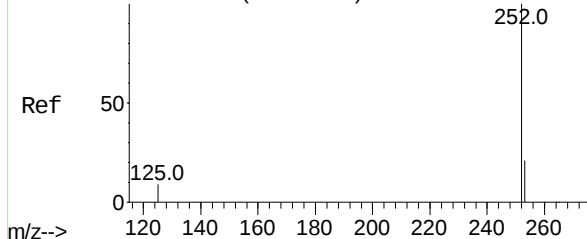


Benzo(k)fluoranthene
Concen: 0.39 ng
RT: 22.695 min Scan# 2316
Delta R.T. -0.004 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Tgt Ion:	252	Resp:	34317
Ion	Ratio	Lower	Upper
252	100		
253	24.5	20.5	30.7
125	12.5	12.3	18.5

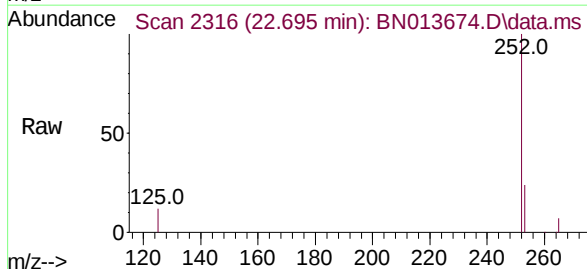


Abundance Scan 2316 (22.695 min): BN013674.D\data.ms (-2231) (-)

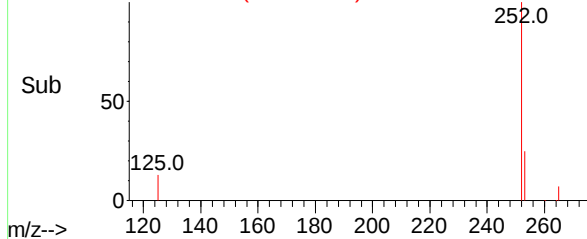

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Abundance Scan 2468 (23.209 min): BN013594.D\data.ms (-2439) (-)




Benzo(a)pyrene
Concen: 0.40 ng
RT: 23.205 min Scan# 2465
Delta R.T. -0.001 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 29374
Ion Ratio Lower Upper
252 100
253 26.7 21.8 32.6
125 17.8 14.6 21.8

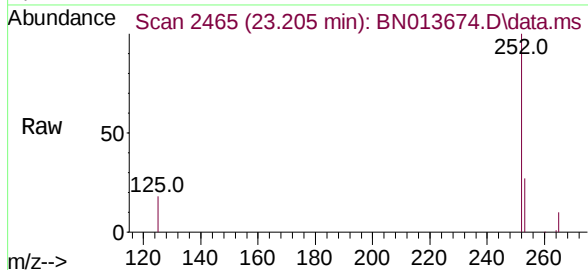

Abundance Scan 2465 (23.205 min): BN013674.D\data.ms (-2407) (-)





Abundance Scan 3128 (25.468 min): BN013594.D\data.ms (-3100) (-)




Dibenzo(a,h)anthracene
Concen: 0.37 ng
RT: 25.461 min Scan# 3124
Delta R.T. 0.003 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28


Tgt Ion:278 Resp: 29837
Ion Ratio Lower Upper
278 100
139 17.6 13.1 19.7
279 25.5 21.4 32.0

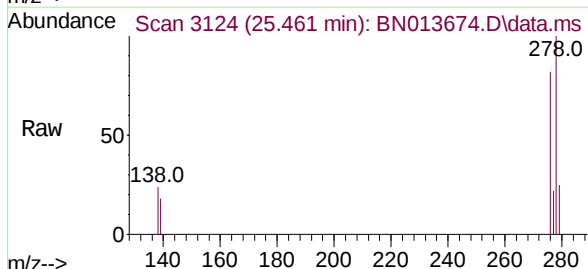

Abundance Scan 3124 (25.461 min): BN013674.D\data.ms (-3100) (-)

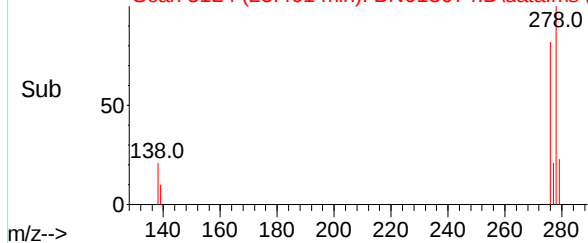


Abundance Scan 3314 (26.105 min): BN013594.D\data.ms (-3250) (-)

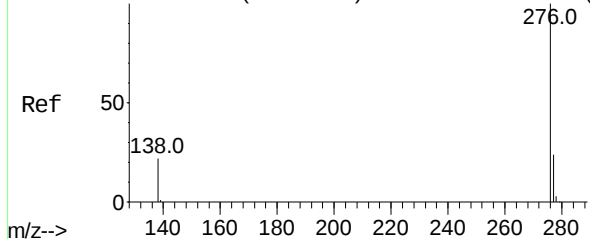

Benzo(g,h,i)perylene
Concen: 0.37 ng
RT: 26.098 min Scan# 3310
Delta R.T. -0.001 min
Lab File: BN013674.D
Acq: 18 Feb 2021 16:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Abundance Scan 3310 (26.098 min): BN013674.D\data.ms

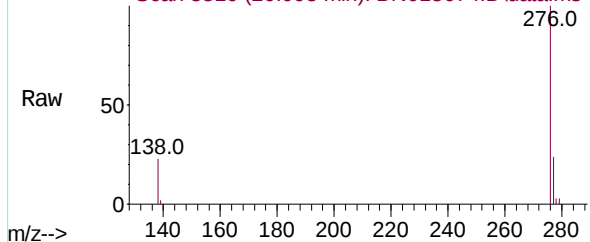

Tgt Ion:	276	Resp:	30980
Ion	Ratio	Lower	Upper
276	100		
277	24.2	20.0	30.0
138	22.7	17.8	26.8

Abundance Scan 3310 (26.098 min): BN013674.D\data.ms (-3252) (-)

