
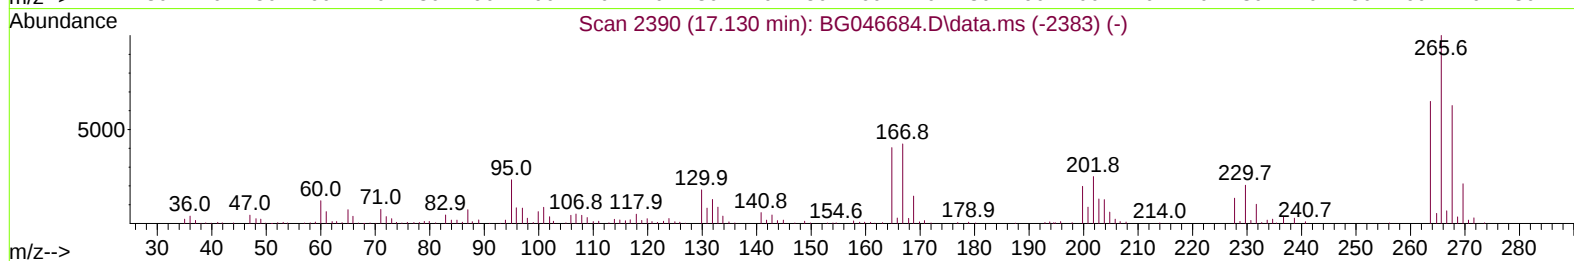
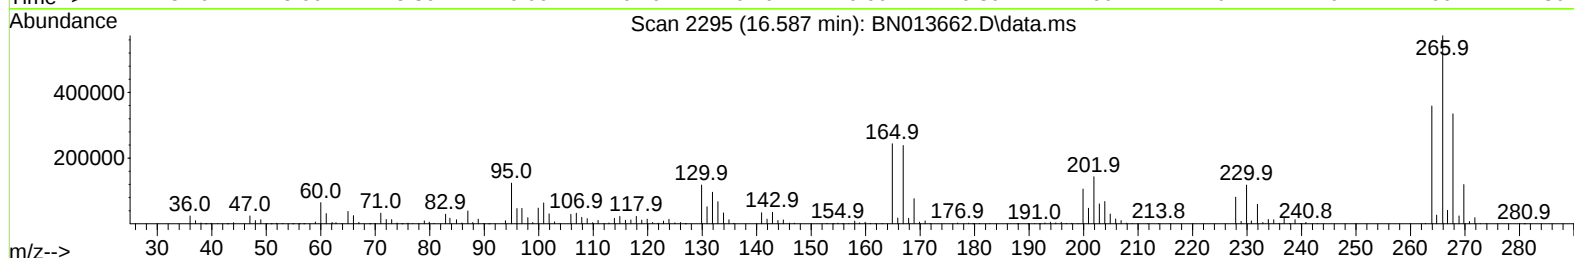


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
Data File : BN013662.D
Acq On : 18 Feb 2021 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 01:57:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

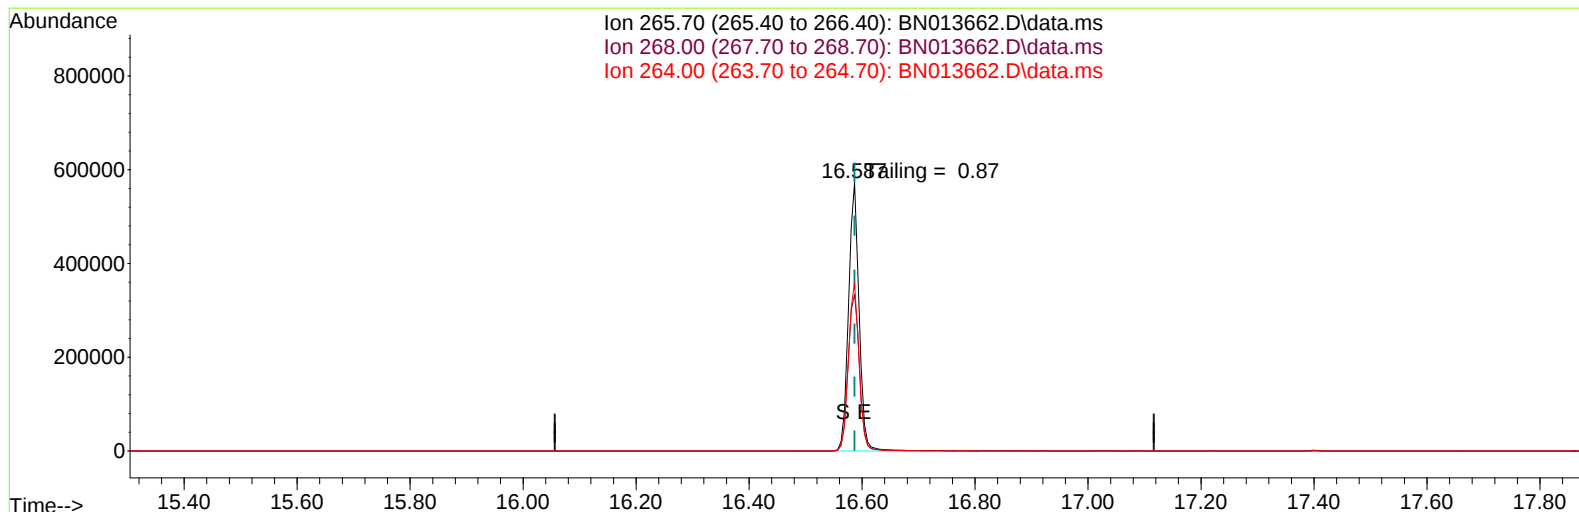

TIC: BN013662.D\data.ms

(70) Pentachlorophenol (C)




16.587min (+ 0.000) 23146.36 ng

response 744207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.50
264.00	61.60	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
 Data File : BN013662.D
 Acq On : 18 Feb 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 01:57:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 05:39:20 2021
 Response via : Initial Calibration

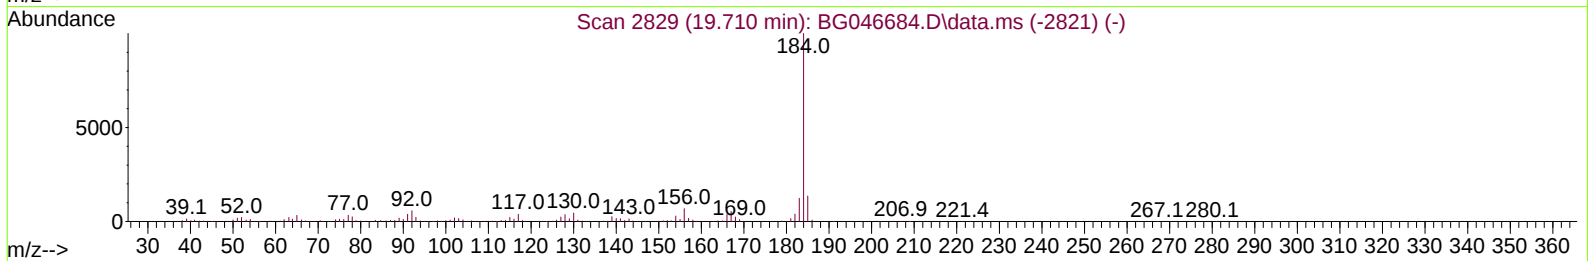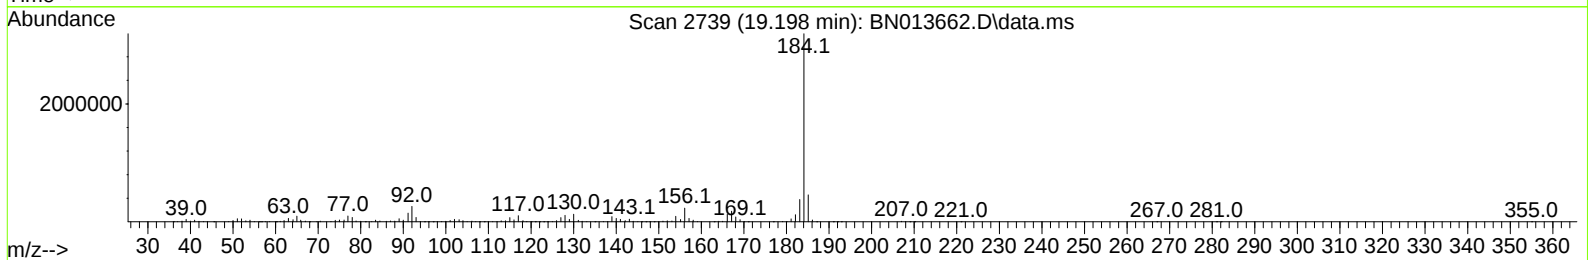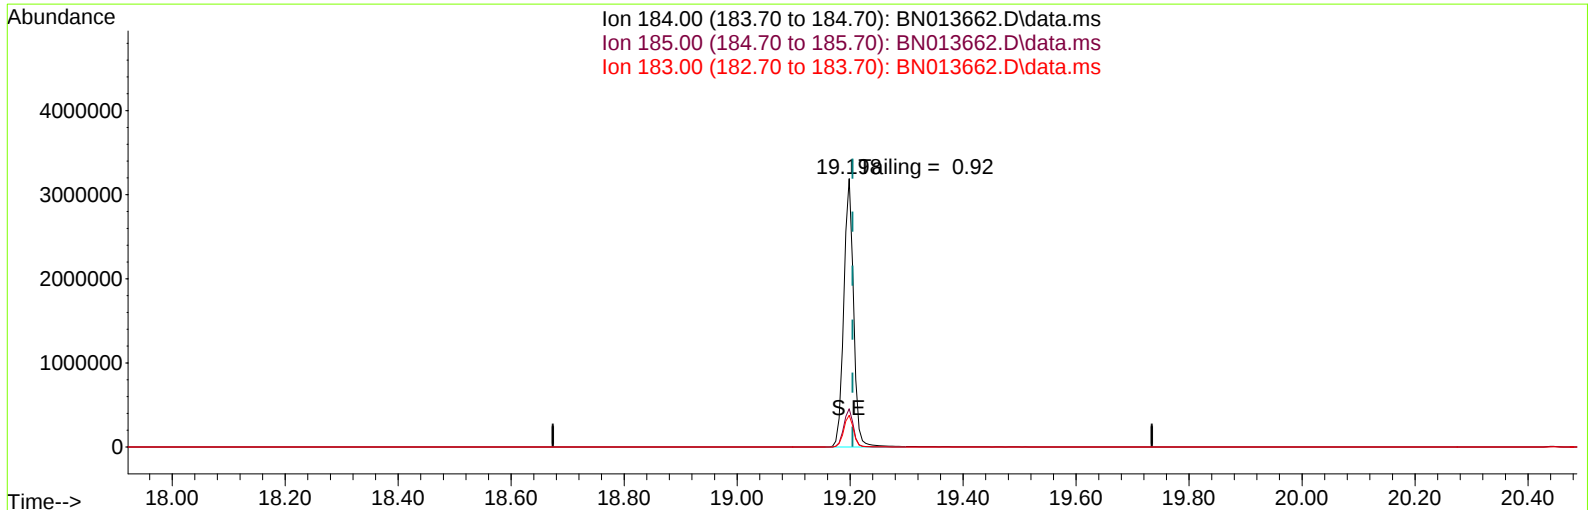

TIC: BN013662.D\data.ms

(77) Benzidine**19.198min (-0.006) 0.00 ng****response 3823392**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.82
0.00	0.00	0.00