
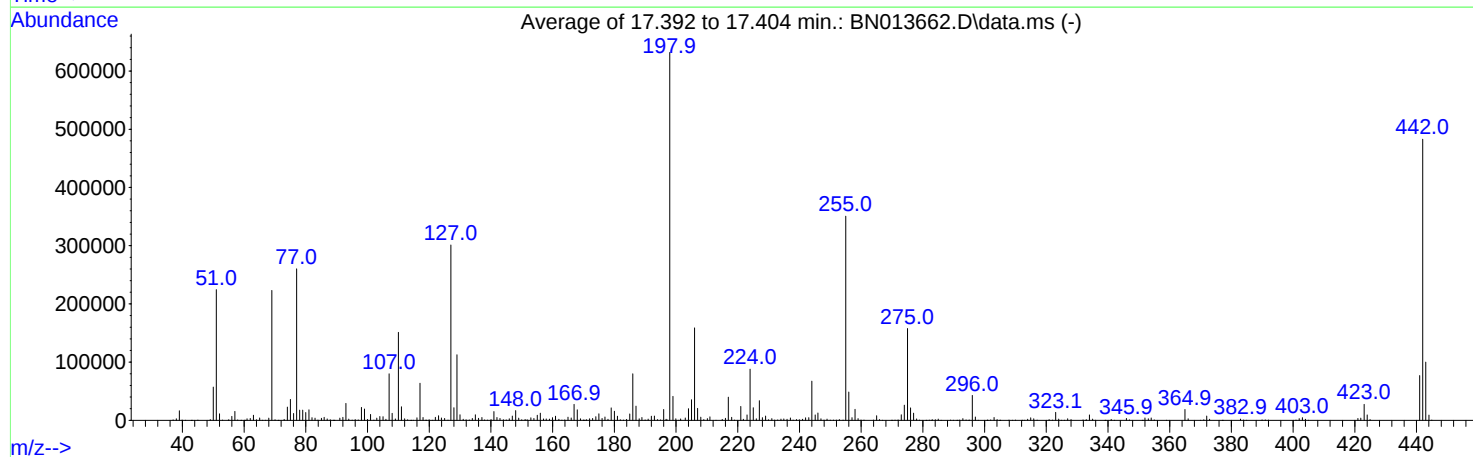


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
 Data File : BN013662.D
 Acq On : 18 Feb 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 18 10:50:10 2021

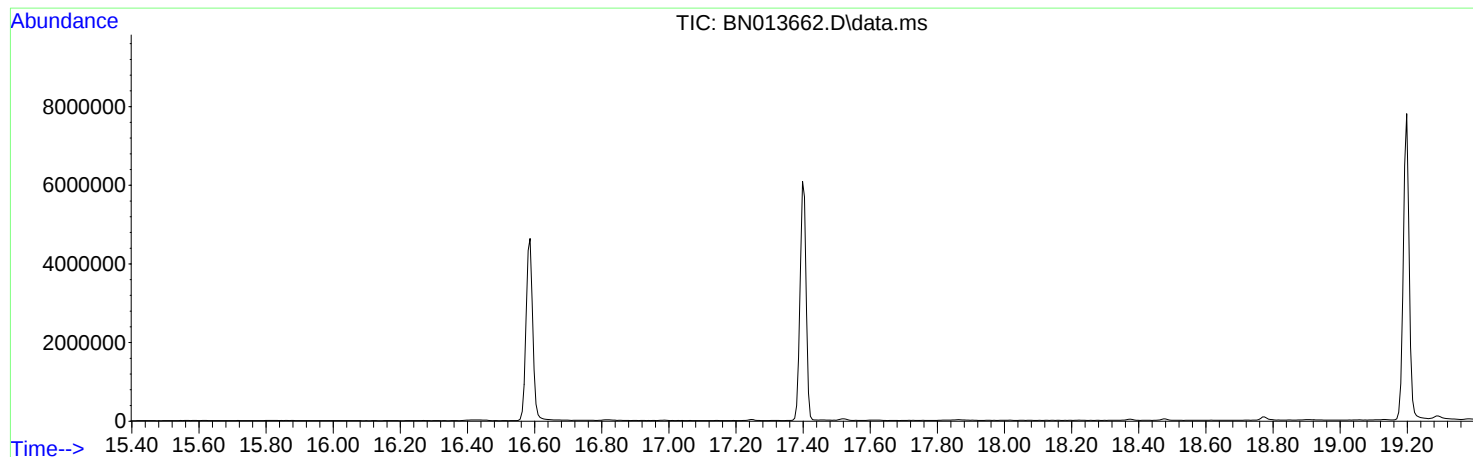

AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	224524	PASS
68	69	0.00	2	1.7	3800	PASS
69	198	0.00	100	35.3	223104	PASS
70	69	0.00	2	0.5	1039	PASS
127	198	10	80	47.7	301312	PASS
197	198	0.00	2	0.3	1981	PASS
198	198	100	100	100.0	631787	PASS
199	198	5	9	6.5	41144	PASS
275	198	10	60	25.0	157816	PASS
365	198	1	100	3.0	18681	PASS
441	198	0.01	100	12.2	76981	PASS
442	442	50	100	100.0	482795	PASS
443	442	15	24	20.7	99915	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/18/2021	BNA_N	<u>BN013662.D</u>
Compound Name	Response	Retention Time
DDT	2196326	20.445
DDD	27460	19.998
DDE	4272	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31732	2228058	1.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
 Data File : BN013662.D
 Acq On : 18 Feb 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 20 01:57:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 05:39:20 2021
 Response via : Initial Calibration

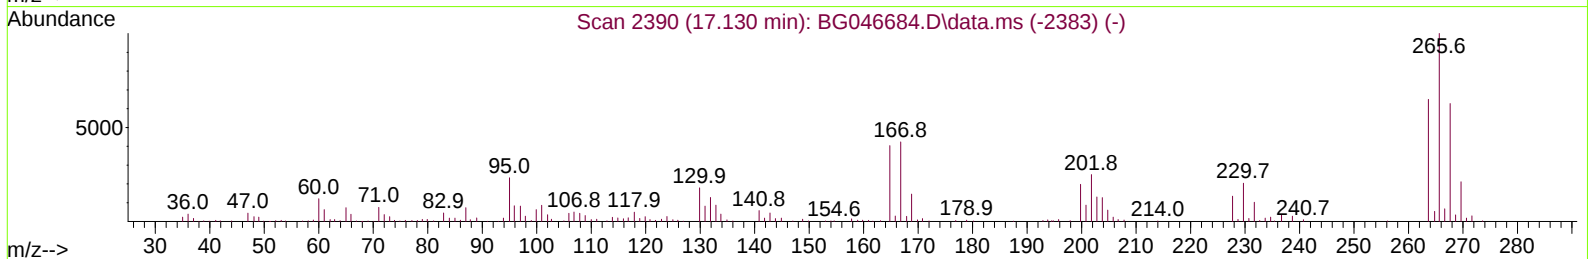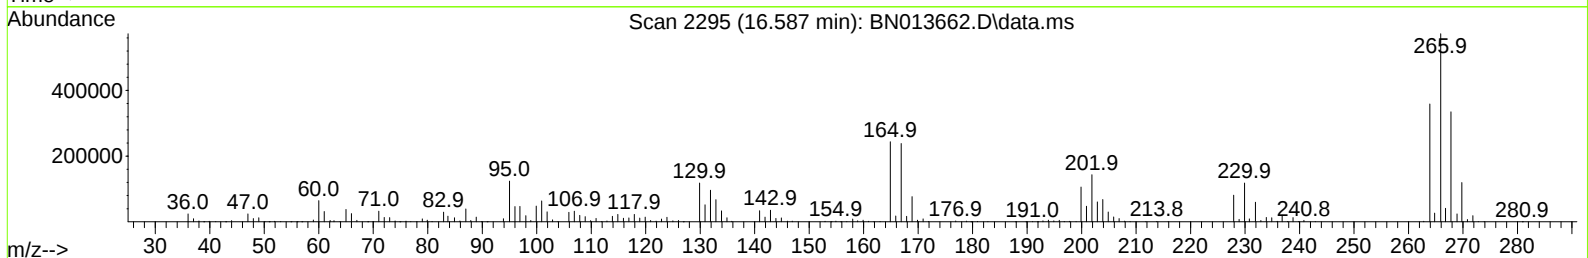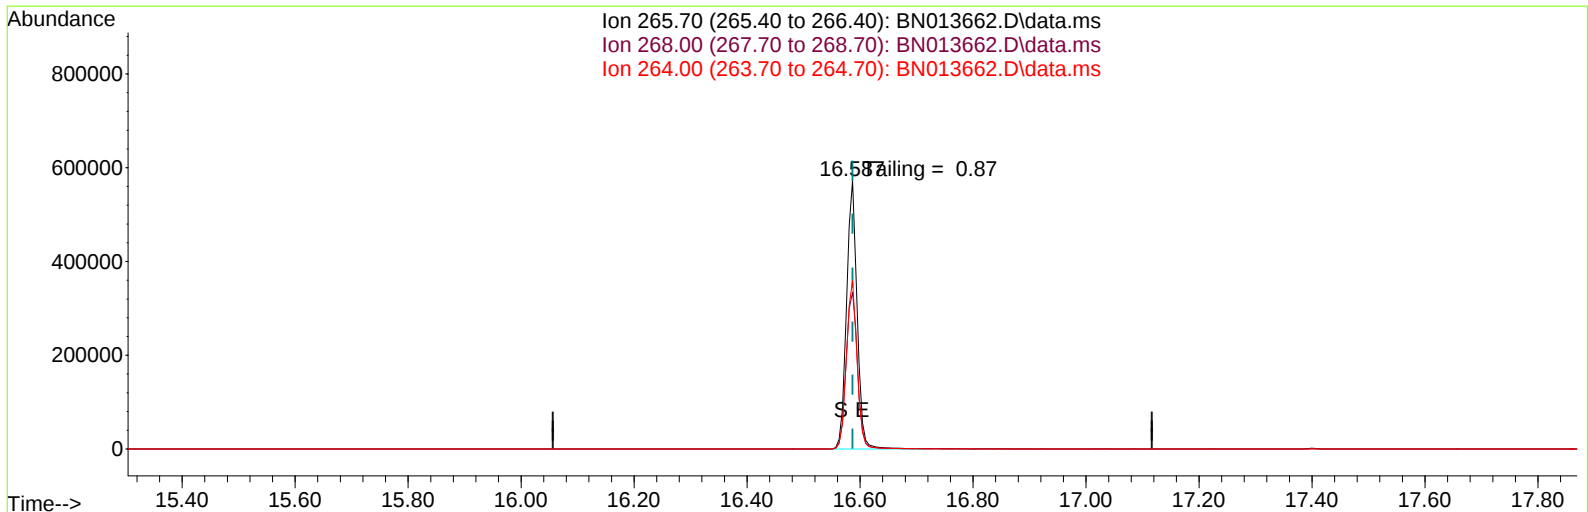

TIC: BN013662.D\data.ms

(70) Pentachlorophenol (C)

16.587min (+ 0.000) 23146.36 ng




response 744207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.50
264.00	61.60	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021821\
Data File : BN013662.D
Acq On : 18 Feb 2021 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 20 01:57:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

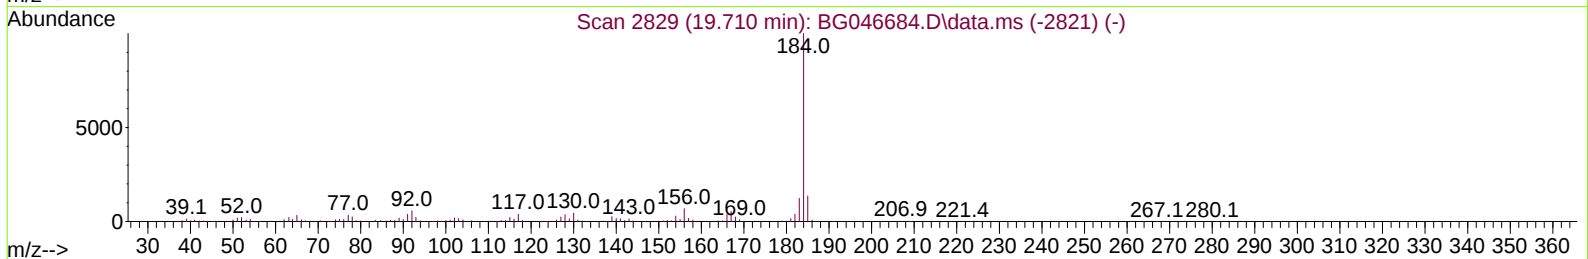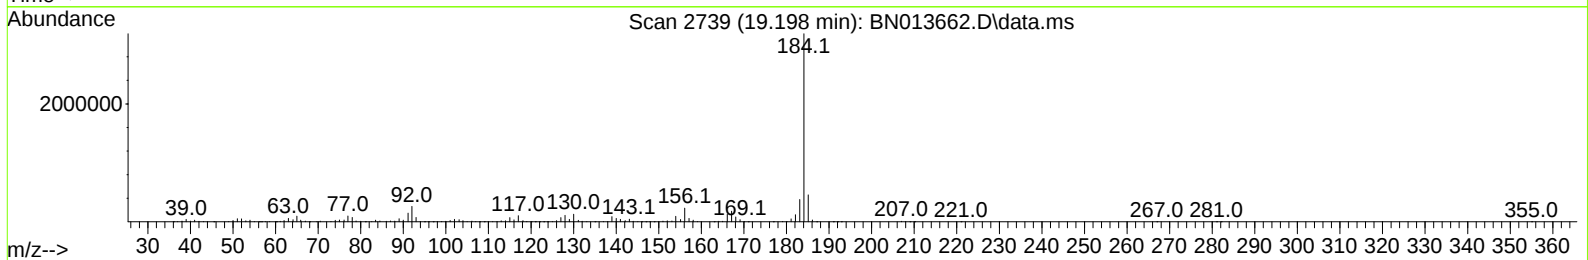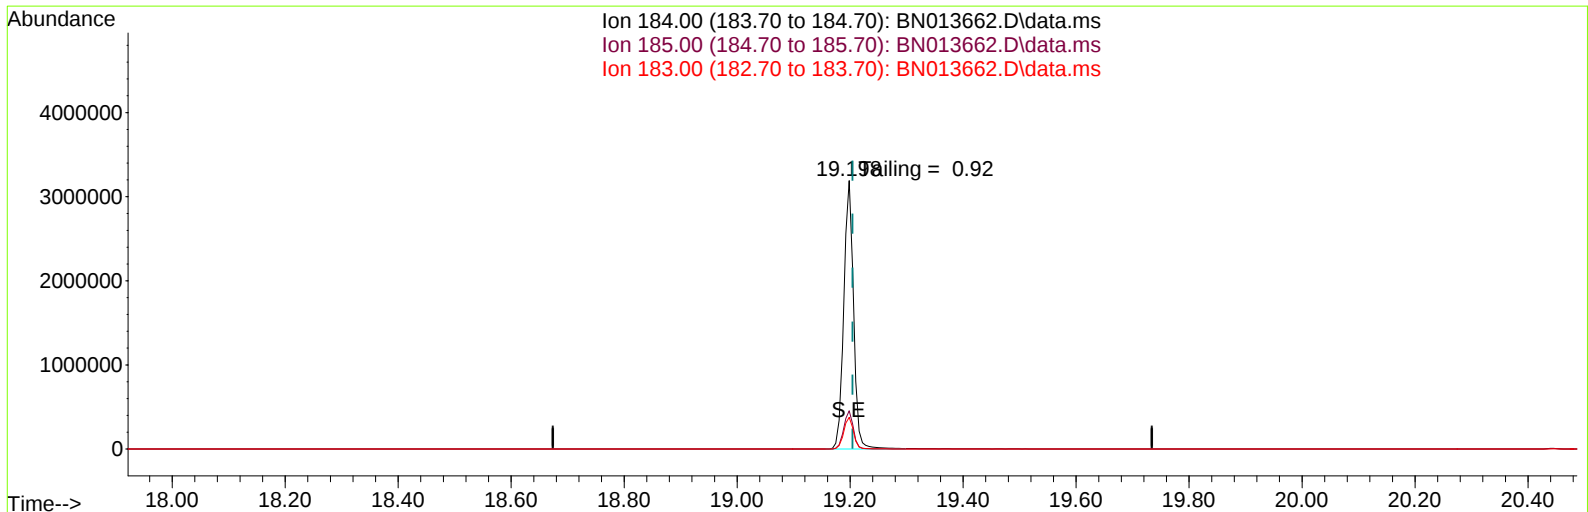

TIC: BN013662.D\data.ms

(77) Benzidine

19.198min (-0.006) 0.00 ng

response 3823392

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.82
0.00	0.00	0.00