
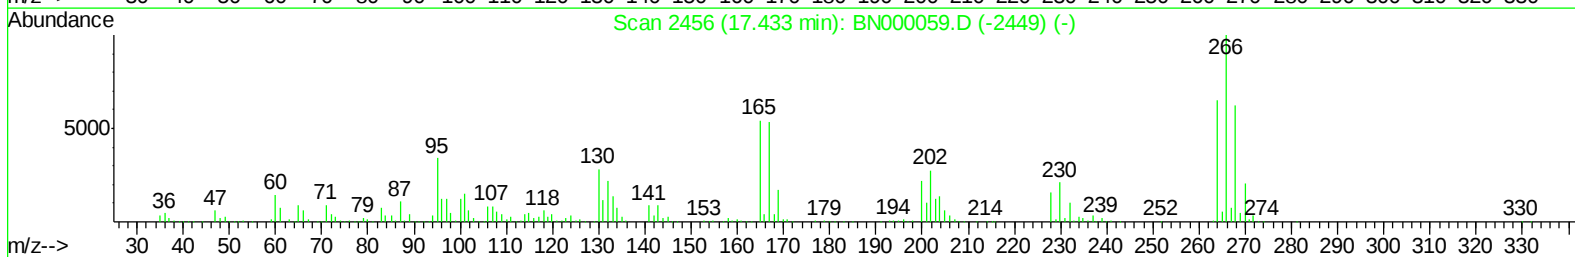
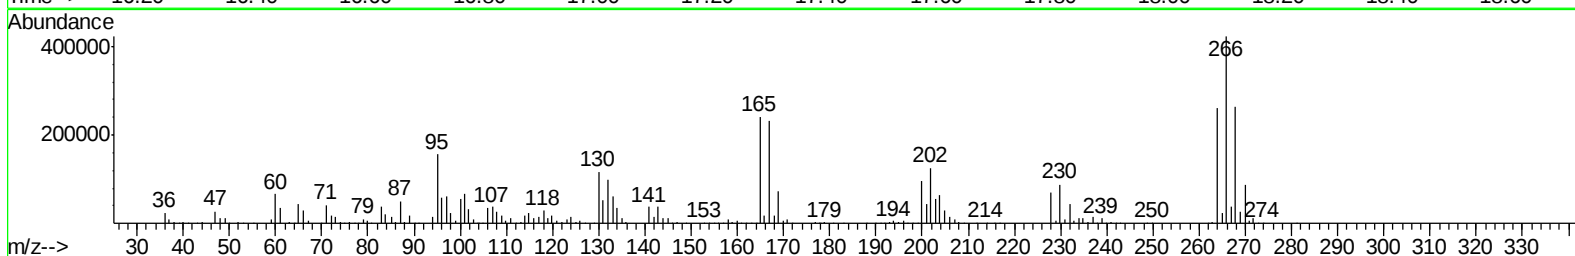


Data Path : Z:\HPCHEM1\BNA N\DATA\BN021918\
Data File : BN000111.D
Acq On : 19 Feb 2018 15:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 04:30:18 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

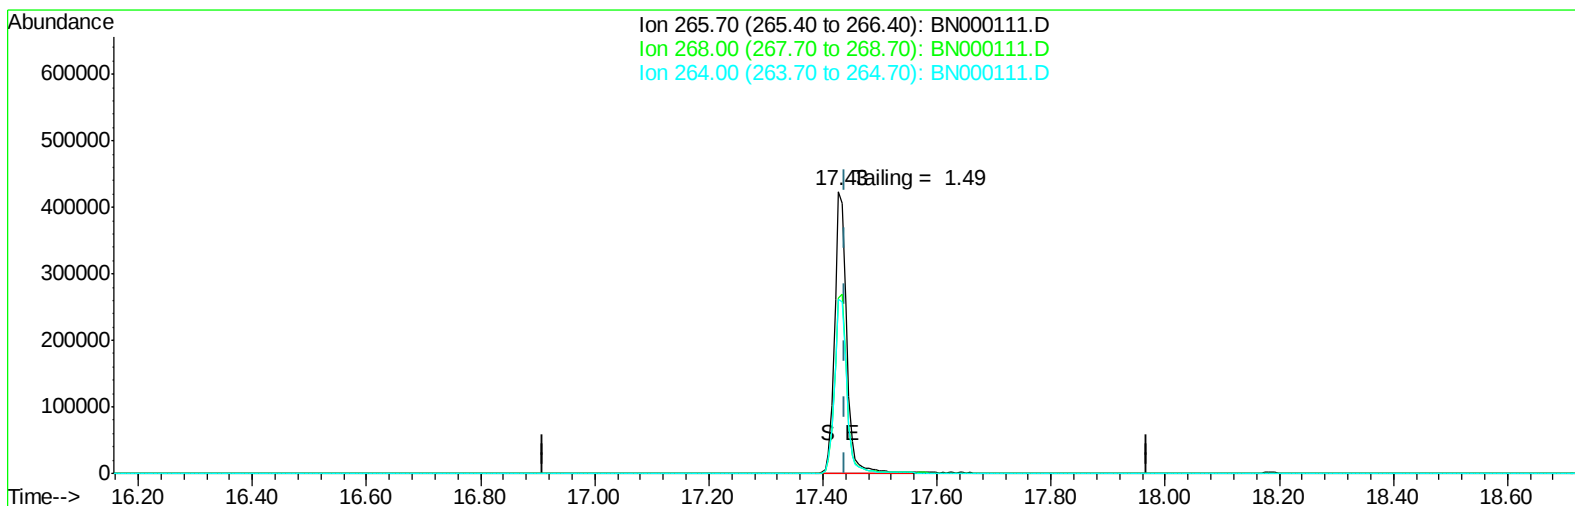

TIC: BN000111.D

(69) Pentachlorophenol (C)




17.428min (-0.011) 115602.85ng

response 615906

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.17
264.00	62.00	61.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021918\
Data File : BN000111.D
Acq On : 19 Feb 2018 15:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 04:30:18 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

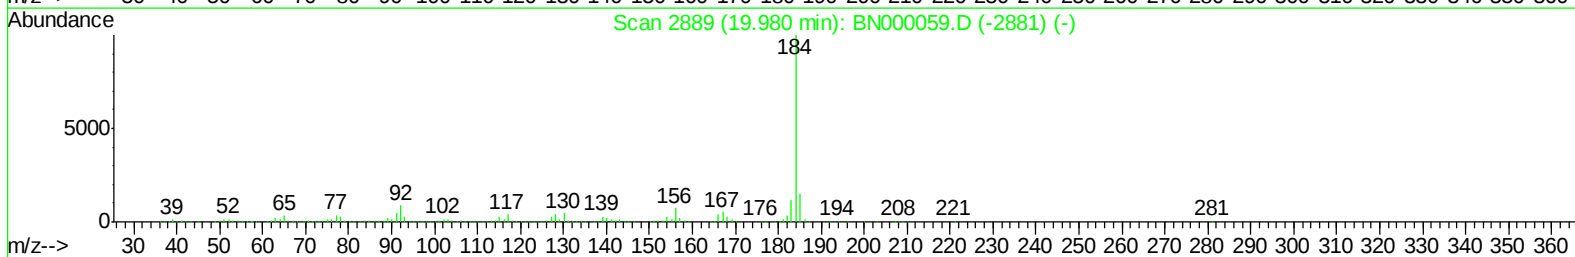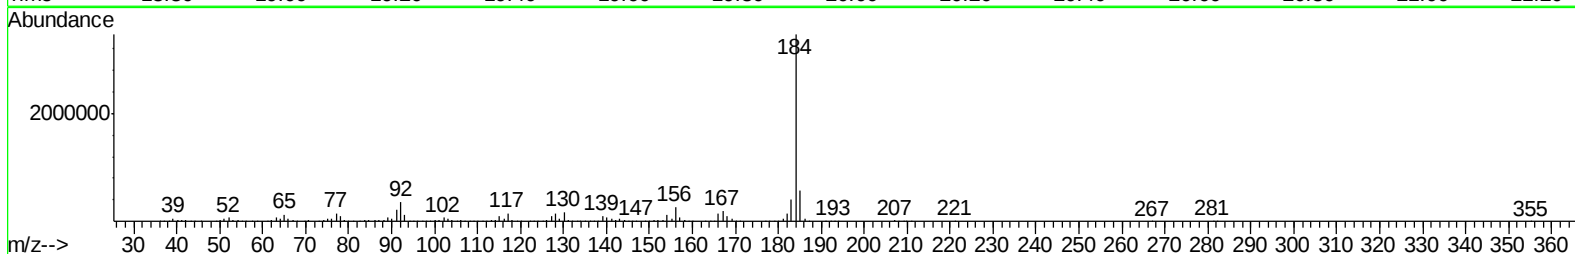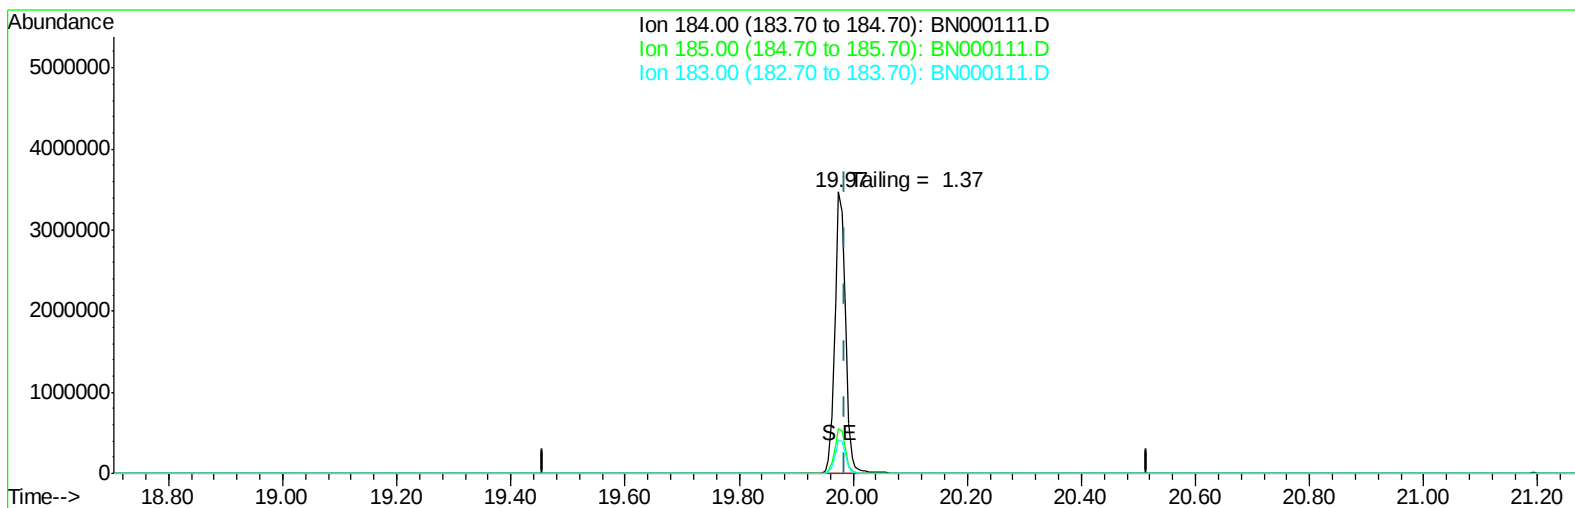

TIC: BN000111.D

(76) Benzidine

19.975min (-0.012) 67601.62ng

response 4432734

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.13
183.00	13.30	11.89
0.00	0.00	0.00