


Data Path : Z:\HPCHEM1\BNA N\Data\BN021918\
 Data File : BN000111.D
 Acq On : 19 Feb 2018 15:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

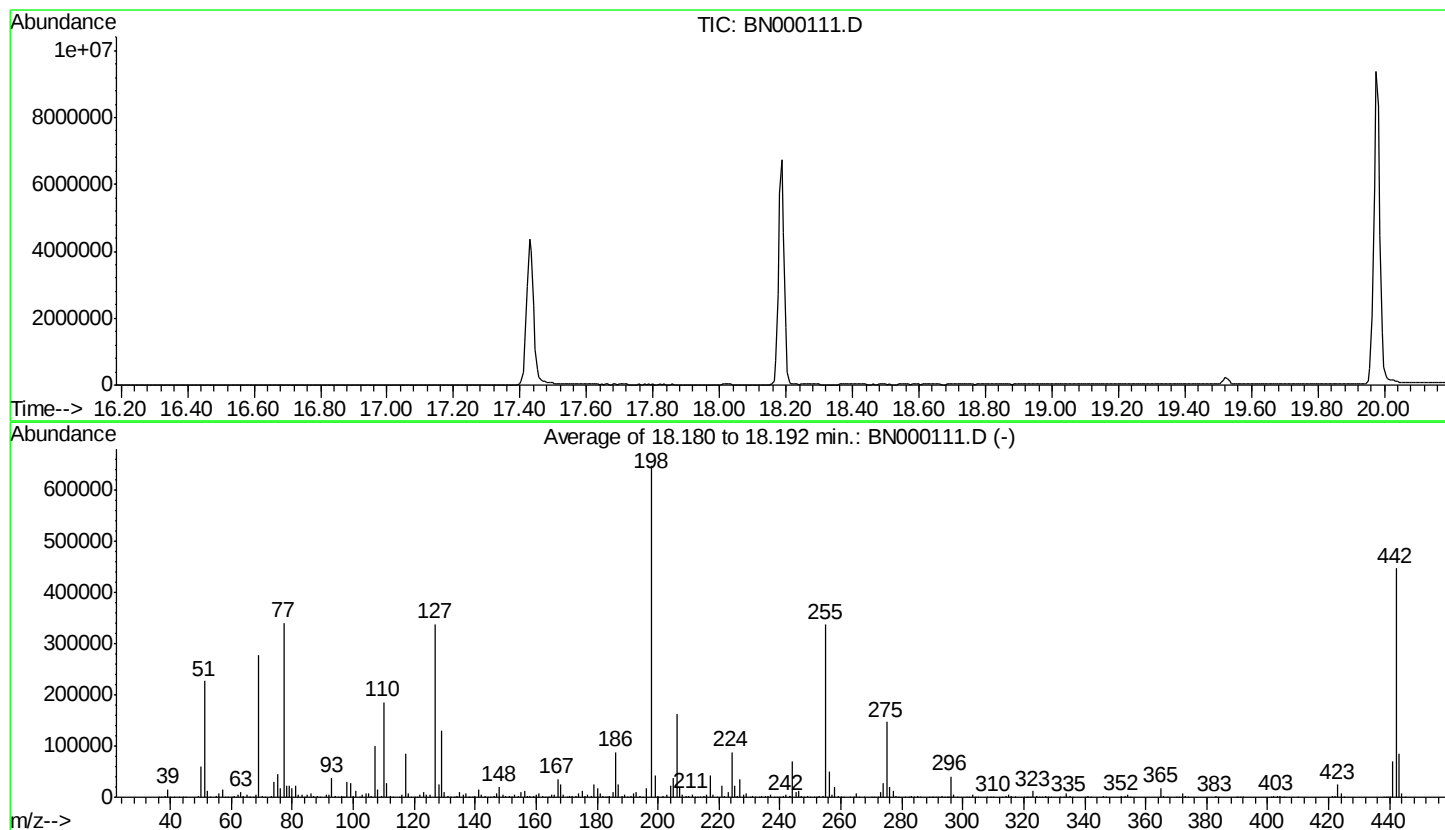

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	226922	PASS
68	69	0.00	2	1.7	4710	PASS
69	198	0.00	100	42.9	277533	PASS
70	69	0.00	2	0.6	1754	PASS
127	198	10	80	52.3	338282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	646997	PASS
199	198	5	9	6.7	43557	PASS
275	198	10	60	22.7	146850	PASS
365	198	1	100	2.7	17751	PASS
441	442	0.01	24	15.6	69720	PASS
442	198	50	100	69.1	446826	PASS
443	442	15	24	19.3	86133	PASS