
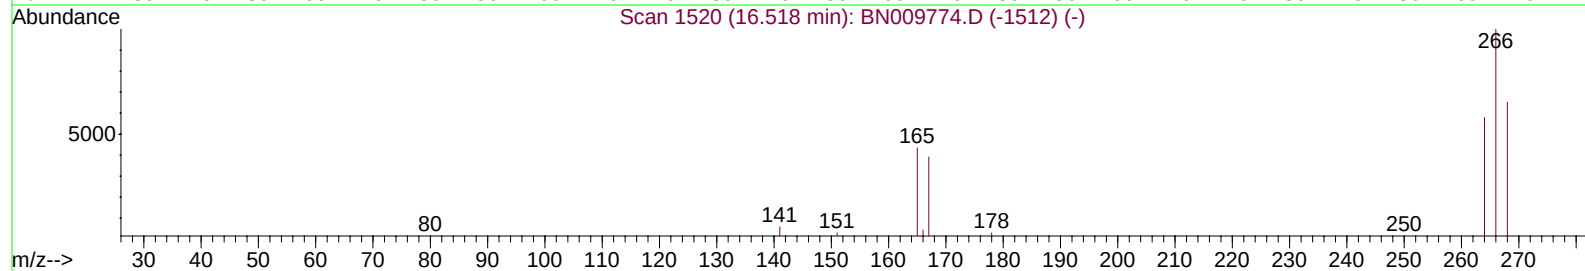
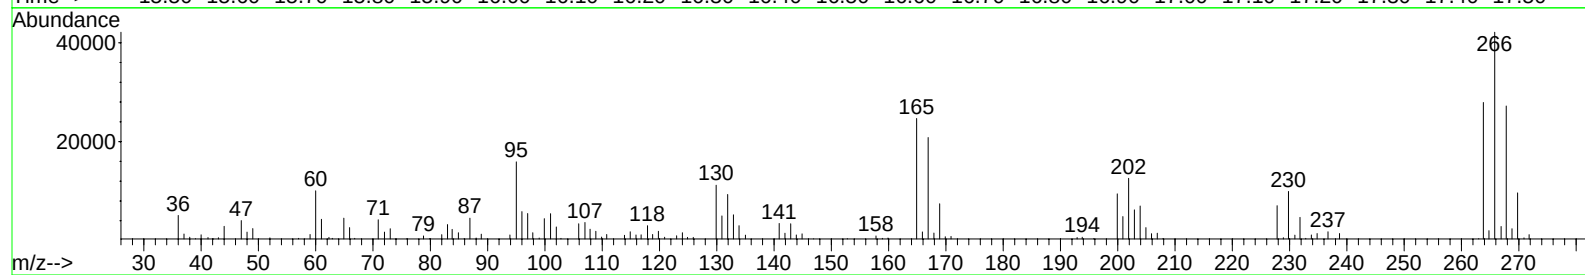


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN021920\
Data File : BN009771.D
Acq On : 19 Feb 2020 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 18:18:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN021920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 19 15:57:43 2020
Response via : Initial Calibration

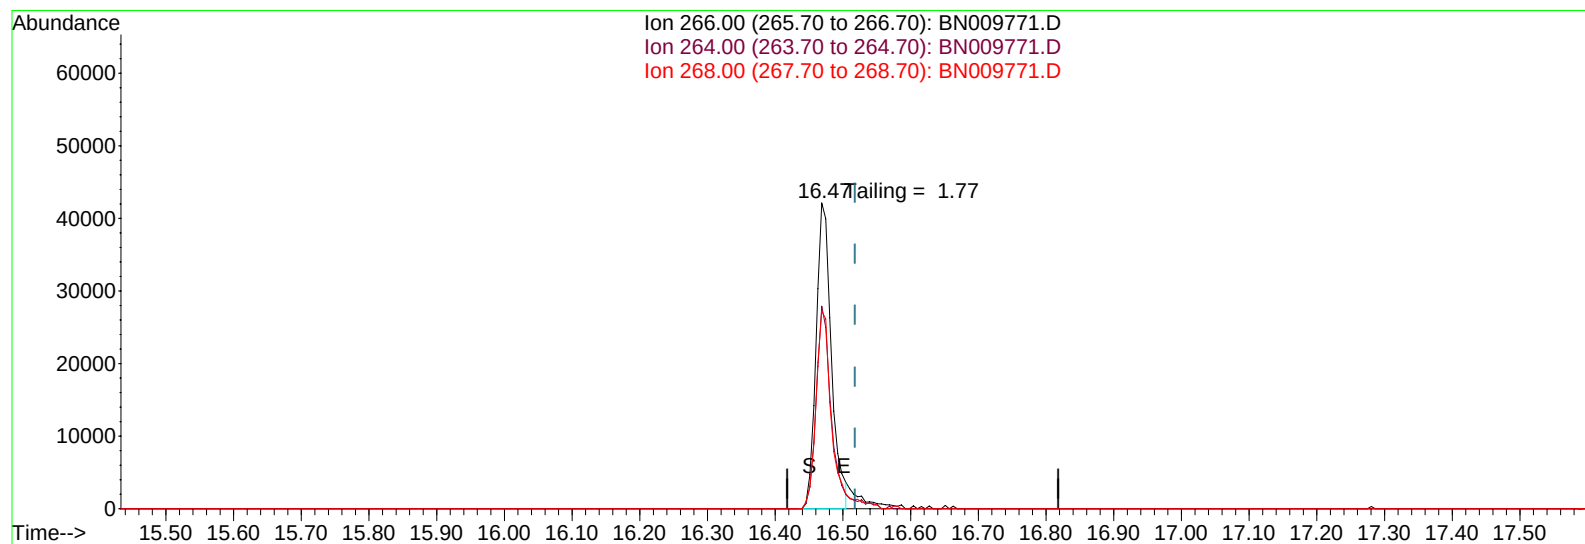

TIC: BN009771.D

(22) Pentachlorophenol

16.469min (-0.049) 0.00ng

response 71472

Ion	Exp%	Act%
266.00	100	100
264.00	72.60	66.25
268.00	82.10	64.62#
0.00	0.00	0.00