


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021920\
 Data File : BN009771.D
 Acq On : 19 Feb 2020 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 19 15:57:43 2020

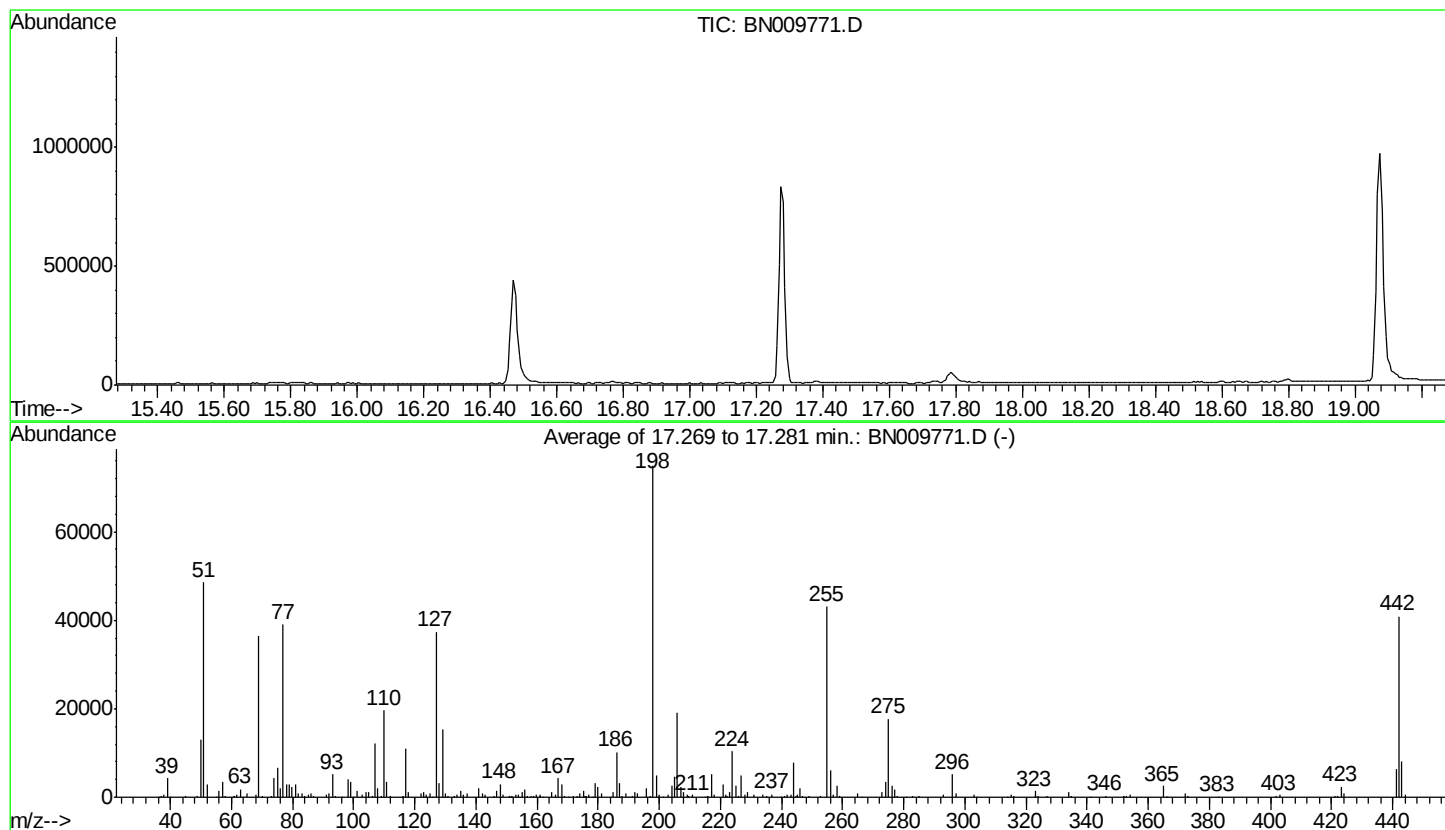

AutoFind: Scans 2428, 2429, 2430; Background Corrected with Scan 2422

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.8	48536	PASS
68	69	0.00	2	1.9	688	PASS
69	198	0.00	100	48.7	36474	PASS
70	69	0.00	2	0.7	263	PASS
127	198	10	80	49.8	37352	PASS
197	198	0.00	2	0.5	399	PASS
198	198	100	100	100.0	74944	PASS
199	198	5	9	6.7	4998	PASS
275	198	10	60	23.6	17654	PASS
365	198	1	100	3.4	2558	PASS
441	198	0.01	100	8.5	6352	PASS
442	198	50	100	54.5	40810	PASS
443	442	15	24	19.7	8029	PASS