
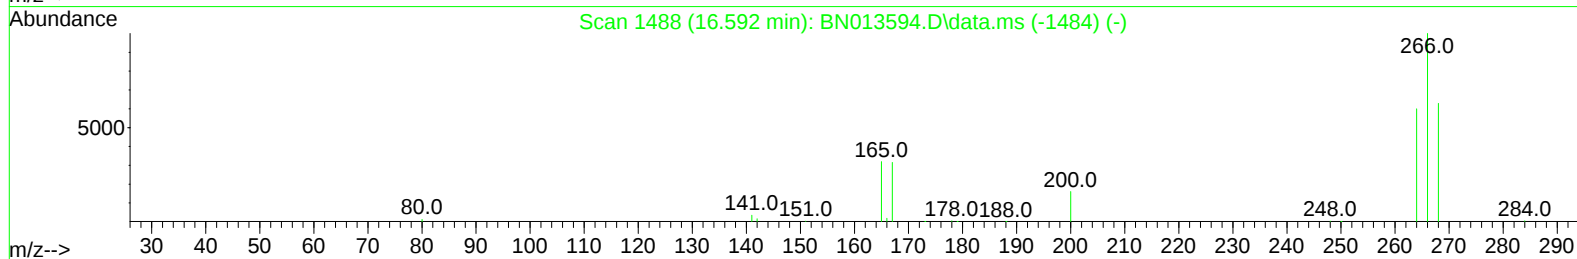
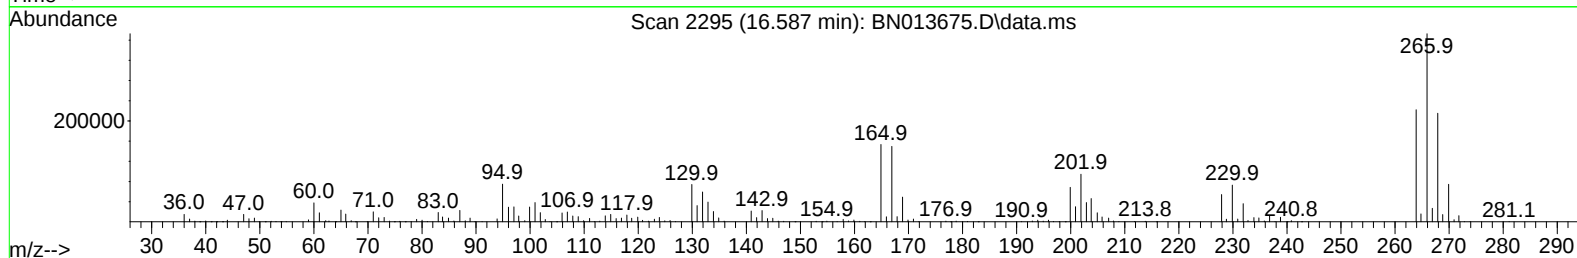


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021921\
Data File : BN013675.D
Acq On : 19 Feb 2021 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 10:13:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 10:50:10 2021
Response via : Initial Calibration

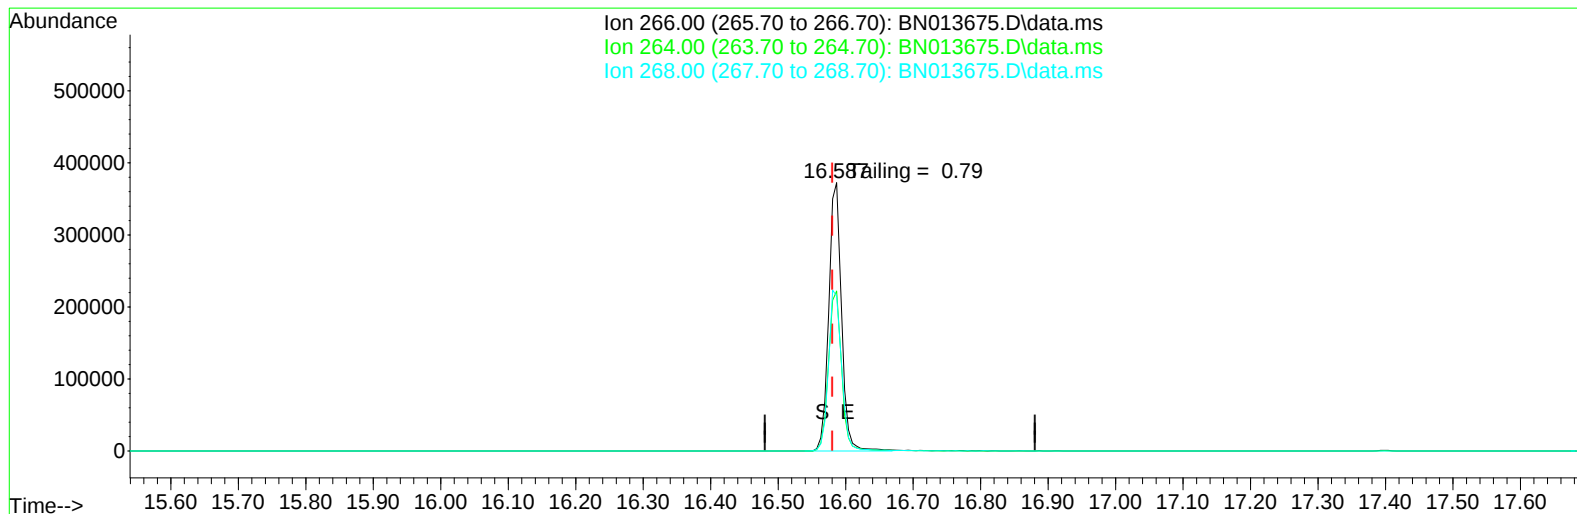

TIC: BN013675.D\data.ms

(24) Pentachlorophenol

16.587min (+ 0.006) 25951.66 ng

response 490143

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	61.49
268.00	68.30	61.54
0.00	0.00	0.00