


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021921\
 Data File : BN013675.D
 Acq On : 19 Feb 2021 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 18 10:50:10 2021

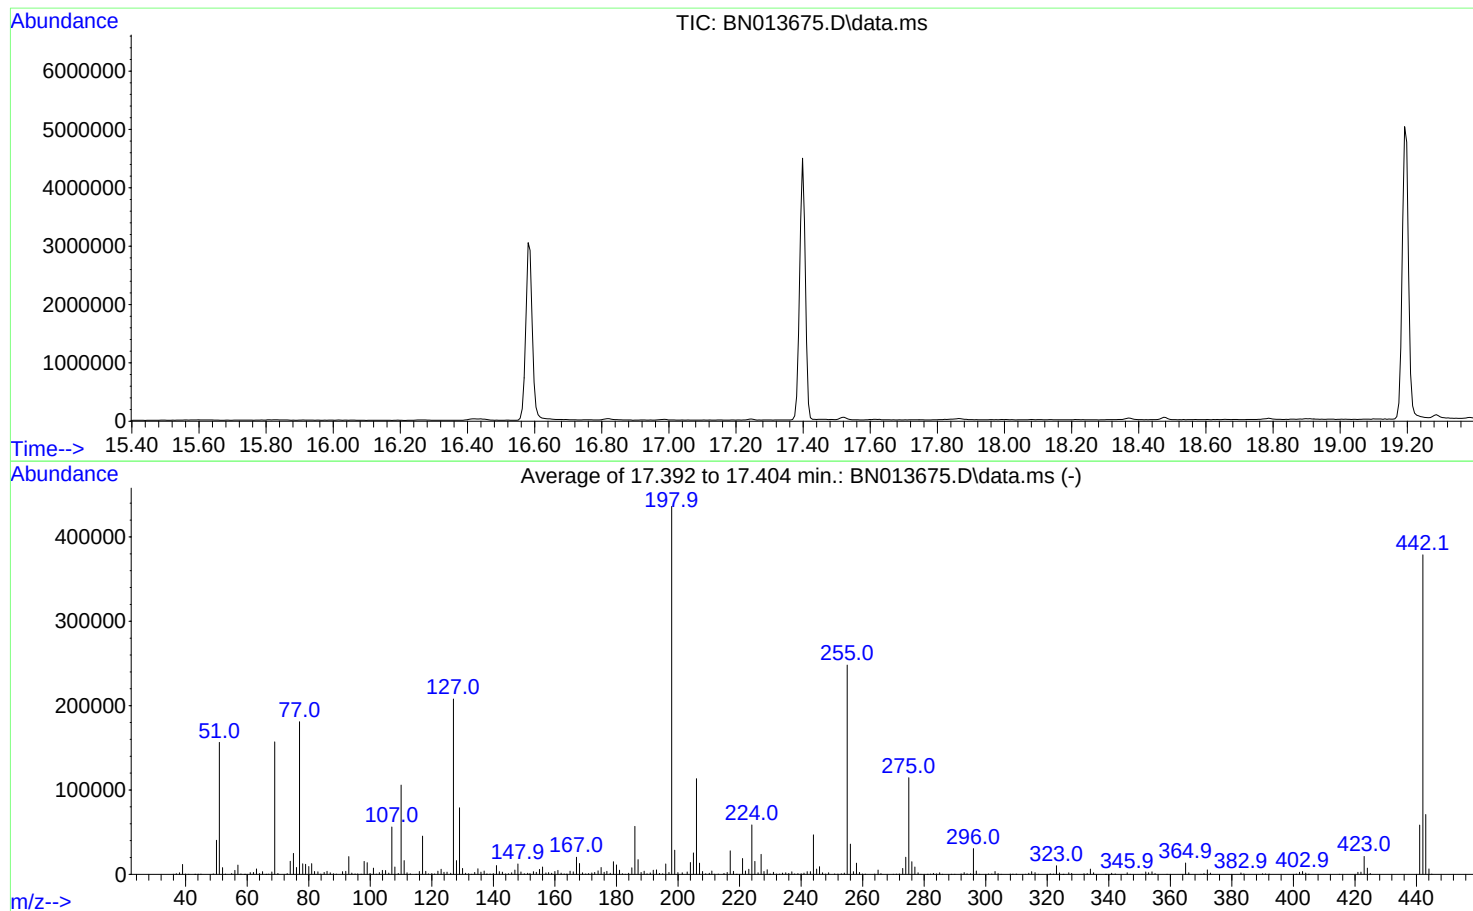

AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	156464	PASS
68	69	0.00	2	1.9	2949	PASS
69	198	0.00	100	36.0	157078	PASS
70	69	0.00	2	0.7	1069	PASS
127	198	10	80	47.7	207979	PASS
197	198	0.00	2	0.5	2357	PASS
198	198	100	100	100.0	436053	PASS
199	198	5	9	6.6	28677	PASS
275	198	10	60	26.3	114627	PASS
365	198	1	100	3.1	13460	PASS
441	198	0.01	100	13.4	58336	PASS
442	442	50	100	100.0	378752	PASS
443	442	15	24	18.7	70917	PASS

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP




Date	Instrument Name	DFTPP Data File
02/19/2021	BNA_N	<u>BN013675.D</u>
Compound Name	Response	Retention Time
DDT	1449510	20.44
DDD	22478	20
DDE	3940	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26418	1475928	1.79

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021921\
Data File : BN013675.D
Acq On : 19 Feb 2021 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 20 04:42:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

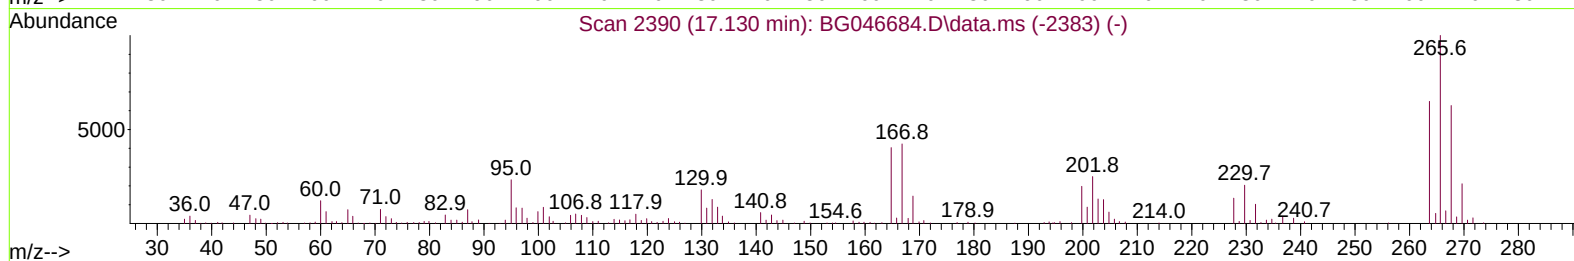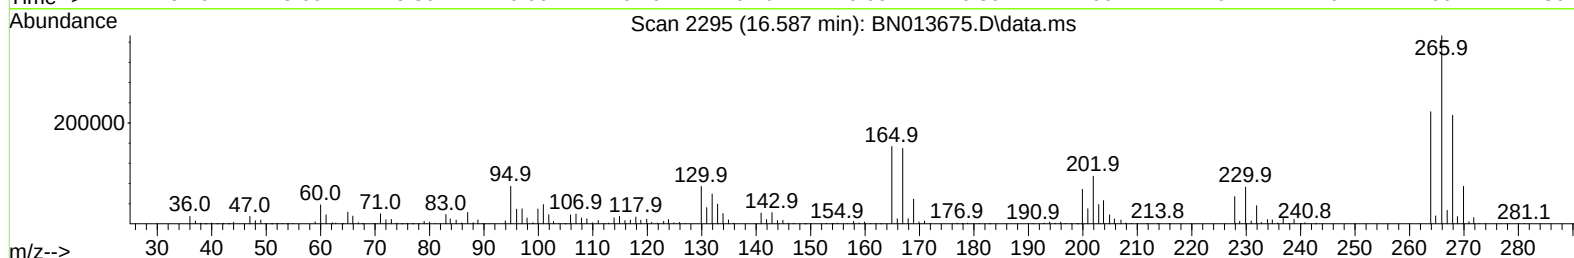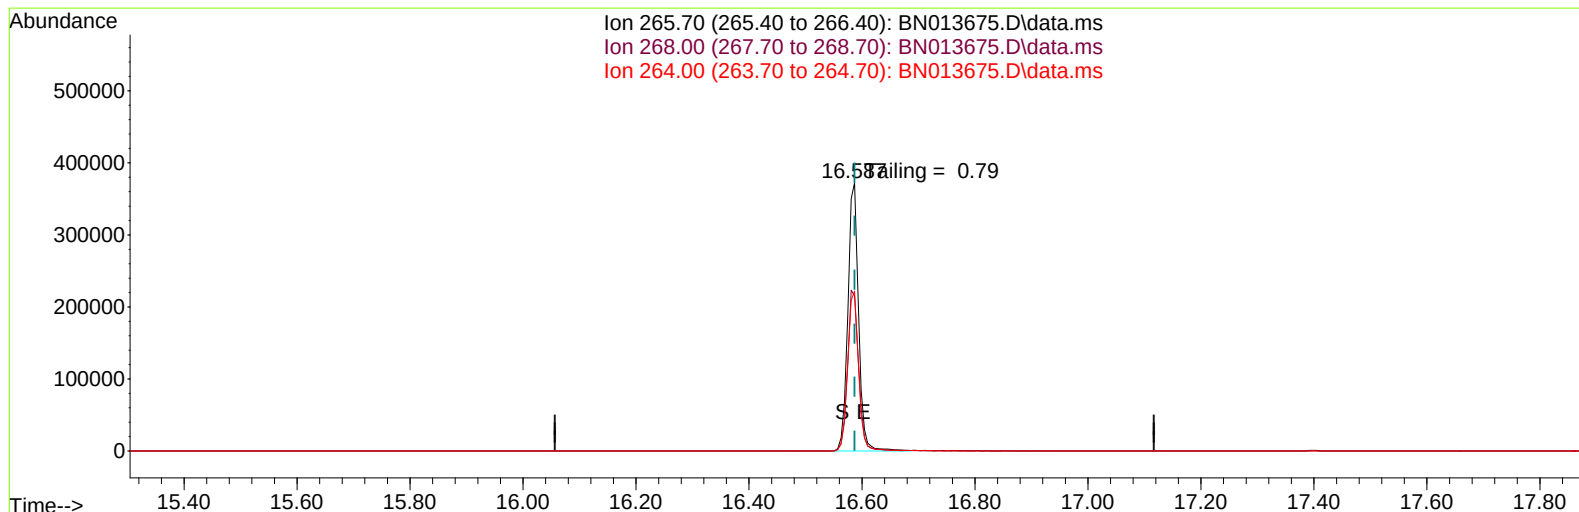

TIC: BN013675.D\data.ms

(70) Pentachlorophenol (C)

16.587min (+ 0.000) 21150.19 ng




response 490143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	59.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021921\
Data File : BN013675.D
Acq On : 19 Feb 2021 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 20 04:42:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

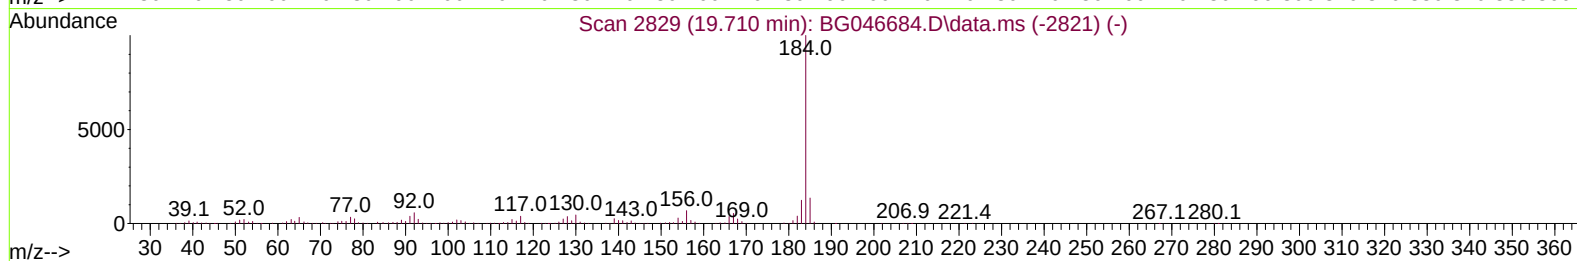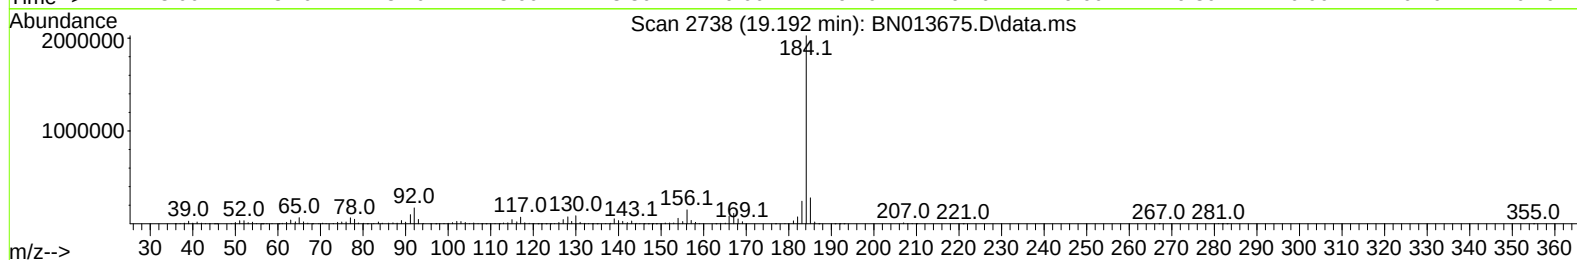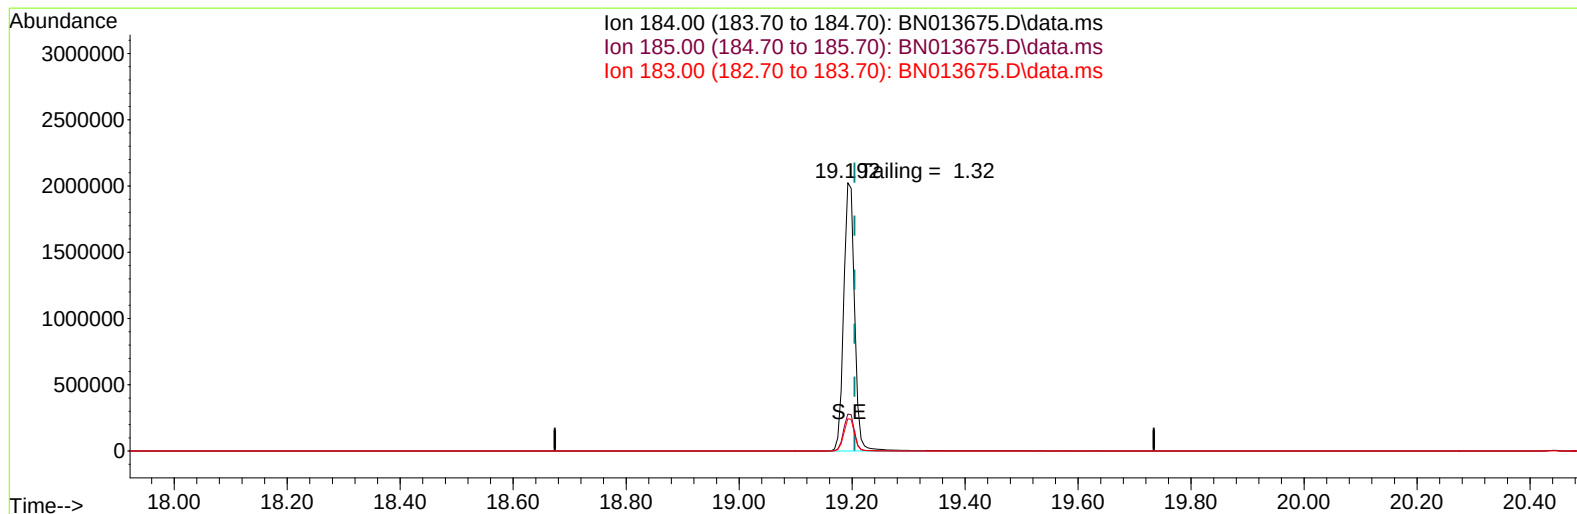

TIC: BN013675.D\data.ms

(77) Benzidine

19.192min (-0.012) 0.00 ng

response 2702976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	12.05
0.00	0.00	0.00