




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029851.D
Acq On : 19 Feb 2024 14:52
Operator : MA/JU
Sample : P1402-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD9

Manual IntegrationsAPPROVED

Quant Time: Feb 19 15:29:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :mohammad ahmed 02/21/2024

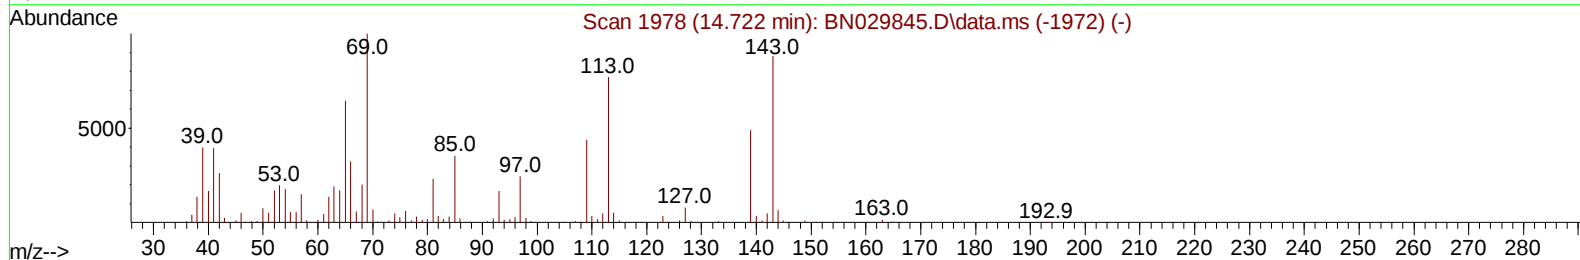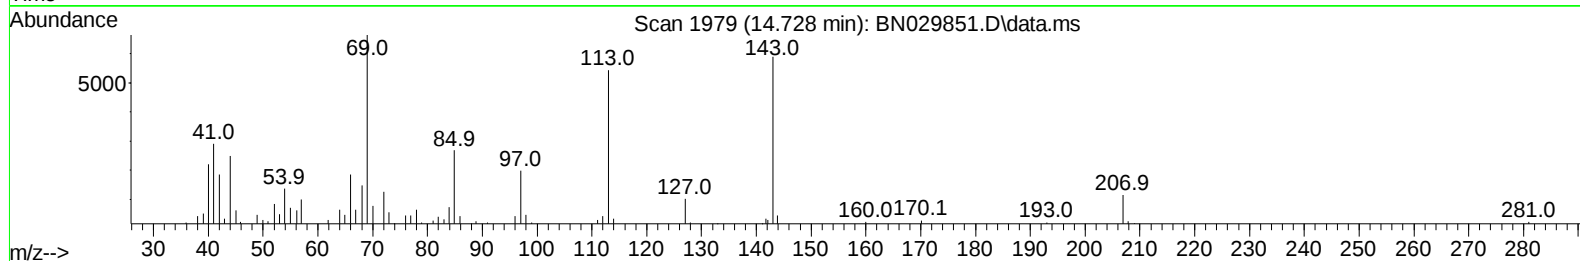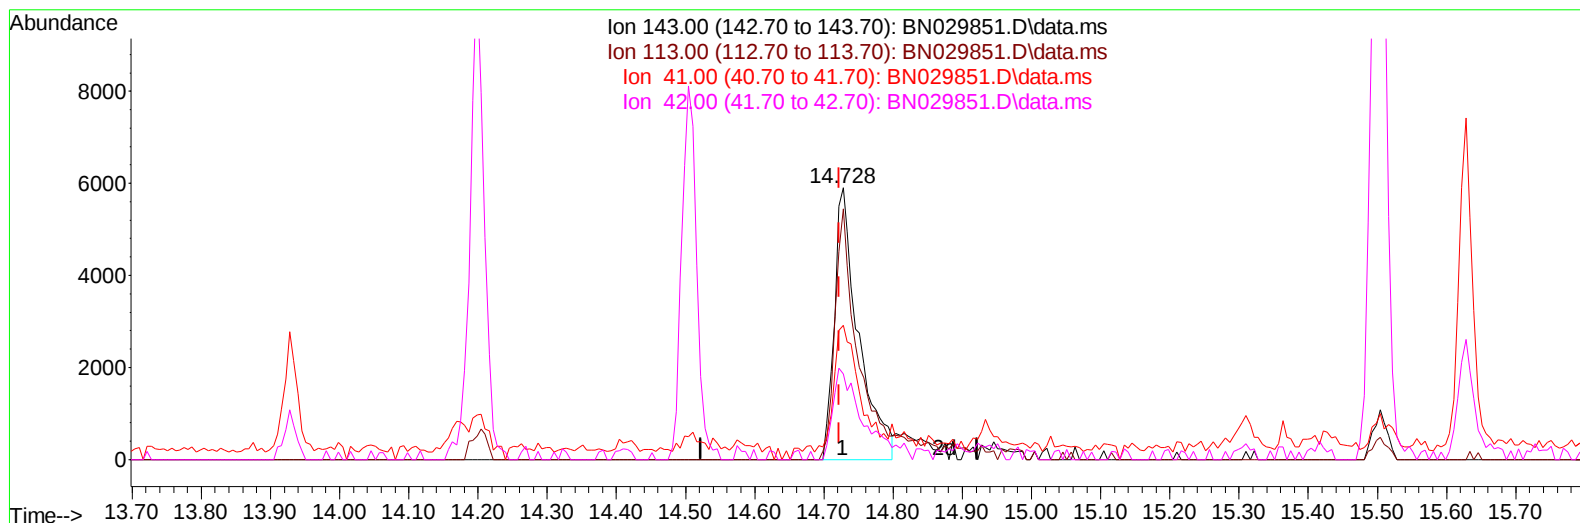

TIC: BN029851.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.006) 3.19 ng/u1

response 14182

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	92.27
41.00	45.90	49.34
42.00	28.40	31.42




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029851.D
Acq On : 19 Feb 2024 14:52
Operator : MA/JU
Sample : P1402-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD9

Manual IntegrationsAPPROVED

Quant Time: Feb 19 15:29:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :mohammad ahmed 02/21/2024

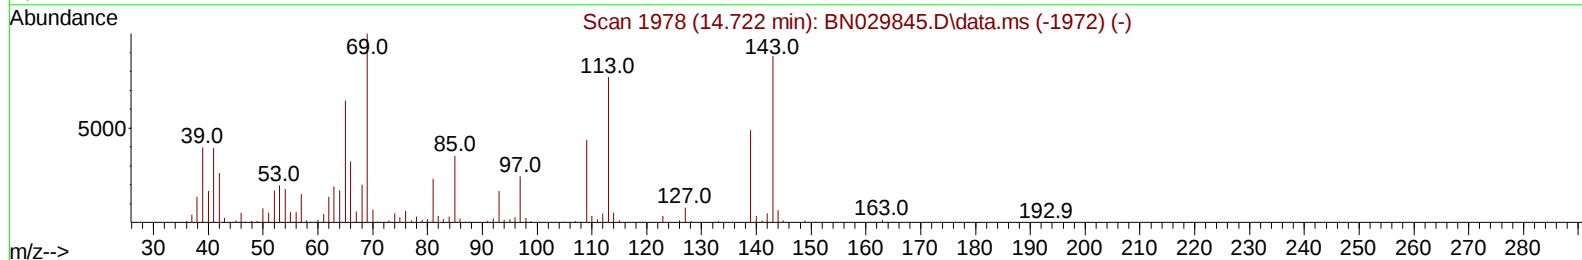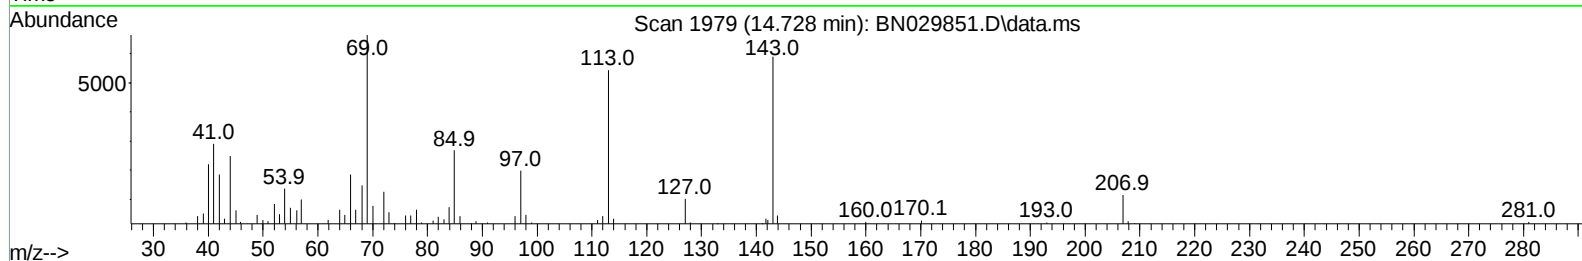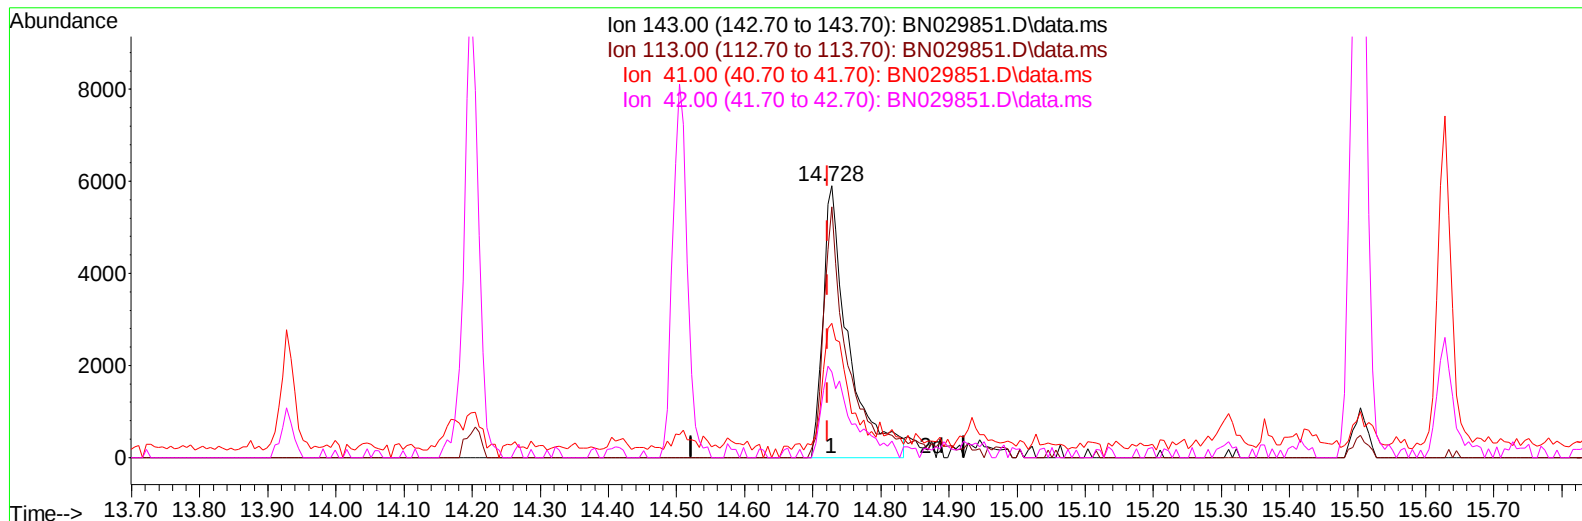

TIC: BN029851.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (+ 0.006) 3.43 ng/ul m

response 15254

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	92.27
41.00	45.90	49.34
42.00	28.40	31.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029851.D
 Acq On : 19 Feb 2024 14:52
 Operator : MA/JU
 Sample : P1402-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/21/2024
 Supervised By :mohammad ahmed 02/21/2024

Quant Time: Feb 19 22:34:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	146051	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	590152	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.504	164	314567	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.257	188	654597	20.000	ng/ul	-0.01
79) Chrysene-d12	21.457	240	564079	20.000	ng/ul	-0.01
88) Perylene-d12	23.827	264	615644	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	17097	3.850	ng/uL	0.00
4) Pyridine-d5	3.740	84	118115	9.974	ng/ul	0.01
7) Phenol-d5	7.034	99	72270	5.290	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	273212	29.967	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.393	132	225752	22.805	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	135578	13.307	ng/ul	-0.01
21) Nitrobenzene-d5	9.034	128	157183	34.317	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	133640	33.501	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	234682	29.805	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.810	131	323992	24.119	ng/ul	0.00
46) Dimethylphthalate-d6	13.928	166	856754	36.582	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	975147	35.061	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	15254m	3.432	ng/ul	0.00
60) Fluorene-d10	15.504	176	749346	37.611	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	86473	27.111	ng/ul	0.00
73) Anthracene-d10	17.357	188	1225172	39.936	ng/ul	0.00
81) Pyrene-d10	19.657	212	1480188	43.727	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	1346190	43.699	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029851.D
Acq On : 19 Feb 2024 14:52
Operator : MA/JU
Sample : P1402-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD9

Manual IntegrationsAPPROVED

Quant Time: Feb 19 22:34:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/21/2024
Supervised By :mohammad ahmed 02/21/2024

