

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029846.D
 Acq On : 19 Feb 2024 11:52
 Operator : MA/JU
 Sample : PB159058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	36	39	47	rVB	72170	91675	2.12%	0.181%
2	3.728	105	109	132	rBV	743840	1272288	29.42%	2.511%
3	4.051	160	164	172	rVB	16690	24487	0.57%	0.048%
4	7.028	663	670	683	rBV	995636	1613804	37.32%	3.184%
5	7.204	693	700	713	rBV	814148	1269670	29.36%	2.505%
6	7.387	724	731	745	rBV	1000892	1619395	37.45%	3.196%
7	7.863	805	812	820	rVB	744628	1202432	27.81%	2.373%
8	8.575	924	933	947	rBV	1161248	1913121	44.25%	3.775%
9	9.028	1002	1010	1019	rBV	941763	1556975	36.01%	3.072%
10	9.745	1124	1132	1147	rBV	724716	1234581	28.55%	2.436%
11	10.281	1215	1223	1242	rBV	1113796	1901425	43.97%	3.752%
12	10.657	1280	1287	1298	rVB	1003537	1676204	38.77%	3.308%
13	10.810	1305	1313	1337	rBV	996472	1918381	44.37%	3.786%
14	12.251	1550	1558	1566	rBV2	19739	33311	0.77%	0.066%
15	13.410	1749	1755	1763	rVV2	17476	29061	0.67%	0.057%
16	13.480	1763	1767	1773	rVB6	3386	6733	0.16%	0.013%
17	13.927	1837	1843	1854	rBV	1848110	2626104	60.73%	5.182%
18	14.198	1881	1889	1908	rBV	2113571	3136673	72.54%	6.190%
19	14.504	1934	1941	1953	rBV	1323117	2015737	46.62%	3.978%
20	14.716	1971	1977	2000	rBV	497776	1082390	25.03%	2.136%
21	15.504	2103	2111	2126	rBV	2607409	3767453	87.13%	7.434%
22	15.627	2126	2132	2147	rVV	671271	960749	22.22%	1.896%
23	15.745	2147	2152	2156	rVB3	12029	19628	0.45%	0.039%
24	16.069	2204	2207	2213	rVB6	4183	5798	0.13%	0.011%
25	16.192	2222	2228	2232	rBV8	3397	6875	0.16%	0.014%
26	16.292	2237	2245	2250	rBV9	9073	15677	0.36%	0.031%
27	16.939	2352	2355	2358	rBV4	4403	4796	0.11%	0.009%
28	17.257	2401	2409	2419	rBV	1538869	2263275	52.34%	4.466%
29	17.357	2419	2426	2443	rVV	2716098	3990473	92.29%	7.874%
30	19.221	2739	2743	2750	rBV2	30089	40362	0.93%	0.080%
31	19.292	2751	2755	2760	rVV2	23757	31548	0.73%	0.062%
32	19.657	2811	2817	2826	rBV	3035043	4323902	100.00%	8.532%
33	21.462	3118	3124	3135	rBV	1632894	2232922	51.64%	4.406%
34	23.150	3408	3411	3416	rVB	58393	81418	1.88%	0.161%
35	23.674	3492	3500	3512	rBV2	2027467	4058982	93.87%	8.010%
36	23.827	3520	3526	3539	rVB	1137478	2318549	53.62%	4.575%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029846.D
Acq On : 19 Feb 2024 11:52
Operator : MA/JU
Sample : PB159058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	24.503	3636	3641	3649	rVB2	78629	163413	3.78%	0.322%
38	25.339	3779	3783	3795	rVB3	73737	166621	3.85%	0.329%




Sum of corrected areas: 50676888

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029846.D
Acq On : 19 Feb 2024 11:52
Operator : MA/JU
Sample : PB159058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

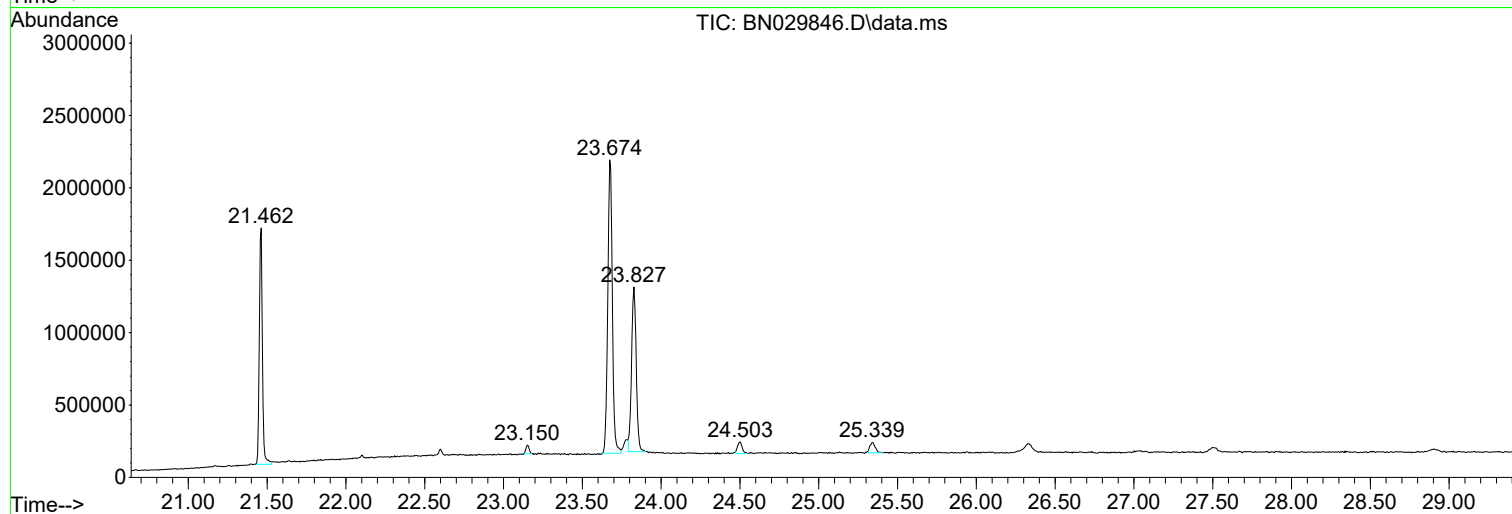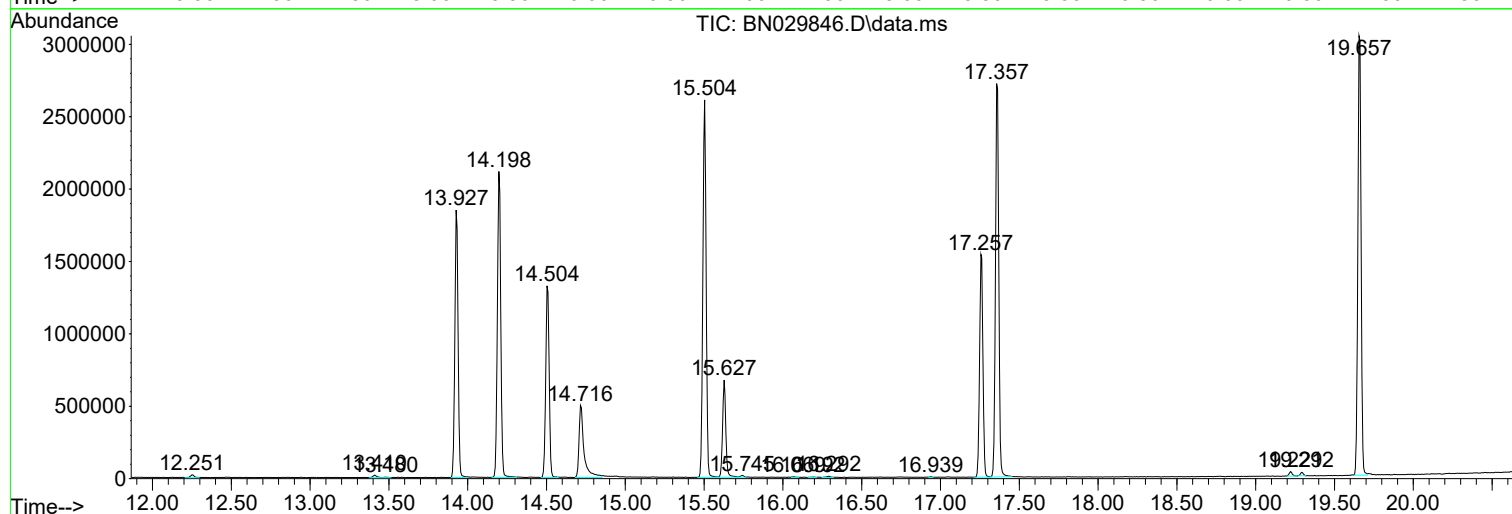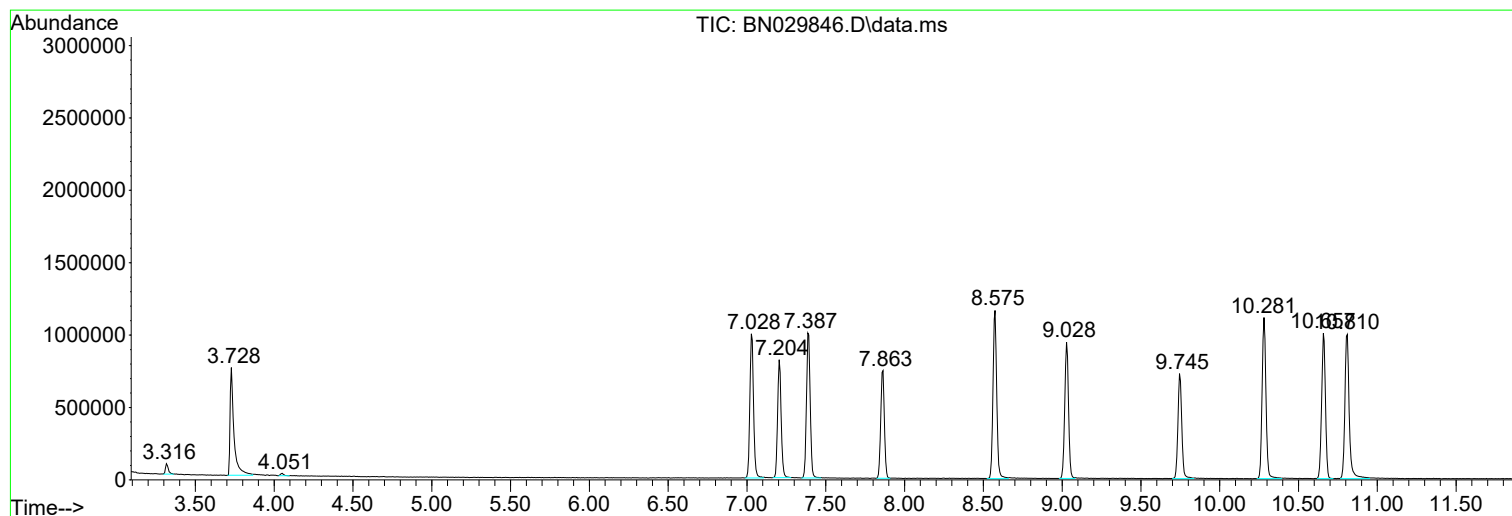

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029846.D
Acq On : 19 Feb 2024 11:52
Operator : MA/JU
Sample : PB159058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029846.D
Acq On : 19 Feb 2024 11:52
Operator : MA/JU
Sample : PB159058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc