

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029849.D
 Acq On : 19 Feb 2024 13:40
 Operator : MA/JU
 Sample : PB158958BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK958

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	36	39	47	rVB	60749	74651	2.03%	0.177%
2	3.569	80	82	85	rVB4	4596	4035	0.11%	0.010%
3	3.728	106	109	133	rBV	599725	1055902	28.77%	2.510%
4	4.052	160	164	169	rVB2	17060	22932	0.62%	0.055%
5	5.499	408	410	414	rVB3	2865	4000	0.11%	0.010%
6	5.981	489	492	494	rBV4	3300	4534	0.12%	0.011%
7	7.034	664	671	683	rBV	846447	1339572	36.49%	3.184%
8	7.210	694	701	712	rVV	661814	1069794	29.14%	2.543%
9	7.393	725	732	745	rVV	863755	1345022	36.64%	3.197%
10	7.863	805	812	820	rVB	639770	1008035	27.46%	2.396%
11	8.575	925	933	945	rBV	977000	1594716	43.44%	3.791%
12	9.034	1003	1011	1022	rBV	762544	1290976	35.17%	3.069%
13	9.751	1125	1133	1142	rBV	588650	1000616	27.26%	2.379%
14	10.281	1215	1223	1237	rBV	909225	1556470	42.40%	3.700%
15	10.663	1280	1288	1295	rBV	809041	1389647	37.86%	3.303%
16	10.810	1304	1313	1332	rBV	855004	1607181	43.78%	3.821%
17	12.257	1554	1559	1564	rBV3	16252	25367	0.69%	0.060%
18	13.410	1750	1755	1761	rBV3	14051	20685	0.56%	0.049%
19	13.481	1761	1767	1771	rVV6	2056	3711	0.10%	0.009%
20	13.928	1837	1843	1857	rBV	1519730	2116258	57.65%	5.031%
21	14.198	1882	1889	1905	rBV	1724103	2547647	69.40%	6.056%
22	14.504	1935	1941	1952	rBV	1076437	1622933	44.21%	3.858%
23	14.716	1970	1977	1995	rBV	413422	907854	24.73%	2.158%
24	14.951	2012	2017	2020	rVB6	4323	6797	0.19%	0.016%
25	15.504	2104	2111	2123	rBV	2164876	3083522	84.00%	7.330%
26	15.627	2126	2132	2144	rVV	544411	777192	21.17%	1.848%
27	15.739	2147	2151	2156	rVB5	10860	18228	0.50%	0.043%
28	16.286	2238	2244	2249	rBV4	6871	10374	0.28%	0.025%
29	16.933	2352	2354	2360	rVB6	2922	4504	0.12%	0.011%
30	17.257	2403	2409	2419	rBV	1314894	1888380	51.44%	4.489%
31	17.357	2419	2426	2438	rBV2	2305910	3336592	90.90%	7.932%
32	19.221	2738	2743	2748	rBV2	26206	34881	0.95%	0.083%
33	19.292	2750	2755	2761	rBV	21212	32026	0.87%	0.076%
34	19.657	2811	2817	2833	rBV	2729607	3670712	100.00%	8.726%
35	19.851	2848	2850	2852	rBV3	3663	3857	0.11%	0.009%
36	21.457	3118	3123	3129	rBV2	1364502	1845086	50.27%	4.386%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029849.D
Acq On : 19 Feb 2024 13:40
Operator : MA/JU
Sample : PB158958BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.151	3408	3411	3418	rVB3	66837	102454	2.79%	0.244%
38	23.674	3493	3500	3511	rBV2	1724159	3387119	92.27%	8.052%
39	23.774	3514	3517	3519	rVV	97718	135117	3.68%	0.321%
40	23.827	3519	3526	3535	rVB	943080	1954015	53.23%	4.645%
41	24.498	3636	3640	3648	rVB3	78108	162677	4.43%	0.387%




Sum of corrected areas: 42066071

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029849.D
Acq On : 19 Feb 2024 13:40
Operator : MA/JU
Sample : PB158958BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

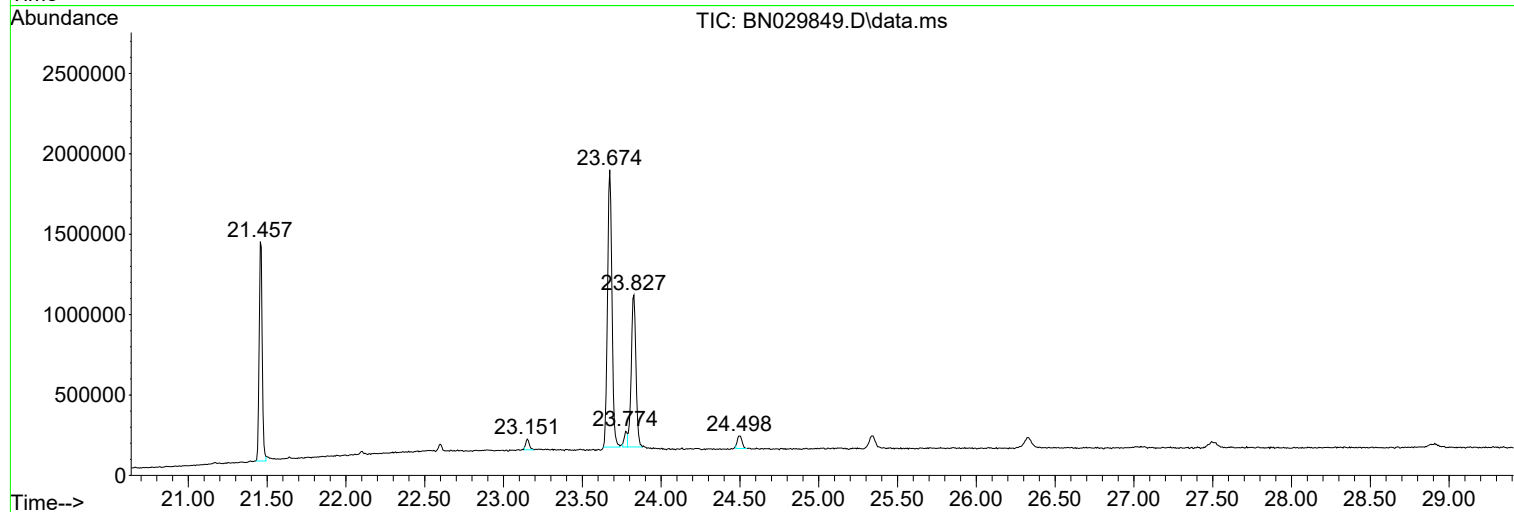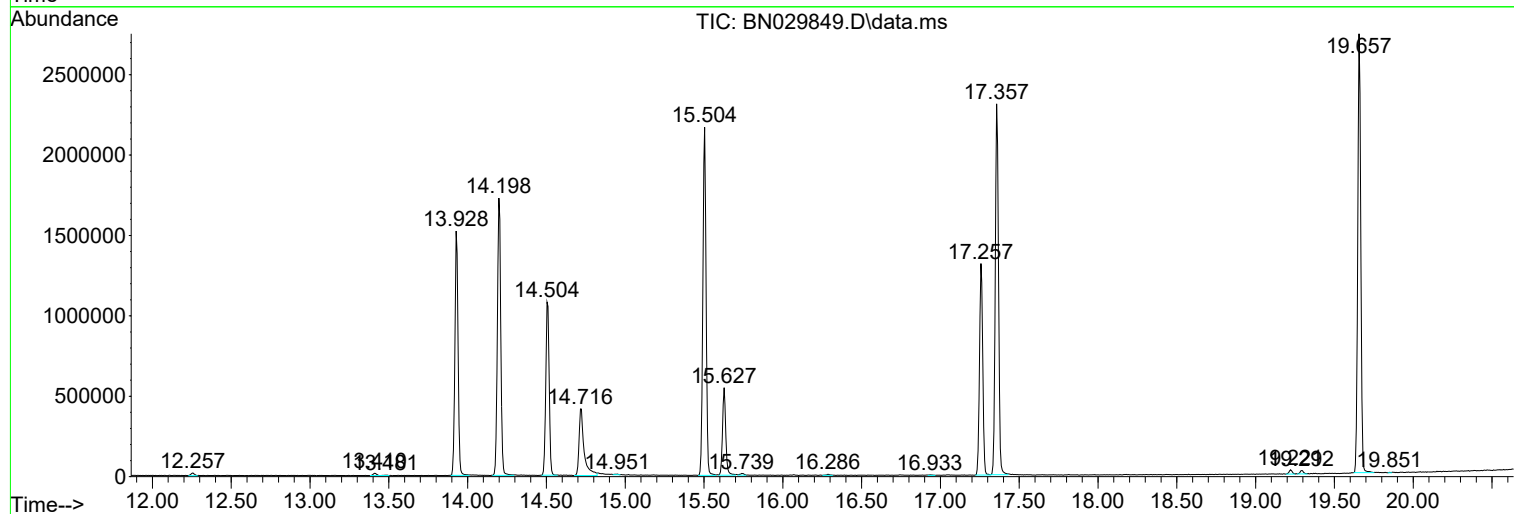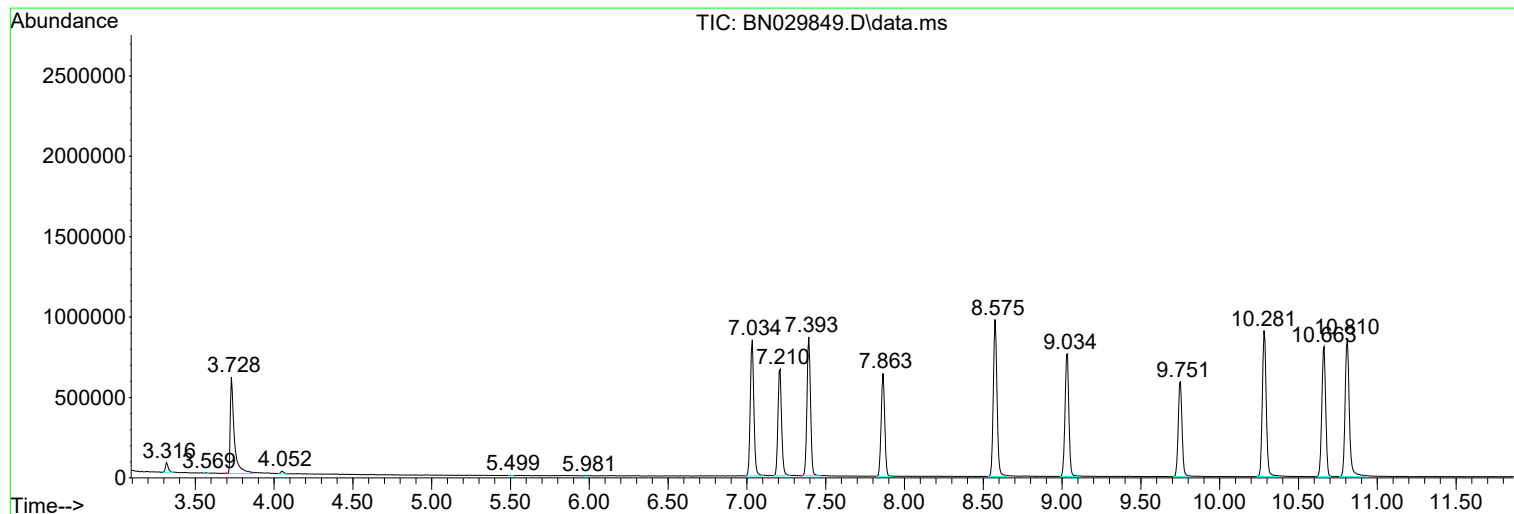

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029849.D
Acq On : 19 Feb 2024 13:40
Operator : MA/JU
Sample : PB158958BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029849.D
Acq On : 19 Feb 2024 13:40
Operator : MA/JU
Sample : PB158958BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc