

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029852.D
 Acq On : 19 Feb 2024 15:29
 Operator : MA/JU
 Sample : P1402-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	44	rBV	732882	1126976	26.83%	2.736%
2	3.740	108	111	128	rBV	89626	195984	4.67%	0.476%
3	4.052	160	164	169	rVB2	12923	21105	0.50%	0.051%
4	4.569	247	252	264	rVB	293978	441234	10.50%	1.071%
5	5.981	488	492	495	rVB5	2944	4848	0.12%	0.012%
6	7.034	665	671	683	rVB	153519	254459	6.06%	0.618%
7	7.210	693	701	714	rBV	660199	1093378	26.03%	2.655%
8	7.393	725	732	743	rBV	643780	1007367	23.98%	2.446%
9	7.469	743	745	754	rVB8	6060	11788	0.28%	0.029%
10	7.863	805	812	821	rBV	666951	1039713	24.75%	2.525%
11	8.575	925	933	944	rBV	434639	724682	17.25%	1.760%
12	9.028	1002	1010	1021	rBV	790181	1318601	31.39%	3.202%
13	9.751	1124	1133	1148	rBV	554201	969475	23.08%	2.354%
14	10.281	1215	1223	1235	rBV	816348	1387389	33.03%	3.369%
15	10.657	1278	1287	1299	rBV	822046	1415684	33.70%	3.437%
16	10.810	1305	1313	1336	rBV	613786	1162413	27.67%	2.822%
17	11.434	1413	1419	1422	rBV5	3008	5025	0.12%	0.012%
18	12.251	1552	1558	1566	rVB3	15737	25010	0.60%	0.061%
19	12.698	1629	1634	1639	rBV8	2967	4287	0.10%	0.010%
20	13.334	1738	1742	1747	rBV6	4420	7707	0.18%	0.019%
21	13.416	1749	1756	1762	rVB5	8621	17093	0.41%	0.042%
22	13.481	1762	1767	1770	rBV6	2741	4713	0.11%	0.011%
23	13.928	1837	1843	1858	rBV	1583180	2264469	53.90%	5.498%
24	14.034	1858	1861	1866	rVB7	3472	5694	0.14%	0.014%
25	14.198	1882	1889	1905	rBV	1757979	2632536	62.66%	6.392%
26	14.504	1935	1941	1951	rBV	1083719	1632795	38.87%	3.965%
27	14.728	1973	1979	1997	rBV2	47698	139140	3.31%	0.338%
28	15.316	2074	2079	2082	rBV2	10970	15818	0.38%	0.038%
29	15.504	2104	2111	2119	rBV	2336216	3312482	78.85%	8.043%
30	15.628	2126	2132	2143	rBV	621814	855075	20.35%	2.076%
31	15.745	2148	2152	2157	rVB4	9938	16683	0.40%	0.041%
32	16.063	2202	2206	2209	rBV6	2966	5842	0.14%	0.014%
33	16.292	2240	2245	2249	rBV4	7220	12579	0.30%	0.031%
34	17.039	2368	2372	2375	rBV5	3153	4390	0.10%	0.011%
35	17.257	2402	2409	2419	rBV	1302278	1872115	44.56%	4.546%
36	17.357	2420	2426	2441	rVV2	2580483	3688186	87.79%	8.955%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029852.D
 Acq On : 19 Feb 2024 15:29
 Operator : MA/JU
 Sample : P1402-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.939	2521	2525	2529	rVB5	8658	12058	0.29%	0.029%
38	18.169	2558	2564	2575	rBV2	48498	77237	1.84%	0.188%
39	18.251	2575	2578	2580	rVB4	4503	5202	0.12%	0.013%
40	19.033	2707	2711	2713	rBV4	3648	4312	0.10%	0.010%
41	19.222	2739	2743	2748	rBV3	29651	42702	1.02%	0.104%
42	19.292	2751	2755	2759	rBV	26262	36092	0.86%	0.088%
43	19.457	2779	2783	2787	rBV4	17694	26675	0.63%	0.065%
44	19.610	2806	2809	2811	rBV4	11492	11898	0.28%	0.029%
45	19.657	2811	2817	2827	rVV	3107741	4201019	100.00%	10.200%
46	19.898	2856	2858	2864	rVB3	6247	6557	0.16%	0.016%
47	21.198	3076	3079	3086	rVB6	28595	41404	0.99%	0.101%
48	21.463	3118	3124	3135	rBV	1412177	1917873	45.65%	4.657%
49	23.680	3493	3501	3512	rBV	2047657	4143402	98.63%	10.061%
50	23.827	3519	3526	3537	rVB	957716	1961393	46.69%	4.762%




Sum of corrected areas: 41184559

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029852.D
Acq On : 19 Feb 2024 15:29
Operator : MA/JU
Sample : P1402-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

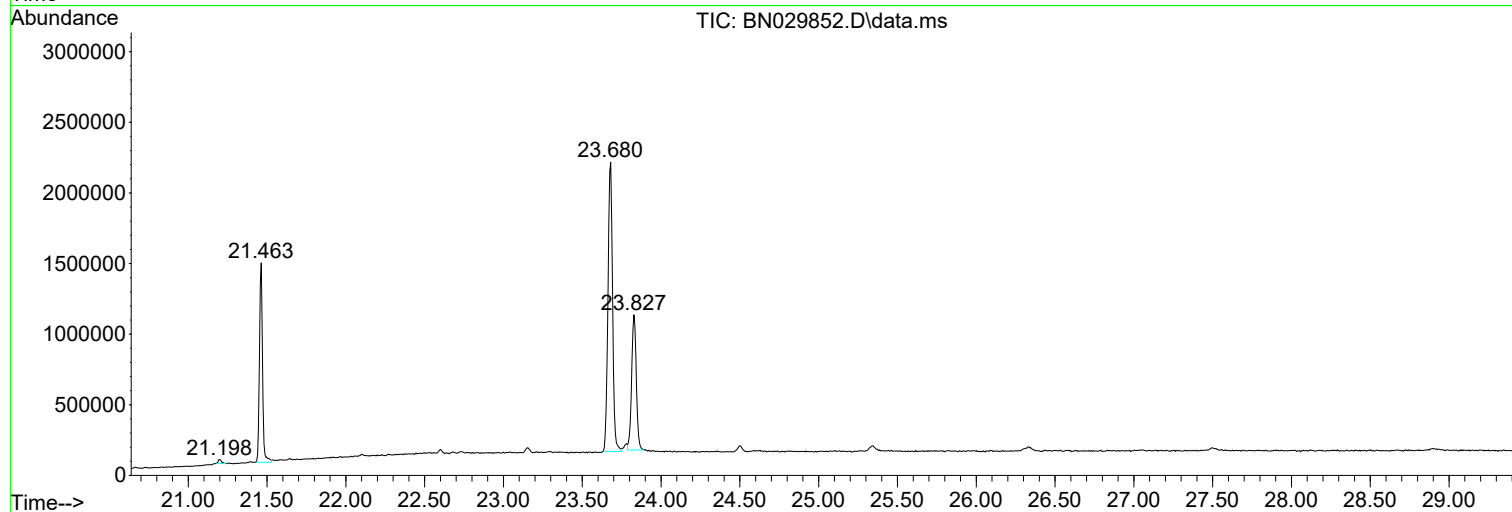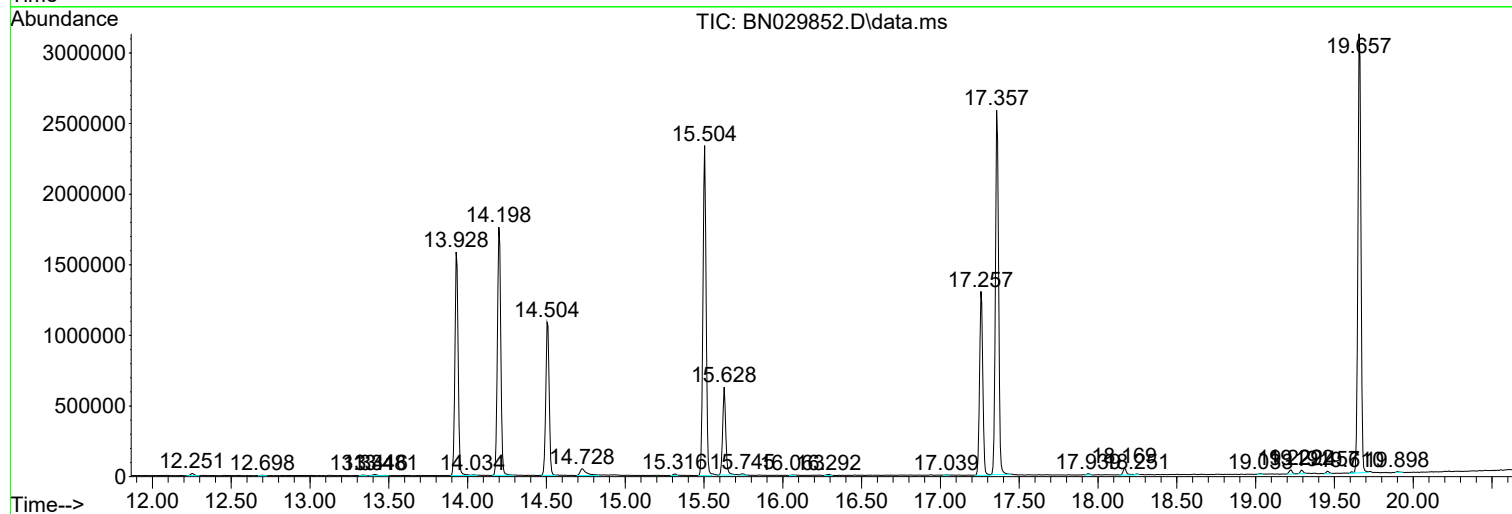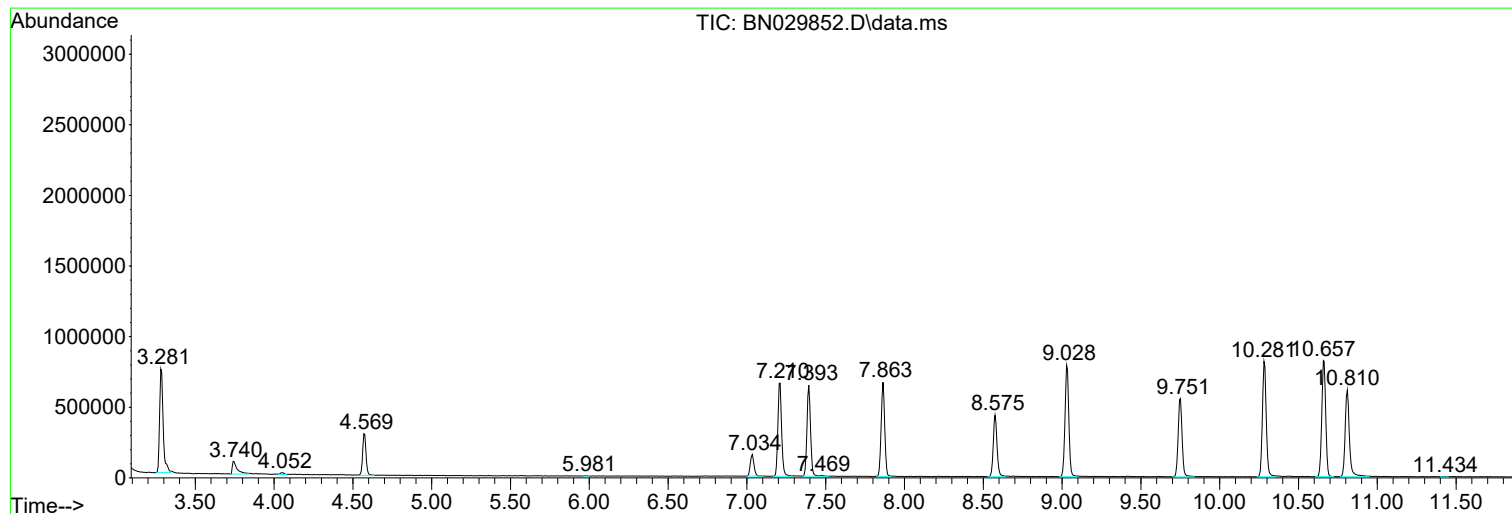

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029852.D
Acq On : 19 Feb 2024 15:29
Operator : MA/JU
Sample : P1402-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029852.D
Acq On : 19 Feb 2024 15:29
Operator : MA/JU
Sample : P1402-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc