

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029853.D
 Acq On : 19 Feb 2024 16:05
 Operator : MA/JU
 Sample : P1402-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	38	rBV	188311	280241	6.68%	0.701%
2	3.316	38	39	43	rVV	39187	44041	1.05%	0.110%
3	3.352	43	45	53	rVB	28577	41050	0.98%	0.103%
4	3.740	108	111	125	rBV	120596	226046	5.38%	0.565%
5	4.052	161	164	167	rVB	11889	14458	0.34%	0.036%
6	4.569	247	252	261	rVB	378032	560288	13.35%	1.401%
7	7.034	665	671	680	rVV	176674	288155	6.86%	0.721%
8	7.210	694	701	710	rBV	700099	1142926	27.22%	2.858%
9	7.393	725	732	744	rBV	703047	1100921	26.22%	2.753%
10	7.475	744	746	750	rVB5	5329	5899	0.14%	0.015%
11	7.863	805	812	822	rBV	561281	878760	20.93%	2.198%
12	8.575	926	933	946	rBV	496966	810798	19.31%	2.028%
13	9.028	1002	1010	1022	rBV	818598	1393993	33.20%	3.486%
14	9.745	1125	1132	1145	rBV	609013	1032954	24.60%	2.583%
15	10.281	1215	1223	1237	rBV	881559	1496597	35.65%	3.743%
16	10.657	1280	1287	1299	rBV	699796	1204875	28.70%	3.013%
17	10.810	1303	1313	1329	rBV	645640	1215624	28.96%	3.040%
18	12.251	1551	1558	1566	rBV2	15707	26714	0.64%	0.067%
19	13.339	1739	1743	1746	rBV5	3295	5101	0.12%	0.013%
20	13.410	1749	1755	1761	rVV5	7375	12605	0.30%	0.032%
21	13.928	1837	1843	1856	rBV	1656602	2346429	55.89%	5.868%
22	14.198	1882	1889	1899	rBV	1839218	2741700	65.31%	6.857%
23	14.510	1934	1942	1950	rBV	907222	1380972	32.89%	3.454%
24	14.728	1972	1979	1989	rBV2	54821	135467	3.23%	0.339%
25	14.928	2011	2013	2022	rVB7	3651	8348	0.20%	0.021%
26	15.316	2071	2079	2086	rBV	13524	21702	0.52%	0.054%
27	15.504	2104	2111	2126	rBV	2405987	3449740	82.17%	8.628%
28	15.628	2126	2132	2142	rBV	652222	899527	21.43%	2.250%
29	15.739	2148	2151	2157	rVB4	11688	17041	0.41%	0.043%
30	16.075	2202	2208	2210	rBV7	3893	5350	0.13%	0.013%
31	16.286	2241	2244	2250	rVB6	8635	13180	0.31%	0.033%
32	16.680	2306	2311	2314	rBV6	2392	4689	0.11%	0.012%
33	17.257	2403	2409	2420	rBV	1098517	1597673	38.06%	3.996%
34	17.357	2420	2426	2443	rVV2	2547859	3711100	88.40%	9.281%
35	17.633	2471	2473	2477	rBV4	3219	5428	0.13%	0.014%
36	17.939	2521	2525	2530	rVB6	11093	17121	0.41%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029853.D
 Acq On : 19 Feb 2024 16:05
 Operator : MA/JU
 Sample : P1402-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	18.004	2530	2536	2541	rBV10	2962	4994	0.12%	0.012%
38	18.169	2558	2564	2570	rBV2	41052	58996	1.41%	0.148%
39	18.251	2574	2578	2581	rVV4	3924	6167	0.15%	0.015%
40	18.492	2615	2619	2625	rBV6	3868	7735	0.18%	0.019%
41	18.610	2635	2639	2640	rBV3	4177	5090	0.12%	0.013%
42	18.651	2643	2646	2648	rBV4	3337	4832	0.12%	0.012%
43	19.027	2707	2710	2713	rBV5	8363	10796	0.26%	0.027%
44	19.221	2738	2743	2748	rBV2	34692	50899	1.21%	0.127%
45	19.292	2751	2755	2759	rBV2	28418	36969	0.88%	0.092%
46	19.457	2779	2783	2787	rBV4	17795	24949	0.59%	0.062%
47	19.610	2807	2809	2811	rBV3	6234	6109	0.15%	0.015%
48	19.657	2811	2817	2827	rVV	2993341	4198242	100.00%	10.499%
49	21.198	3076	3079	3085	rVB5	22636	31139	0.74%	0.078%
50	21.463	3118	3124	3138	rBV	1142390	1647912	39.25%	4.121%
51	23.674	3493	3500	3514	rBV2	2090580	4085942	97.33%	10.219%
52	23.827	3519	3526	3536	rVB	799893	1667026	39.71%	4.169%




Sum of corrected areas: 39985310

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029853.D
Acq On : 19 Feb 2024 16:05
Operator : MA/JU
Sample : P1402-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

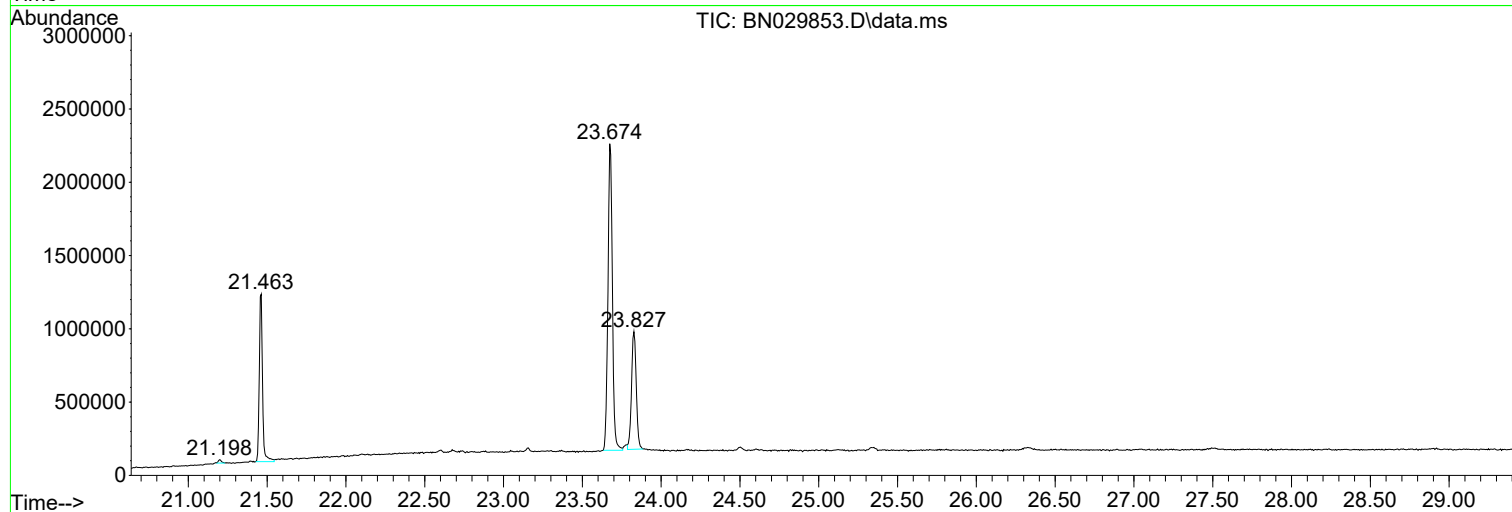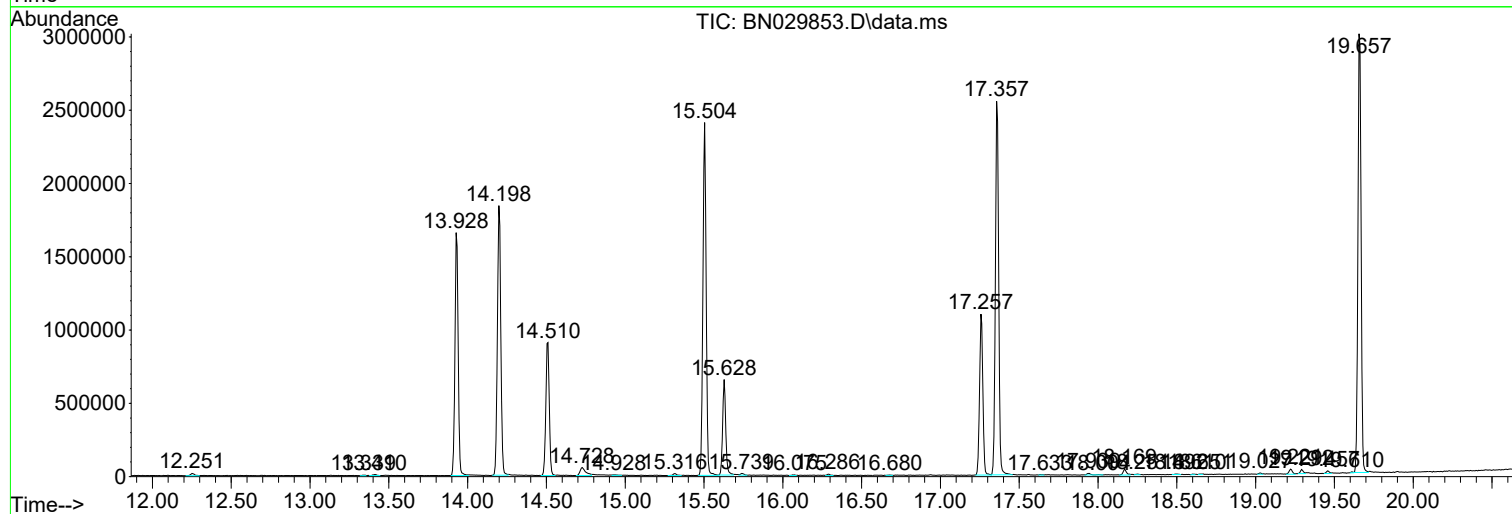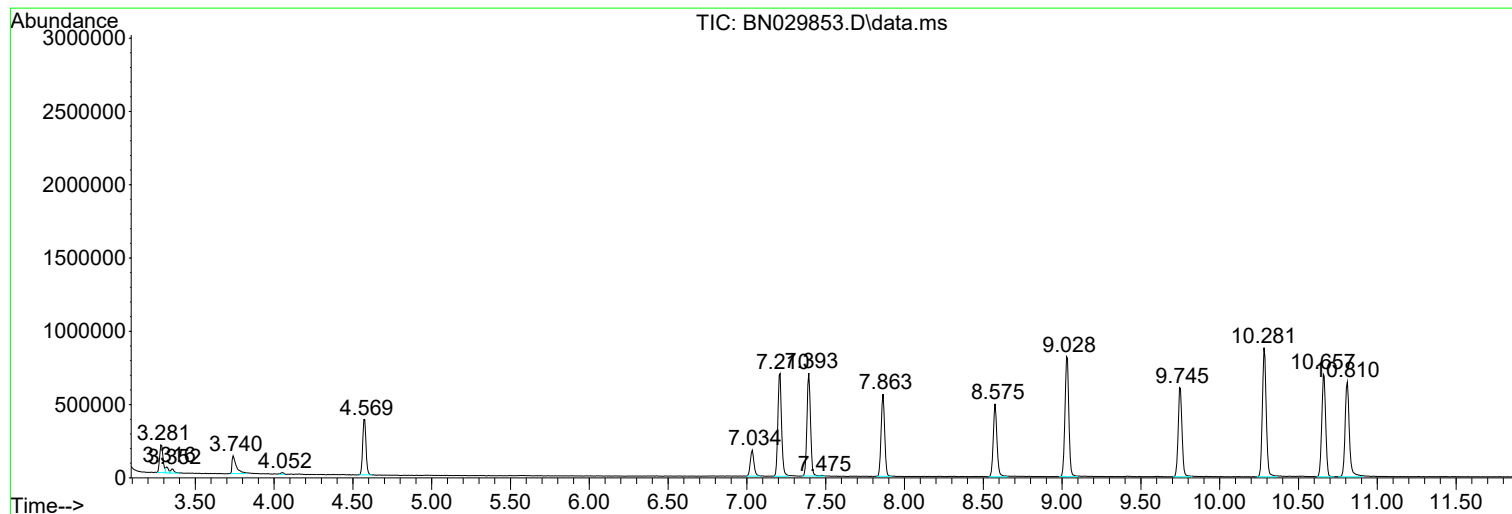

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029853.D
Acq On : 19 Feb 2024 16:05
Operator : MA/JU
Sample : P1402-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029853.D
Acq On : 19 Feb 2024 16:05
Operator : MA/JU
Sample : P1402-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc