

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029854.D
 Acq On : 19 Feb 2024 16:41
 Operator : MA/JU
 Sample : P1402-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	37	rBV	65719	91928	2.10%	0.228%
2	3.317	37	39	45	rVB	31570	40157	0.92%	0.100%
3	3.740	107	111	127	rBV	135551	265268	6.07%	0.659%
4	4.052	161	164	168	rVB	11661	13820	0.32%	0.034%
5	4.570	247	252	259	rBV	90021	131368	3.01%	0.326%
6	4.970	315	320	322	rBV6	3610	5473	0.13%	0.014%
7	7.034	664	671	680	rBV	156215	267121	6.11%	0.664%
8	7.205	694	700	712	rBV	718840	1154403	26.43%	2.869%
9	7.393	724	732	744	rBV	649262	1040811	23.82%	2.586%
10	7.469	744	745	749	rVB4	3763	4558	0.10%	0.011%
11	7.864	804	812	819	rBV	583277	913617	20.91%	2.270%
12	8.575	926	933	948	rBV2	442557	718945	16.46%	1.786%
13	9.028	1002	1010	1020	rBV	831931	1399341	32.03%	3.477%
14	9.611	1103	1109	1114	rBV6	2866	5087	0.12%	0.013%
15	9.746	1124	1132	1141	rBV	599234	998095	22.85%	2.480%
16	10.281	1216	1223	1236	rBV	824207	1419867	32.50%	3.528%
17	10.658	1279	1287	1297	rBV	735223	1237885	28.34%	3.076%
18	10.810	1305	1313	1337	rBV	707923	1355936	31.04%	3.369%
19	12.252	1554	1558	1566	rVB2	16792	27964	0.64%	0.069%
20	13.134	1702	1708	1713	rBV4	5040	8237	0.19%	0.020%
21	13.410	1750	1755	1761	rBV2	14794	23427	0.54%	0.058%
22	13.481	1763	1767	1770	rBV6	3734	5700	0.13%	0.014%
23	13.928	1834	1843	1855	rBV	1751455	2425258	55.52%	6.026%
24	14.198	1882	1889	1902	rBV2	1939933	2846660	65.16%	7.074%
25	14.504	1935	1941	1949	rBV	942443	1394244	31.92%	3.464%
26	14.722	1973	1978	1990	rBV	50739	131972	3.02%	0.328%
27	15.310	2073	2078	2084	rBV	19913	29770	0.68%	0.074%
28	15.504	2103	2111	2125	rBV	2411126	3532603	80.86%	8.778%
29	15.628	2126	2132	2148	rVV	644037	909475	20.82%	2.260%
30	15.745	2148	2152	2156	rVB5	11099	16689	0.38%	0.041%
31	16.287	2241	2244	2248	rVB5	7958	11292	0.26%	0.028%
32	16.940	2352	2355	2359	rVB5	3594	4779	0.11%	0.012%
33	17.257	2402	2409	2417	rBV	1156263	1611790	36.89%	4.005%
34	17.357	2419	2426	2443	rVV	2635871	3809030	87.19%	9.465%
35	17.557	2457	2460	2465	rVB4	3076	4382	0.10%	0.011%
36	17.939	2518	2525	2531	rBV10	13449	22527	0.52%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029854.D
 Acq On : 19 Feb 2024 16:41
 Operator : MA/JU
 Sample : P1402-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	18.169	2559	2564	2571	rBV2	39442	58185	1.33%	0.145%
38	18.251	2574	2578	2582	rVB4	6024	7681	0.18%	0.019%
39	18.498	2615	2620	2623	rBV3	12752	20962	0.48%	0.052%
40	18.610	2635	2639	2642	rBV6	4446	8277	0.19%	0.021%
41	18.645	2642	2645	2651	rVB6	6857	11657	0.27%	0.029%
42	18.939	2693	2695	2699	rBV5	3911	5423	0.12%	0.013%
43	19.222	2738	2743	2749	rBV2	33564	48162	1.10%	0.120%
44	19.292	2751	2755	2760	rBV	30414	47113	1.08%	0.117%
45	19.457	2779	2783	2788	rBV3	22084	29936	0.69%	0.074%
46	19.610	2806	2809	2811	rBV4	9739	12128	0.28%	0.030%
47	19.657	2811	2817	2827	rVV	3193242	4368600	100.00%	10.855%
48	20.663	2986	2988	2992	rVB5	8900	8558	0.20%	0.021%
49	21.198	3076	3079	3084	rVB5	23235	29549	0.68%	0.073%
50	21.457	3118	3123	3135	rBV	1178030	1627865	37.26%	4.045%
51	23.674	3492	3500	3512	rBV2	2159053	4335524	99.24%	10.773%
52	23.827	3519	3526	3539	rVB	825479	1744745	39.94%	4.335%




Sum of corrected areas: 40243844

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029854.D
Acq On : 19 Feb 2024 16:41
Operator : MA/JU
Sample : P1402-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

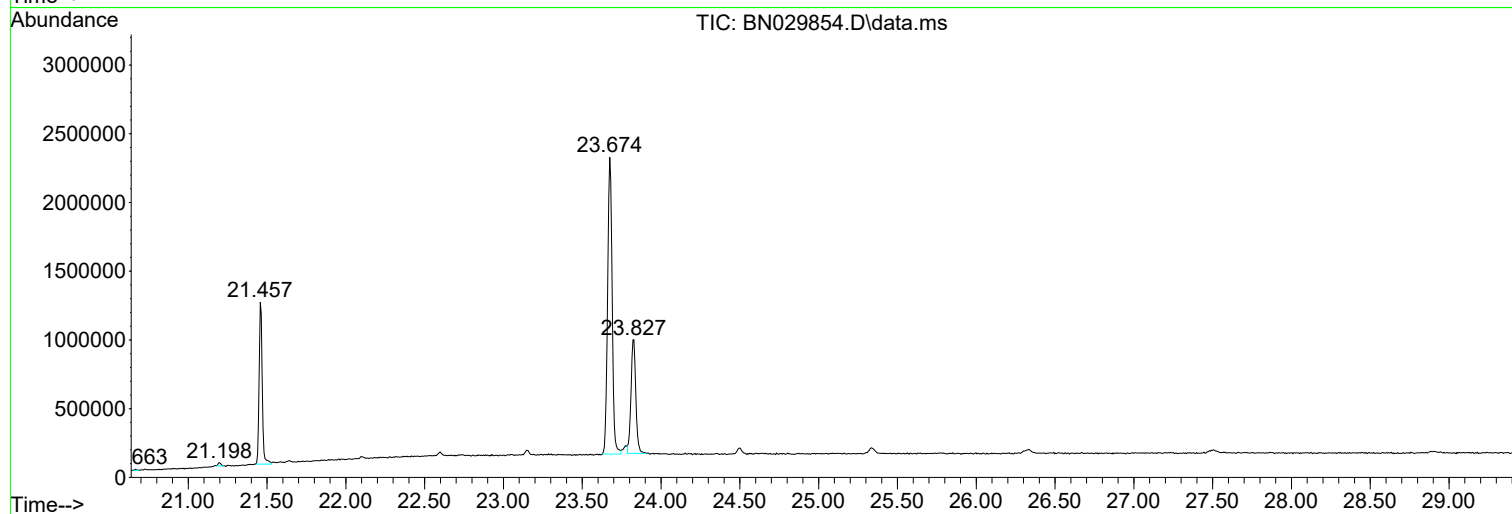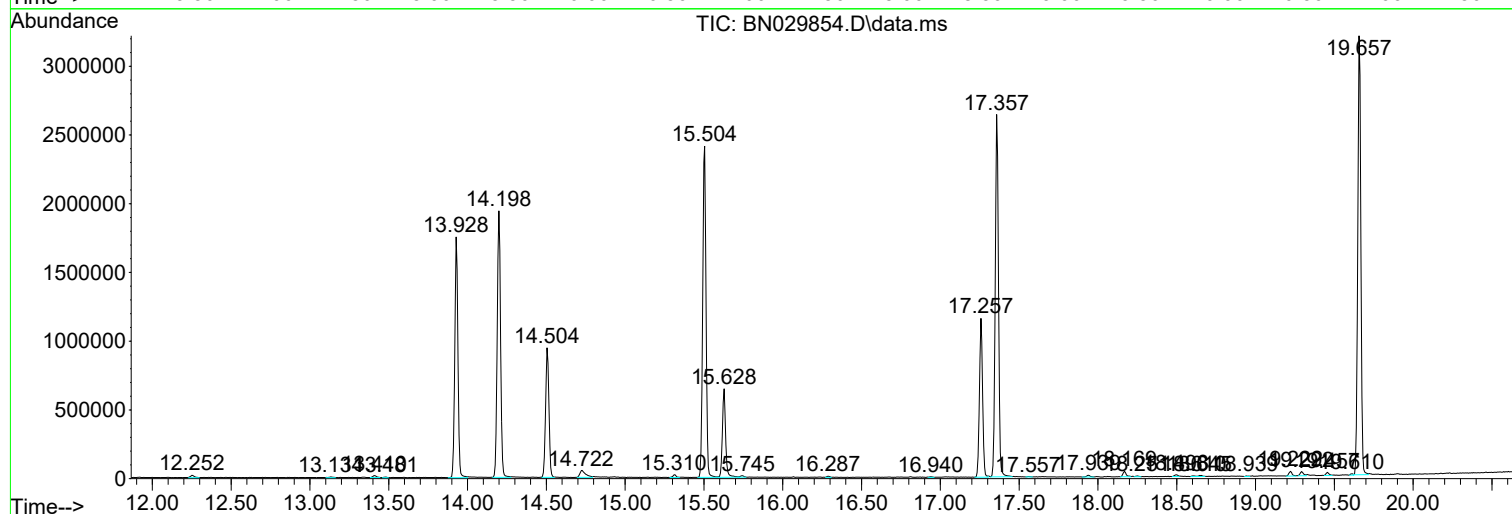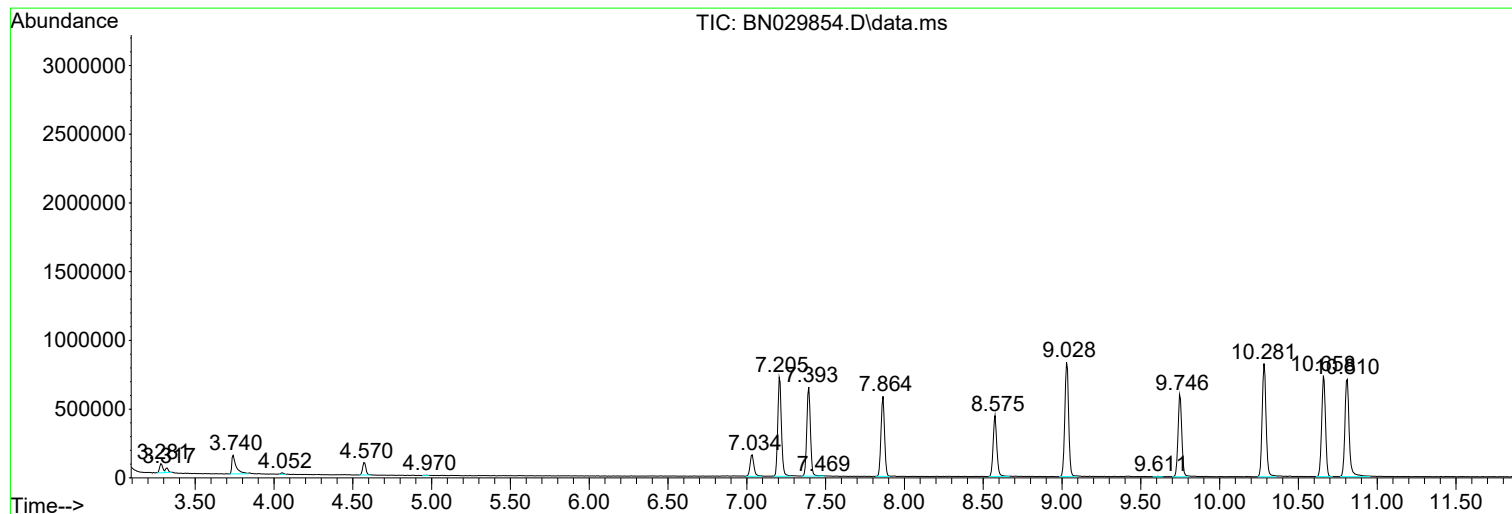

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029854.D
Acq On : 19 Feb 2024 16:41
Operator : MA/JU
Sample : P1402-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029854.D
Acq On : 19 Feb 2024 16:41
Operator : MA/JU
Sample : P1402-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc