

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029855.D
 Acq On : 19 Feb 2024 17:17
 Operator : MA/JU
 Sample : P1402-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	37	rBV	115171	156522	3.06%	0.346%
2	3.322	37	40	45	rVB	38988	52282	1.02%	0.116%
3	3.734	107	110	127	rBV	207755	385250	7.53%	0.853%
4	4.052	161	164	168	rVB2	12900	17352	0.34%	0.038%
5	4.569	248	252	259	rVB2	28430	43208	0.84%	0.096%
6	7.034	664	671	680	rBV	183825	299834	5.86%	0.664%
7	7.205	694	700	712	rBV	725779	1183573	23.13%	2.619%
8	7.393	725	732	742	rBV	718769	1150135	22.48%	2.545%
9	7.475	744	746	753	rVB7	6388	8658	0.17%	0.019%
10	7.863	803	812	821	rBV	602528	950448	18.57%	2.103%
11	8.575	926	933	946	rBV	535036	872093	17.04%	1.930%
12	9.028	1003	1010	1020	rBV	894500	1483763	29.00%	3.284%
13	9.746	1125	1132	1144	rBV	650100	1095825	21.42%	2.425%
14	10.281	1215	1223	1234	rBV	951340	1597637	31.22%	3.536%
15	10.657	1276	1287	1296	rBV	775365	1333734	26.06%	2.952%
16	10.810	1304	1313	1326	rBV	731461	1351808	26.42%	2.992%
17	12.251	1553	1558	1567	rBV2	17418	32367	0.63%	0.072%
18	13.134	1703	1708	1713	rVB6	5276	9044	0.18%	0.020%
19	13.410	1747	1755	1760	rBV4	13080	22192	0.43%	0.049%
20	13.928	1837	1843	1853	rBV	1811964	2539493	49.63%	5.620%
21	14.198	1881	1889	1900	rBV	2042123	3020421	59.03%	6.684%
22	14.504	1934	1941	1953	rBV	1040778	1575915	30.80%	3.488%
23	14.616	1956	1960	1966	rVB7	3558	6846	0.13%	0.015%
24	14.722	1972	1978	1990	rBV2	71753	184925	3.61%	0.409%
25	15.310	2074	2078	2085	rBV2	8602	13239	0.26%	0.029%
26	15.504	2104	2111	2126	rBV	2578399	3776532	73.80%	8.358%
27	15.628	2126	2132	2148	rVV	788492	1111302	21.72%	2.459%
28	15.745	2148	2152	2156	rVB5	10196	15612	0.31%	0.035%
29	16.198	2223	2229	2231	rBV6	3487	5263	0.10%	0.012%
30	16.292	2241	2245	2250	rVB6	9228	12823	0.25%	0.028%
31	17.257	2403	2409	2420	rBV	1303033	1881276	36.77%	4.163%
32	17.357	2420	2426	2442	rVV2	2926182	4380163	85.60%	9.693%
33	17.563	2458	2461	2467	rVB7	3953	7073	0.14%	0.016%
34	17.939	2519	2525	2530	rVB7	15065	22574	0.44%	0.050%
35	18.169	2559	2564	2570	rBV2	61220	88125	1.72%	0.195%
36	18.604	2634	2638	2641	rBV5	5922	7085	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029855.D
Acq On : 19 Feb 2024 17:17
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	18.751	2659	2663	2666	rBV5	5866	9475	0.19%	0.021%
38	19.222	2739	2743	2748	rBV2	37650	50236	0.98%	0.111%
39	19.292	2751	2755	2760	rBV	33034	48482	0.95%	0.107%
40	19.457	2778	2783	2788	rBV4	33030	47986	0.94%	0.106%
41	19.616	2806	2810	2811	rBV3	13375	14932	0.29%	0.033%
42	19.657	2811	2817	2826	rVV	3654959	5115432	99.97%	11.321%
43	19.904	2855	2859	2862	rBV4	8493	11932	0.23%	0.026%
44	21.198	3076	3079	3085	rVB4	38203	51259	1.00%	0.113%
45	21.463	3118	3124	3136	rBV	1456728	1977457	38.64%	4.376%
46	23.680	3493	3501	3513	rBV2	2607196	5116991	100.00%	11.324%
47	23.827	3519	3526	3534	rVB	994552	2048710	40.04%	4.534%




Sum of corrected areas: 45187284

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029855.D
Acq On : 19 Feb 2024 17:17
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

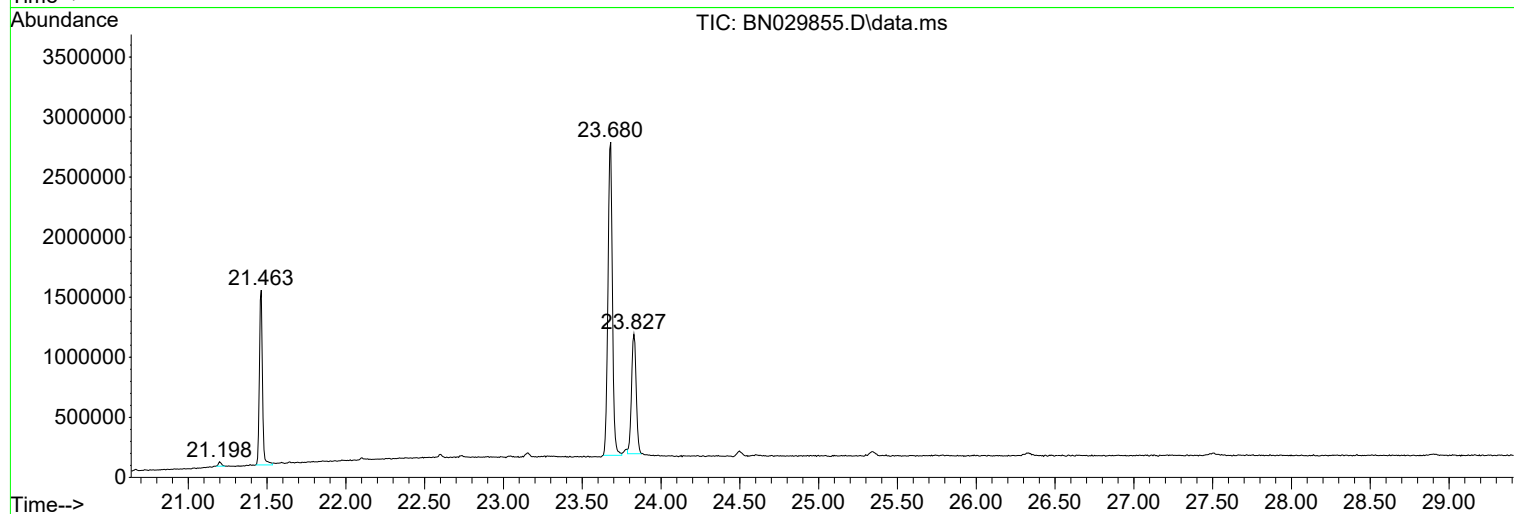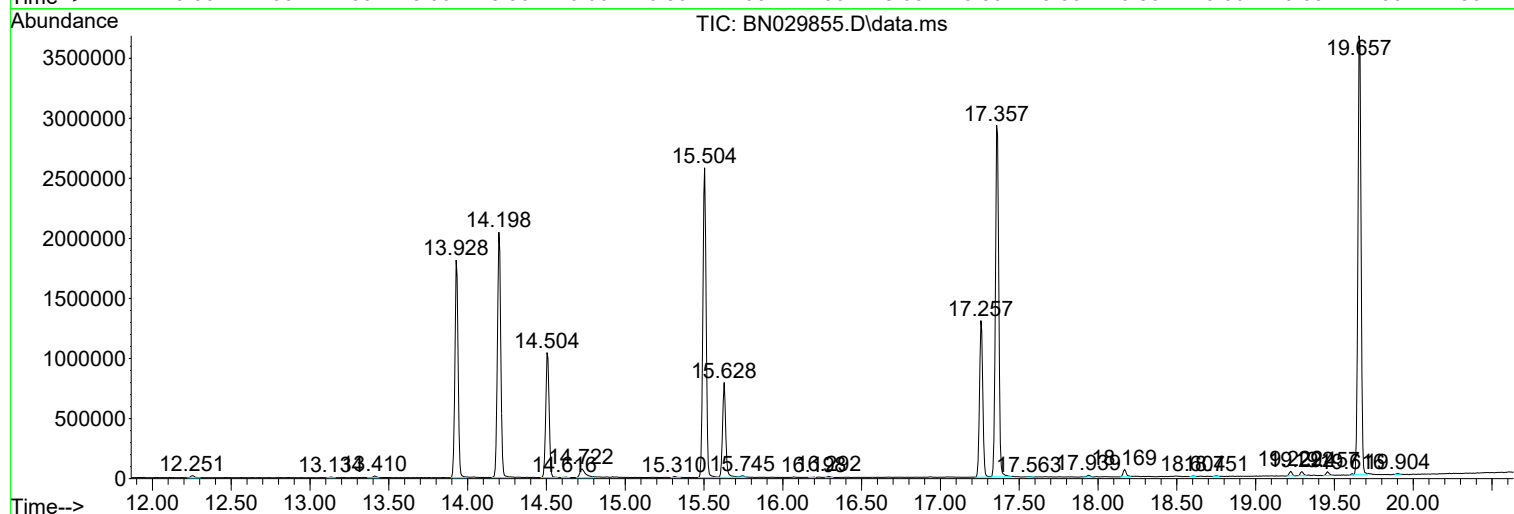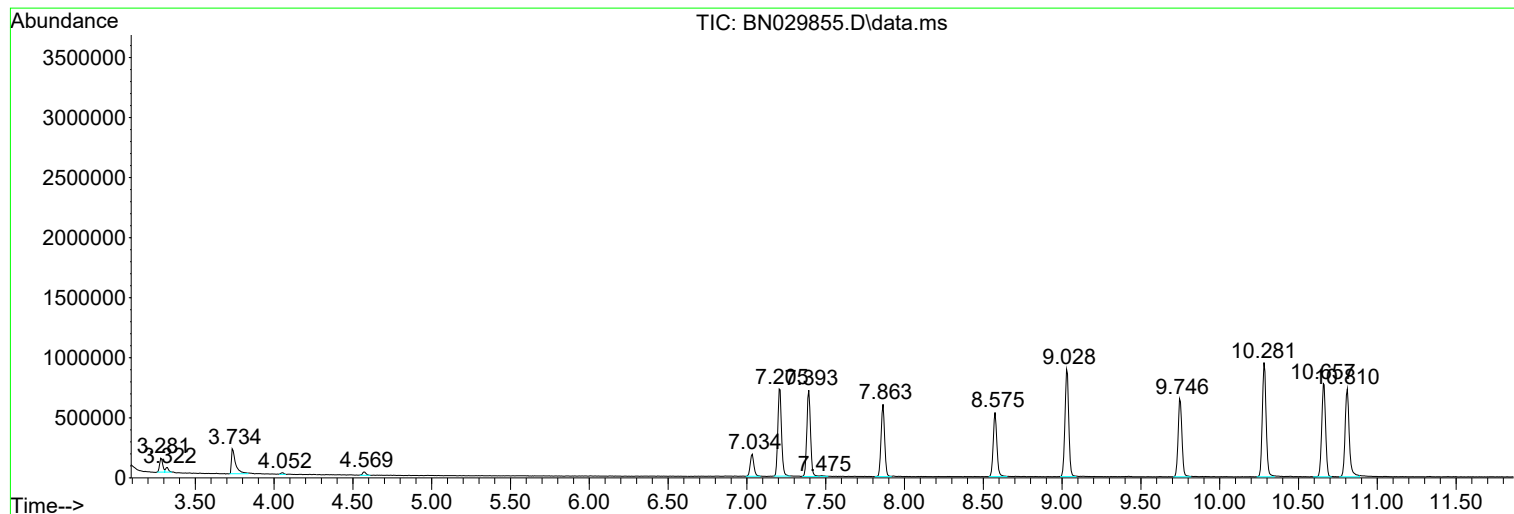

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029855.D
Acq On : 19 Feb 2024 17:17
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029855.D
Acq On : 19 Feb 2024 17:17
Operator : MA/JU
Sample : P1402-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------