

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029856.D
 Acq On : 19 Feb 2024 17:53
 Operator : MA/JU
 Sample : P1402-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	44	rBV	40134	51130	1.11%	0.119%
2	3.740	107	111	131	rBV	131088	269343	5.84%	0.627%
3	4.052	160	164	171	rVB4	13531	17740	0.38%	0.041%
4	5.522	409	414	420	rVB	34507	50858	1.10%	0.118%
5	7.034	664	671	679	rBV	186795	305055	6.61%	0.711%
6	7.205	694	700	712	rBV	714911	1140685	24.73%	2.657%
7	7.393	725	732	743	rBV	710393	1126421	24.42%	2.624%
8	7.863	805	812	822	rVB	661875	1047888	22.72%	2.441%
9	8.575	926	933	947	rBV	524924	861793	18.68%	2.007%
10	9.028	1002	1010	1021	rBV	837786	1396057	30.26%	3.252%
11	9.416	1071	1076	1079	rBV5	3778	5979	0.13%	0.014%
12	9.746	1123	1132	1141	rBV	623565	1054173	22.85%	2.455%
13	10.281	1214	1223	1240	rBV	910132	1544229	33.48%	3.597%
14	10.657	1279	1287	1297	rVB	832541	1449547	31.42%	3.376%
15	10.804	1304	1312	1329	rBV	721434	1352206	29.31%	3.149%
16	12.251	1552	1558	1565	rBV2	15409	26415	0.57%	0.062%
17	13.140	1703	1709	1713	rVB5	3072	6363	0.14%	0.015%
18	13.410	1748	1755	1761	rBV3	14004	25330	0.55%	0.059%
19	13.475	1761	1766	1772	rVB6	2226	4705	0.10%	0.011%
20	13.928	1836	1843	1855	rBV	1660075	2327149	50.45%	5.420%
21	14.198	1882	1889	1903	rBV2	1917920	2806844	60.85%	6.537%
22	14.504	1934	1941	1950	rBV	1141870	1697284	36.79%	3.953%
23	14.722	1971	1978	1992	rBV3	67091	183987	3.99%	0.429%
24	15.310	2074	2078	2081	rBV3	3724	5193	0.11%	0.012%
25	15.504	2104	2111	2125	rBV	2404766	3476381	75.36%	8.097%
26	15.628	2125	2132	2146	rVV	741025	1040023	22.55%	2.422%
27	15.740	2148	2151	2161	rVB5	12722	21886	0.47%	0.051%
28	16.287	2241	2244	2248	rVB4	7089	9025	0.20%	0.021%
29	17.257	2400	2409	2419	rBV	1379688	1960492	42.50%	4.566%
30	17.357	2419	2426	2443	rVB2	2893737	4093006	88.73%	9.533%
31	17.939	2520	2525	2530	rBV7	6834	10138	0.22%	0.024%
32	18.169	2559	2564	2570	rBV2	32278	45305	0.98%	0.106%
33	18.498	2616	2620	2628	rVB9	4743	7987	0.17%	0.019%
34	19.222	2738	2743	2748	rBV2	32377	45269	0.98%	0.105%
35	19.292	2748	2755	2760	rBV	29811	46028	1.00%	0.107%
36	19.457	2777	2783	2788	rBV7	15885	28164	0.61%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029856.D
Acq On : 19 Feb 2024 17:53
Operator : MA/JU
Sample : P1402-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.610	2806	2809	2811	rBV3	11703	12462	0.27%	0.029%
38	19.657	2811	2817	2826	rVV2	3439638	4612918	100.00%	10.744%
39	21.463	3118	3124	3136	rBV2	1436377	2039701	44.22%	4.751%
40	23.674	3492	3500	3512	rBV2	2263727	4572137	99.12%	10.649%
41	23.827	3519	3526	3541	rVB	1045111	2157682	46.77%	5.025%




Sum of corrected areas: 42934978

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029856.D
Acq On : 19 Feb 2024 17:53
Operator : MA/JU
Sample : P1402-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

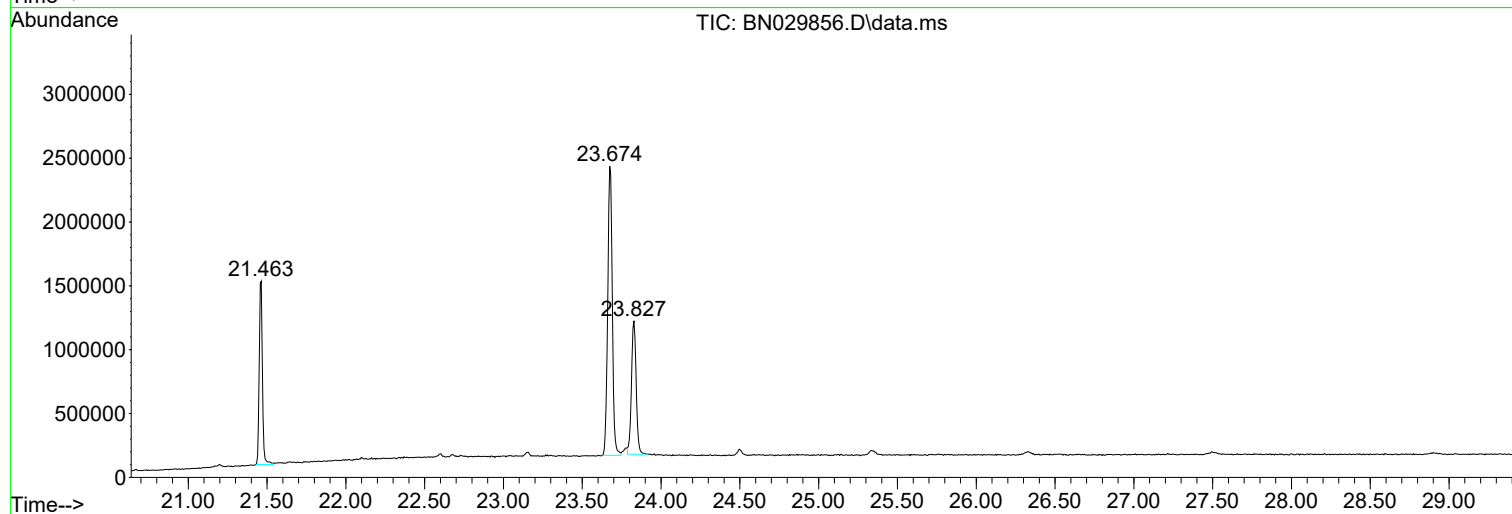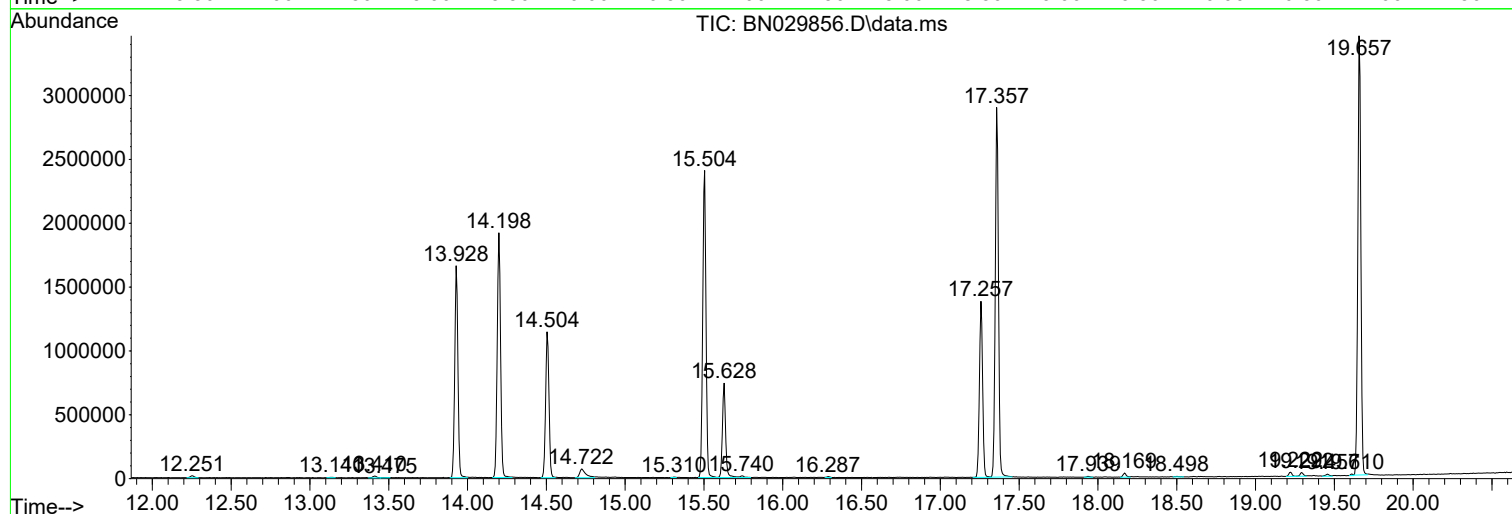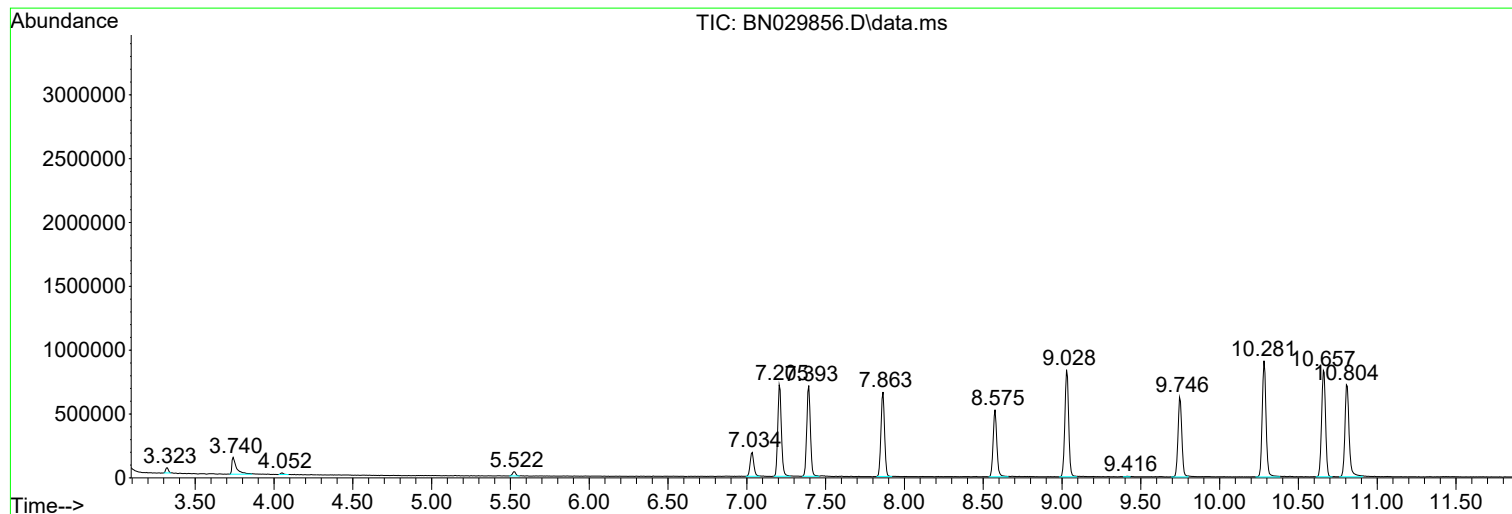

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029856.D
Acq On : 19 Feb 2024 17:53
Operator : MA/JU
Sample : P1402-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029856.D
Acq On : 19 Feb 2024 17:53
Operator : MA/JU
Sample : P1402-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc