

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029857.D
 Acq On : 19 Feb 2024 18:29
 Operator : MA/JU
 Sample : P1402-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	31	33	36	rVV3	7552	6696	0.16%	0.017%
2	3.322	36	40	47	rVB	34357	48976	1.14%	0.127%
3	3.740	107	111	124	rBV	118471	231402	5.41%	0.602%
4	4.052	161	164	171	rVB	12655	18495	0.43%	0.048%
5	4.569	248	252	258	rVB4	10170	15790	0.37%	0.041%
6	4.787	287	289	294	rVB7	2826	4476	0.10%	0.012%
7	7.034	662	671	678	rBV	140763	230339	5.38%	0.599%
8	7.205	694	700	713	rBV	677445	1089184	25.45%	2.831%
9	7.393	725	732	743	rBV	620225	996008	23.27%	2.589%
10	7.487	747	748	753	rVB5	4141	5083	0.12%	0.013%
11	7.863	805	812	821	rBV	588647	918064	21.45%	2.387%
12	8.575	926	933	945	rBV	420142	696793	16.28%	1.811%
13	9.028	1001	1010	1020	rBV	791075	1312130	30.66%	3.411%
14	9.622	1108	1111	1118	rVB8	3526	5350	0.13%	0.014%
15	9.746	1123	1132	1145	rBV	570925	971732	22.70%	2.526%
16	10.281	1214	1223	1239	rBV	805134	1380967	32.27%	3.590%
17	10.657	1280	1287	1297	rVB	743232	1253127	29.28%	3.258%
18	10.810	1305	1313	1332	rBV	602651	1163408	27.18%	3.024%
19	11.422	1413	1417	1423	rBV5	6077	11326	0.26%	0.029%
20	12.251	1553	1558	1564	rBV2	14015	22489	0.53%	0.058%
21	13.128	1701	1707	1710	rBV9	2999	4409	0.10%	0.011%
22	13.328	1736	1741	1743	rBV4	3275	4666	0.11%	0.012%
23	13.410	1749	1755	1761	rBV2	15981	26320	0.61%	0.068%
24	13.928	1837	1843	1855	rBV	1536002	2160173	50.47%	5.616%
25	14.198	1880	1889	1899	rBV	1755713	2559107	59.79%	6.653%
26	14.351	1913	1915	1920	rVB5	2744	4480	0.10%	0.012%
27	14.504	1934	1941	1951	rBV	942905	1433870	33.50%	3.728%
28	14.728	1973	1979	1993	rBV2	43045	120650	2.82%	0.314%
29	15.310	2074	2078	2082	rBV	7469	11157	0.26%	0.029%
30	15.504	2104	2111	2118	rBV	2168134	3153072	73.67%	8.197%
31	15.628	2125	2132	2147	rBV	627815	894850	20.91%	2.326%
32	15.739	2148	2151	2158	rVB5	10255	16178	0.38%	0.042%
33	15.892	2172	2177	2180	rVB6	3447	5871	0.14%	0.015%
34	16.228	2231	2234	2241	rBV5	2852	5291	0.12%	0.014%
35	16.292	2241	2245	2249	rVB5	6210	8829	0.21%	0.023%
36	17.039	2368	2372	2375	rBV5	3847	5625	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029857.D
 Acq On : 19 Feb 2024 18:29
 Operator : MA/JU
 Sample : P1402-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.257	2402	2409	2420	rBV	1135102	1635963	38.22%	4.253%
38	17.357	2420	2426	2438	rBV2	2499334	3691155	86.25%	9.596%
39	17.563	2456	2461	2464	rVB3	4924	7325	0.17%	0.019%
40	17.775	2493	2497	2500	rBV6	2801	4884	0.11%	0.013%
41	17.939	2522	2525	2531	rVB7	8131	10225	0.24%	0.027%
42	18.169	2559	2564	2572	rVV2	68415	103861	2.43%	0.270%
43	18.239	2574	2576	2581	rVB2	8585	13499	0.32%	0.035%
44	18.604	2635	2638	2643	rVB7	7593	8452	0.20%	0.022%
45	18.645	2643	2645	2652	rBV8	4858	9750	0.23%	0.025%
46	19.222	2739	2743	2749	rVB3	29546	42083	0.98%	0.109%
47	19.292	2750	2755	2759	rBV	28974	41940	0.98%	0.109%
48	19.339	2759	2763	2766	rVV5	5296	8675	0.20%	0.023%
49	19.457	2778	2783	2791	rBV4	39490	61596	1.44%	0.160%
50	19.610	2806	2809	2811	rBV4	10092	8717	0.20%	0.023%
51	19.657	2811	2817	2826	rVV	3087321	4279834	100.00%	11.126%
52	21.198	3076	3079	3088	rVB7	38608	58240	1.36%	0.151%
53	21.463	3118	3124	3140	rBV	1222959	1717648	40.13%	4.465%
54	23.674	3493	3500	3512	rBV2	2103911	4204356	98.24%	10.930%
55	23.827	3520	3526	3537	rVB	844034	1762392	41.18%	4.582%




Sum of corrected areas: 38466978

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029857.D
Acq On : 19 Feb 2024 18:29
Operator : MA/JU
Sample : P1402-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

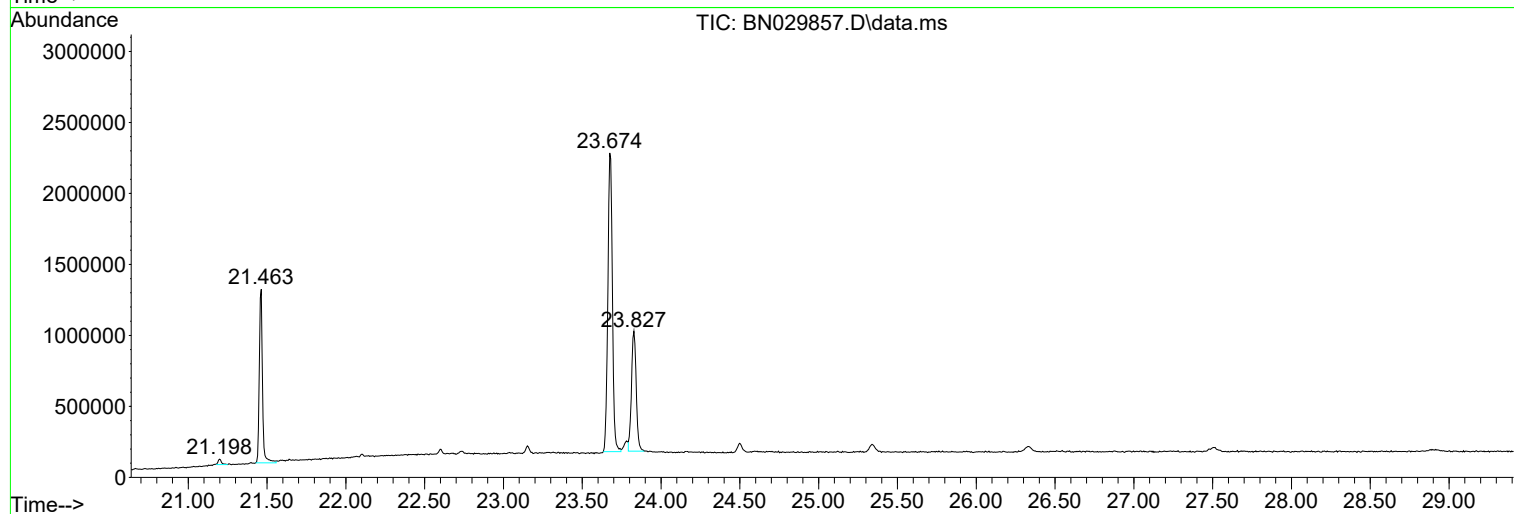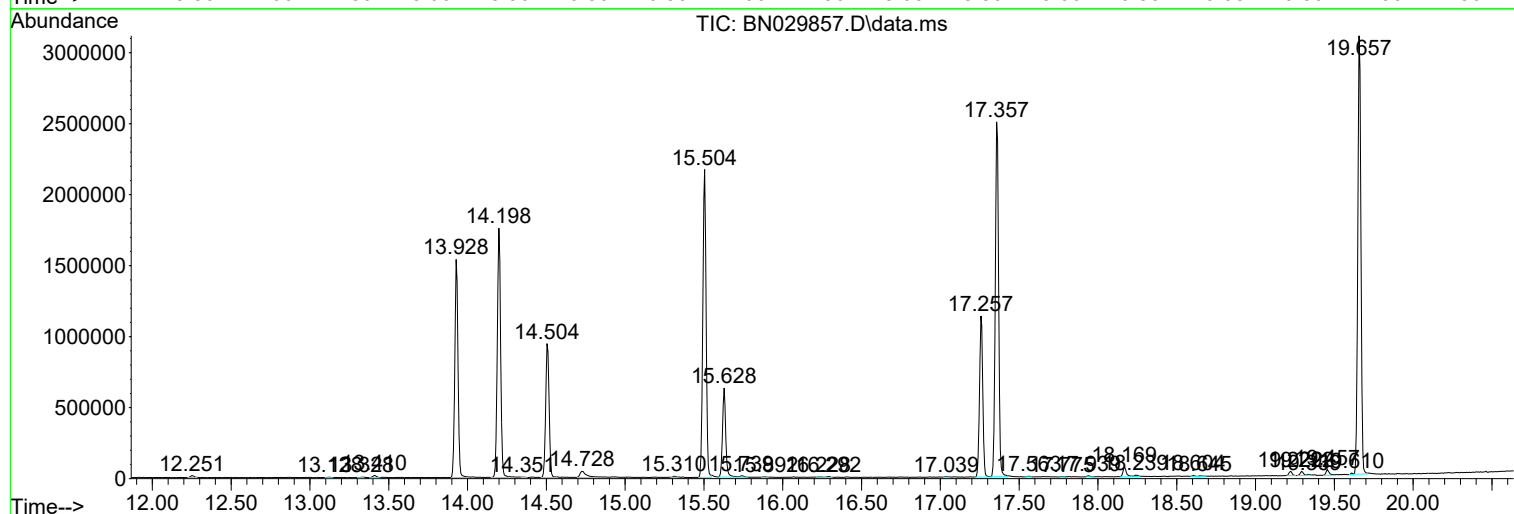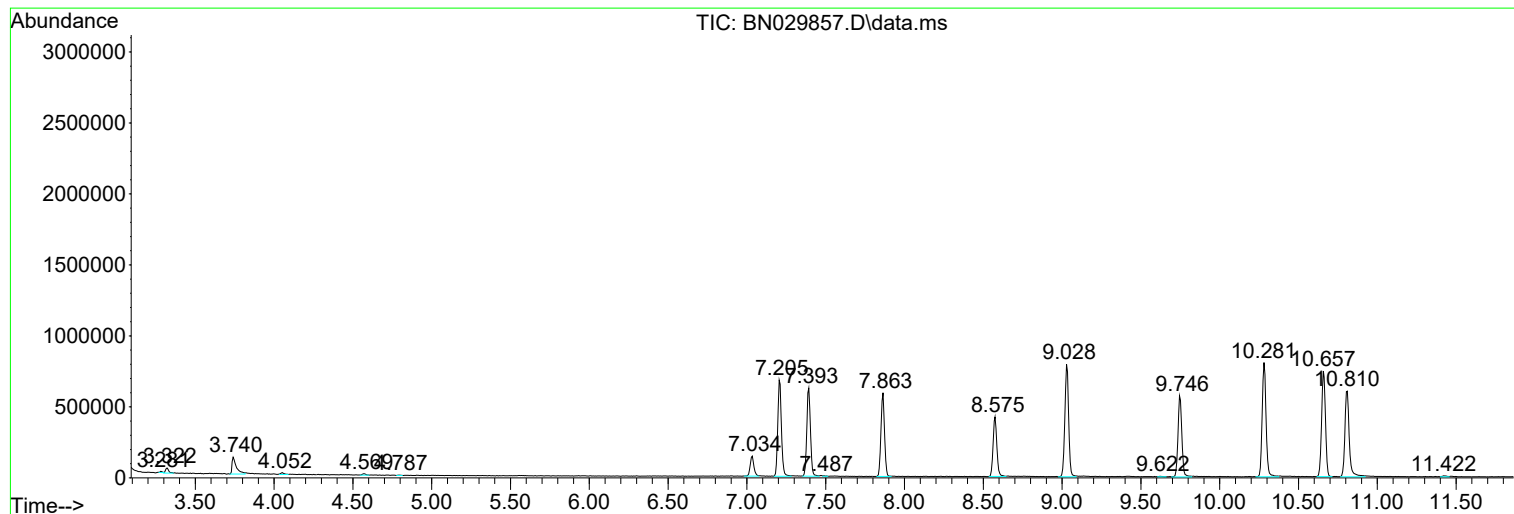

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029857.D
Acq On : 19 Feb 2024 18:29
Operator : MA/JU
Sample : P1402-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029857.D
Acq On : 19 Feb 2024 18:29
Operator : MA/JU
Sample : P1402-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc