

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029859.D
 Acq On : 19 Feb 2024 19:41
 Operator : MA/JU
 Sample : P1402-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	38	rBV	274836	397374	8.34%	0.892%
2	3.317	38	39	42	rVV	51358	52245	1.10%	0.117%
3	3.352	42	45	56	rVB	111138	154910	3.25%	0.348%
4	3.734	107	110	133	rBV	170838	347722	7.29%	0.781%
5	4.052	161	164	168	rVB2	12878	17238	0.36%	0.039%
6	4.164	180	183	187	rVB4	13713	16690	0.35%	0.037%
7	4.570	246	252	267	rVB	992179	1492511	31.31%	3.352%
8	7.034	664	671	679	rVB	172436	290256	6.09%	0.652%
9	7.205	694	700	714	rBV	691712	1128639	23.68%	2.535%
10	7.393	725	732	744	rBV	679098	1075974	22.57%	2.417%
11	7.475	744	746	750	rVB6	5111	6639	0.14%	0.015%
12	7.863	803	812	820	rBV	578147	927098	19.45%	2.082%
13	8.575	926	933	945	rBV	473285	778520	16.33%	1.748%
14	9.028	1003	1010	1021	rBV	823439	1378691	28.92%	3.096%
15	9.140	1025	1029	1034	rVB5	5813	10615	0.22%	0.024%
16	9.193	1034	1038	1042	rBV6	3269	5091	0.11%	0.011%
17	9.469	1079	1085	1095	rVB	51632	93419	1.96%	0.210%
18	9.610	1104	1109	1113	rBV7	4857	7397	0.16%	0.017%
19	9.746	1125	1132	1144	rBV	606957	1038622	21.79%	2.333%
20	10.081	1184	1189	1194	rBV7	10840	16988	0.36%	0.038%
21	10.281	1216	1223	1238	rBV	882856	1495588	31.37%	3.359%
22	10.657	1280	1287	1295	rBV	778590	1289862	27.06%	2.897%
23	10.805	1305	1312	1327	rBV	654840	1240389	26.02%	2.786%
24	10.916	1327	1331	1336	rVV6	20382	39445	0.83%	0.089%
25	10.963	1338	1339	1343	rVB4	5820	6620	0.14%	0.015%
26	11.075	1350	1358	1364	rBV8	20766	54139	1.14%	0.122%
27	11.228	1378	1384	1391	rVB9	11395	27816	0.58%	0.062%
28	11.416	1410	1416	1419	rBV6	7823	14795	0.31%	0.033%
29	11.469	1419	1425	1427	rVV3	20599	35752	0.75%	0.080%
30	11.493	1427	1429	1437	rVB	23412	38707	0.81%	0.087%
31	11.563	1437	1441	1445	rBV6	10439	17498	0.37%	0.039%
32	11.610	1445	1449	1454	rVV4	8431	12094	0.25%	0.027%
33	12.251	1550	1558	1564	rBV2	17264	28292	0.59%	0.064%
34	13.334	1739	1742	1746	rVB5	5741	7928	0.17%	0.018%
35	13.410	1751	1755	1760	rBV3	11992	22212	0.47%	0.050%
36	13.928	1836	1843	1857	rBV	1705715	2332084	48.92%	5.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029859.D
 Acq On : 19 Feb 2024 19:41
 Operator : MA/JU
 Sample : P1402-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	14.198	1879	1889	1902	rBV	1834275	2762869	57.96%	6.205%
38	14.416	1920	1926	1930	rVB6	9303	14061	0.29%	0.032%
39	14.504	1934	1941	1950	rBV	1009186	1498329	31.43%	3.365%
40	14.722	1970	1978	1991	rBV2	75024	187547	3.93%	0.421%
41	14.887	2000	2006	2010	rBV8	3736	8538	0.18%	0.019%
42	15.034	2028	2031	2035	rVB5	3953	5245	0.11%	0.012%
43	15.240	2062	2066	2070	rBV7	4063	6241	0.13%	0.014%
44	15.316	2073	2079	2082	rVV	20675	30070	0.63%	0.068%
45	15.363	2085	2087	2091	rVB3	13874	16455	0.35%	0.037%
46	15.504	2104	2111	2125	rVB	2331560	3417691	71.70%	7.676%
47	15.628	2125	2132	2144	rBV	698623	982023	20.60%	2.206%
48	15.740	2147	2151	2156	rVV5	12728	21809	0.46%	0.049%
49	15.875	2171	2174	2179	rBV8	5986	8960	0.19%	0.020%
50	15.928	2179	2183	2189	rVB9	3262	5818	0.12%	0.013%
51	16.204	2225	2230	2231	rBV5	3512	5409	0.11%	0.012%
52	16.234	2231	2235	2241	rVV3	19798	32020	0.67%	0.072%
53	16.287	2241	2244	2250	rVB6	9374	12685	0.27%	0.028%
54	16.804	2328	2332	2337	rBV7	6017	8396	0.18%	0.019%
55	16.928	2350	2353	2359	rBV7	3546	5960	0.13%	0.013%
56	17.028	2366	2370	2375	rBV3	24616	34074	0.71%	0.077%
57	17.081	2375	2379	2383	rVB6	6426	9527	0.20%	0.021%
58	17.257	2402	2409	2419	rBV	1225996	1758223	36.88%	3.949%
59	17.357	2419	2426	2440	rVV	2718518	3860019	80.97%	8.669%
60	17.563	2456	2461	2466	rVB4	6072	11560	0.24%	0.026%
61	17.769	2493	2496	2501	rBV2	17613	23915	0.50%	0.054%
62	17.939	2520	2525	2532	rVB8	24598	35427	0.74%	0.080%
63	17.998	2532	2535	2540	rBV7	3475	5742	0.12%	0.013%
64	18.169	2559	2564	2569	rBV	96798	131495	2.76%	0.295%
65	18.245	2575	2577	2584	rVB3	8141	11441	0.24%	0.026%
66	18.469	2612	2615	2618	rBV3	12853	15192	0.32%	0.034%
67	18.604	2636	2638	2642	rVB5	6267	7109	0.15%	0.016%
68	18.651	2642	2646	2649	rBV6	6097	10363	0.22%	0.023%
69	19.022	2707	2709	2712	rBV3	8346	11471	0.24%	0.026%
70	19.104	2720	2723	2731	rVB7	11503	17408	0.37%	0.039%
71	19.222	2738	2743	2748	rBV2	33546	50256	1.05%	0.113%
72	19.292	2751	2755	2759	rBV2	32092	53902	1.13%	0.121%
73	19.333	2760	2762	2767	rVB5	17491	21768	0.46%	0.049%
74	19.457	2779	2783	2788	rBV2	61277	84801	1.78%	0.190%
75	19.604	2806	2808	2811	rBV4	8770	9767	0.20%	0.022%
76	19.657	2811	2817	2826	rBV	3499980	4729832	99.22%	10.623%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029859.D
Acq On : 19 Feb 2024 19:41
Operator : MA/JU
Sample : P1402-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

77	20.410	2942	2945	2951	rBV2	30422	41179	0.86%	0.092%
78	21.198	3076	3079	3085	rVB4	48417	67985	1.43%	0.153%
79	21.392	3110	3112	3116	rVB	19942	23444	0.49%	0.053%
80	21.457	3118	3123	3137	rBV	1402315	1886096	39.57%	4.236%
81	23.674	3492	3500	3512	rBV	2367929	4766985	100.00%	10.706%
82	23.827	3519	3526	3536	rVB	938700	1916532	40.20%	4.304%




Sum of corrected areas: 44525499

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029859.D
Acq On : 19 Feb 2024 19:41
Operator : MA/JU
Sample : P1402-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

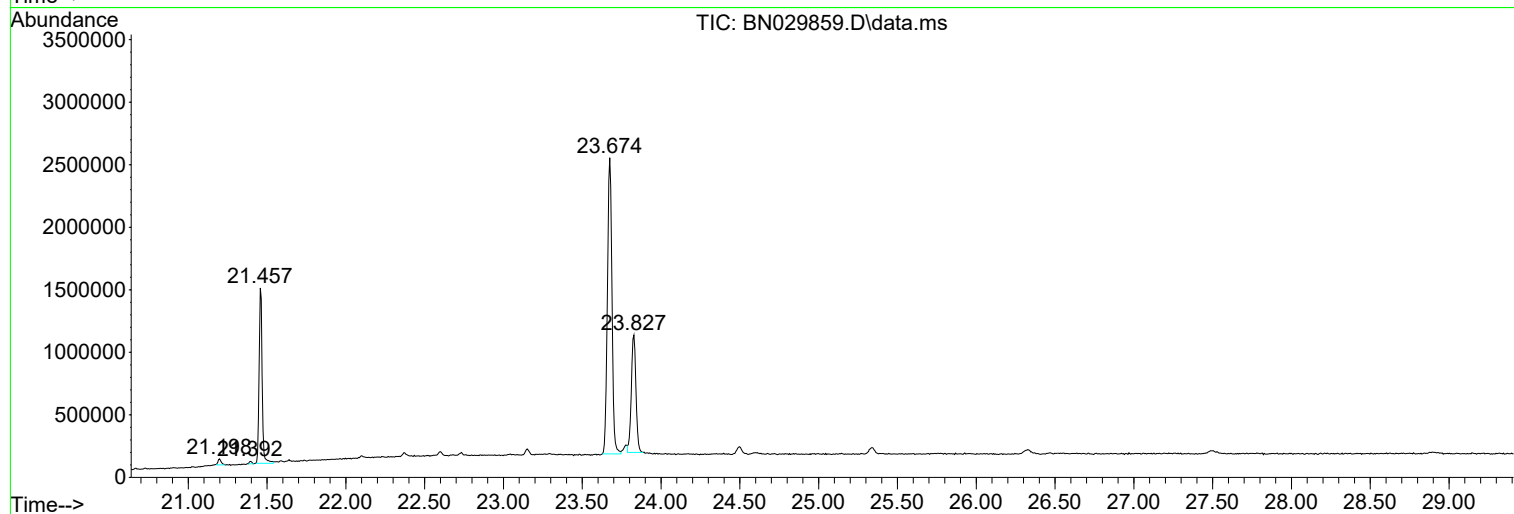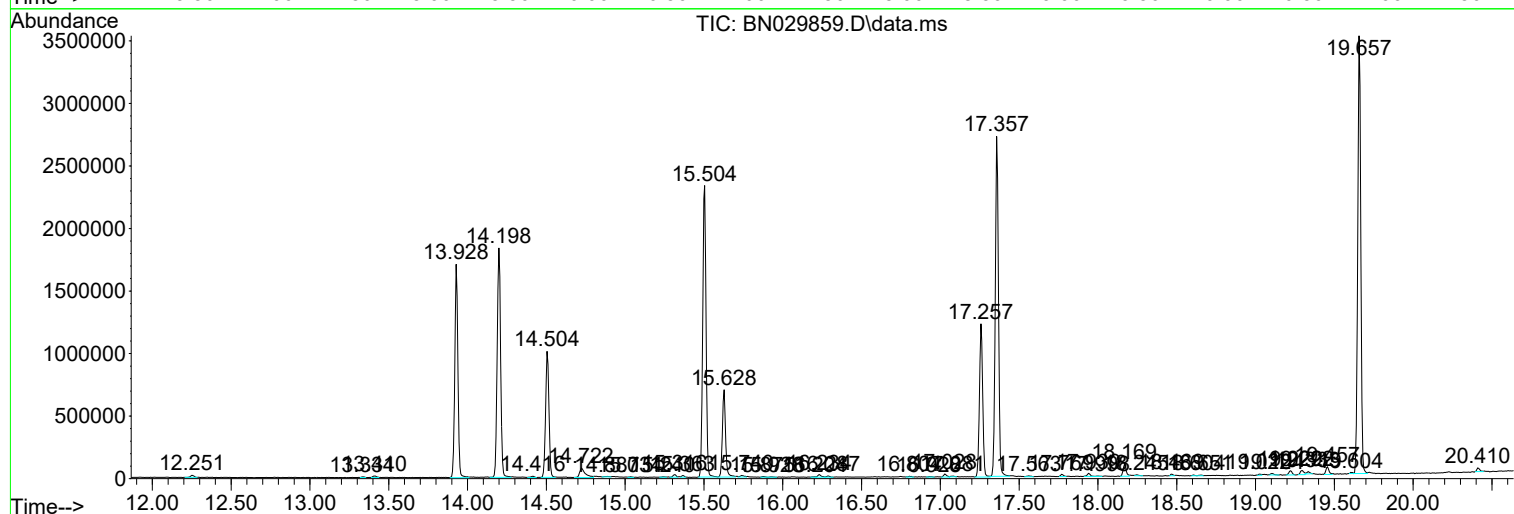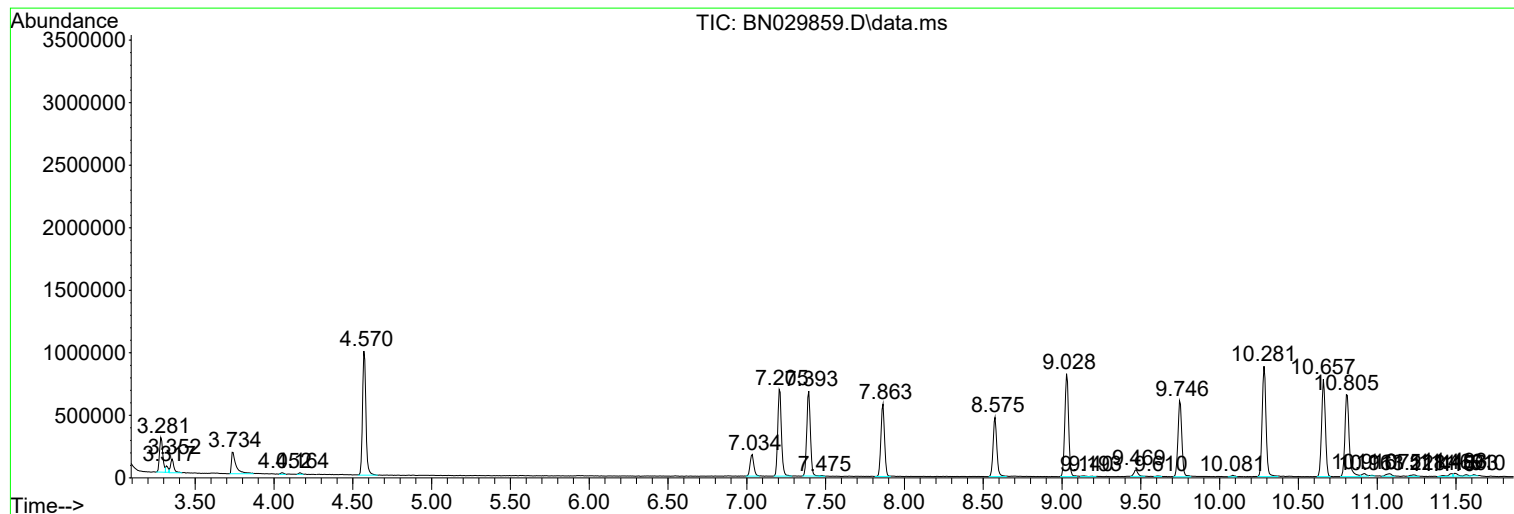

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029859.D
Acq On : 19 Feb 2024 19:41
Operator : MA/JU
Sample : P1402-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029859.D
Acq On : 19 Feb 2024 19:41
Operator : MA/JU
Sample : P1402-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------