

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029861.D
 Acq On : 19 Feb 2024 21:29
 Operator : MA/JU
 Sample : PB159013BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	46	rBV	58353	71301	1.95%	0.175%
2	3.728	106	109	133	rBV	620431	1043724	28.57%	2.555%
3	4.046	160	163	169	rVB2	10285	14718	0.40%	0.036%
4	7.028	664	670	685	rBV	842012	1362953	37.31%	3.336%
5	7.205	694	700	712	rBV	675121	1063983	29.12%	2.604%
6	7.393	725	732	740	rBV	852105	1363741	37.33%	3.338%
7	7.863	804	812	821	rVB	574045	911260	24.94%	2.231%
8	8.575	924	933	944	rBV	989062	1616192	44.24%	3.956%
9	8.769	965	966	972	rVB5	2625	3761	0.10%	0.009%
10	9.028	1003	1010	1022	rBV	787989	1301197	35.61%	3.185%
11	9.746	1122	1132	1145	rBV	615562	1030719	28.21%	2.523%
12	10.281	1215	1223	1236	rBV	912555	1559184	42.68%	3.816%
13	10.657	1280	1287	1296	rVB	761505	1271485	34.80%	3.112%
14	10.805	1304	1312	1329	rBV	859591	1573357	43.06%	3.851%
15	11.593	1440	1446	1450	rVB5	2264	4707	0.13%	0.012%
16	12.257	1554	1559	1566	rVB2	14143	24490	0.67%	0.060%
17	13.404	1751	1754	1759	rVB3	12560	19765	0.54%	0.048%
18	13.475	1762	1766	1768	rBV5	2803	3882	0.11%	0.010%
19	13.928	1836	1843	1856	rBV	1503309	2086546	57.11%	5.107%
20	14.198	1882	1889	1907	rBV	1719735	2542319	69.59%	6.223%
21	14.504	1934	1941	1949	rBV	998788	1468075	40.18%	3.593%
22	14.716	1970	1977	1995	rBV	450337	939607	25.72%	2.300%
23	14.975	2019	2021	2028	rVB6	2346	3794	0.10%	0.009%
24	15.498	2104	2110	2125	rBV	2064401	3057330	83.68%	7.484%
25	15.628	2125	2132	2144	rVV	536904	796894	21.81%	1.951%
26	15.740	2146	2151	2157	rVB7	9105	16923	0.46%	0.041%
27	16.292	2240	2245	2250	rVB6	6074	9264	0.25%	0.023%
28	16.734	2318	2320	2323	rBV3	3746	5781	0.16%	0.014%
29	17.039	2368	2372	2378	rVB7	2652	5122	0.14%	0.013%
30	17.257	2402	2409	2420	rBV	1166102	1684436	46.10%	4.123%
31	17.357	2420	2426	2444	rVB	2375489	3310590	90.61%	8.103%
32	19.222	2738	2743	2750	rVB3	25243	35804	0.98%	0.088%
33	19.292	2750	2755	2760	rBV2	22379	34230	0.94%	0.084%
34	19.657	2811	2817	2826	rBV2	2664319	3653535	100.00%	8.943%
35	20.157	2899	2902	2904	rBV4	5237	6001	0.16%	0.015%
36	21.457	3118	3123	3134	rBV2	1294389	1695080	46.40%	4.149%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029861.D
Acq On : 19 Feb 2024 21:29
Operator : MA/JU
Sample : PB159013BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK013

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.669	3492	3499	3510	rBV2	1751466	3532681	96.69%	8.647%
38	23.821	3519	3525	3534	rVB2	857744	1729419	47.34%	4.233%




Sum of corrected areas: 40853850

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029861.D
Acq On : 19 Feb 2024 21:29
Operator : MA/JU
Sample : PB159013BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

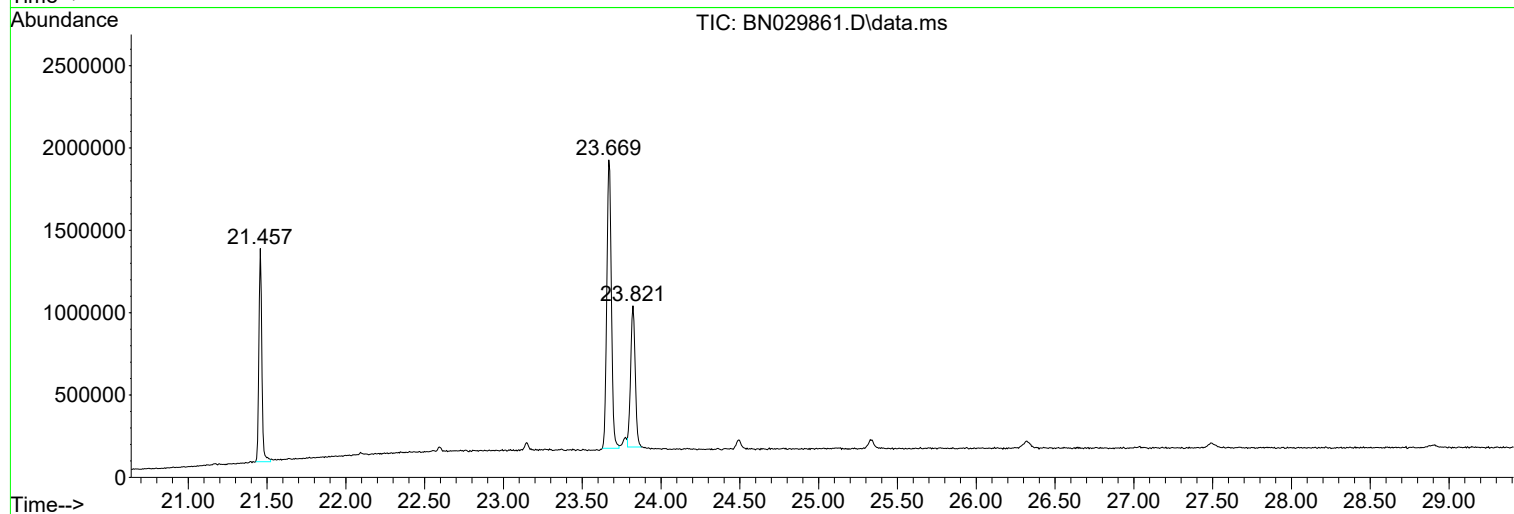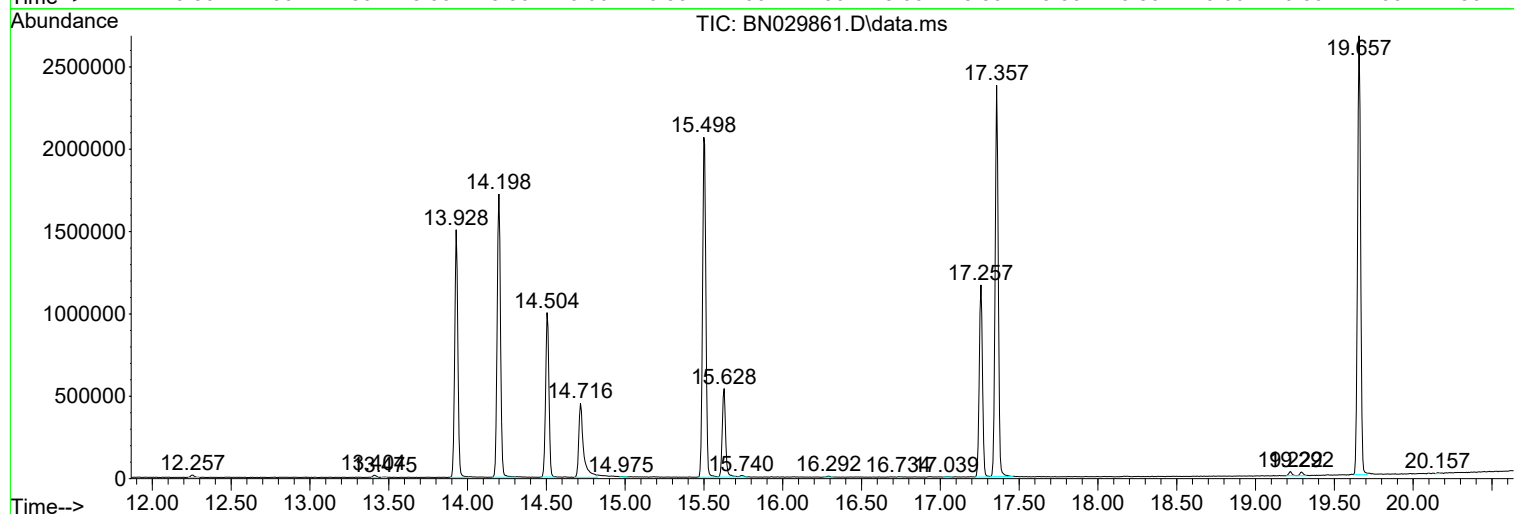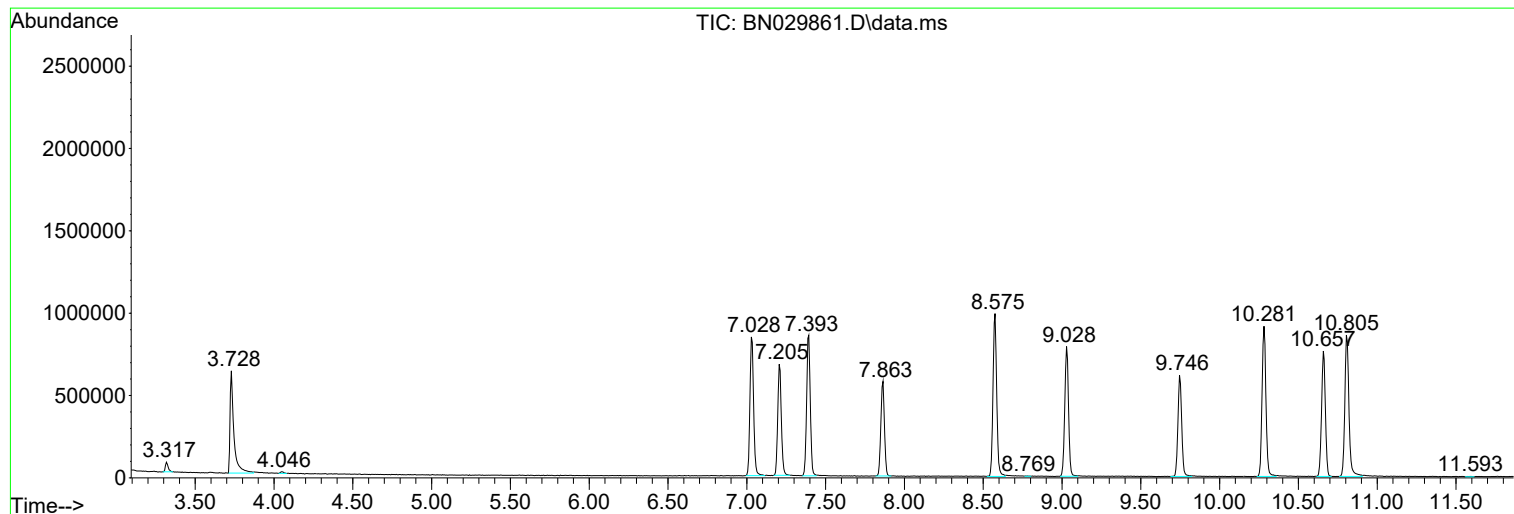

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029861.D
Acq On : 19 Feb 2024 21:29
Operator : MA/JU
Sample : PB159013BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029861.D
Acq On : 19 Feb 2024 21:29
Operator : MA/JU
Sample : PB159013BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------