

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029863.D
 Acq On : 19 Feb 2024 22:41
 Operator : MA/JU
 Sample : P1402-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	36	rBV4	16988	19730	0.45%	0.046%
2	3.317	36	39	43	rVB	36326	40879	0.92%	0.096%
3	3.734	106	110	128	rBV	247824	445919	10.08%	1.043%
4	4.052	160	164	168	rVB2	10490	13622	0.31%	0.032%
5	4.569	247	252	261	rVB	74683	109467	2.48%	0.256%
6	5.569	419	422	426	rVB7	4135	6284	0.14%	0.015%
7	7.028	663	670	680	rBV	181903	302521	6.84%	0.708%
8	7.205	694	700	712	rBV	815784	1292791	29.23%	3.024%
9	7.393	724	732	743	rBV	770958	1246649	28.19%	2.916%
10	7.863	805	812	822	rBV	552415	885442	20.02%	2.071%
11	8.575	926	933	943	rBV2	531122	893781	20.21%	2.091%
12	9.028	1003	1010	1024	rBV	961873	1575811	35.63%	3.686%
13	9.140	1024	1029	1032	rVB7	2850	4711	0.11%	0.011%
14	9.416	1073	1076	1081	rBV5	4078	6920	0.16%	0.016%
15	9.604	1103	1108	1115	rBV2	37677	66615	1.51%	0.156%
16	9.746	1125	1132	1141	rBV	721492	1186440	26.82%	2.775%
17	10.281	1215	1223	1240	rBV	1021850	1736159	39.25%	4.061%
18	10.451	1249	1252	1255	rVB5	3501	5357	0.12%	0.013%
19	10.657	1280	1287	1301	rVB	734453	1227165	27.75%	2.870%
20	10.804	1304	1312	1334	rBV	750511	1407170	31.82%	3.292%
21	11.328	1396	1401	1408	rVB9	3044	7664	0.17%	0.018%
22	11.457	1420	1423	1433	rVB9	5463	14499	0.33%	0.034%
23	12.251	1552	1558	1564	rBV3	19095	30613	0.69%	0.072%
24	12.351	1569	1575	1579	rVV7	2890	4589	0.10%	0.011%
25	13.298	1731	1736	1739	rBV6	3872	8547	0.19%	0.020%
26	13.328	1739	1741	1745	rVV3	5736	8050	0.18%	0.019%
27	13.410	1748	1755	1760	rVB4	14585	26511	0.60%	0.062%
28	13.928	1836	1843	1854	rBV	1756559	2479055	56.05%	5.799%
29	14.198	1879	1889	1903	rBV	2112962	3071986	69.46%	7.186%
30	14.292	1903	1905	1910	rVB6	3507	4825	0.11%	0.011%
31	14.410	1924	1925	1933	rVB6	3653	5297	0.12%	0.012%
32	14.504	1933	1941	1950	rBV	945396	1409033	31.86%	3.296%
33	14.722	1972	1978	1989	rBV	63100	159786	3.61%	0.374%
34	14.881	2001	2005	2010	rBV8	3351	5972	0.14%	0.014%
35	14.934	2010	2014	2018	rVB7	6798	10863	0.25%	0.025%
36	14.998	2020	2025	2026	rBV5	5513	8401	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029863.D
 Acq On : 19 Feb 2024 22:41
 Operator : MA/JU
 Sample : P1402-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.139	2046	2049	2051	rBV3	5150	5913	0.13%	0.014%
38	15.192	2056	2058	2064	rVV7	5905	7804	0.18%	0.018%
39	15.310	2074	2078	2081	rVV	12870	18714	0.42%	0.044%
40	15.345	2081	2084	2090	rVB7	8508	15581	0.35%	0.036%
41	15.504	2103	2111	2124	rBV	2473902	3684322	83.30%	8.618%
42	15.628	2125	2132	2148	rVV	684847	997014	22.54%	2.332%
43	15.739	2148	2151	2155	rVB4	11589	17451	0.39%	0.041%
44	16.069	2203	2207	2214	rBV9	5095	10523	0.24%	0.025%
45	16.228	2230	2234	2240	rBV8	8173	15232	0.34%	0.036%
46	16.286	2240	2244	2249	rVB7	10872	17572	0.40%	0.041%
47	16.410	2260	2265	2272	rBV7	5693	10727	0.24%	0.025%
48	16.869	2338	2343	2344	rBV5	6717	8612	0.19%	0.020%
49	16.933	2351	2354	2359	rVB7	6120	11161	0.25%	0.026%
50	16.992	2359	2364	2365	rBV5	6269	8066	0.18%	0.019%
51	17.028	2366	2370	2375	rVV6	9459	16963	0.38%	0.040%
52	17.257	2402	2409	2419	rBV	1136626	1598695	36.15%	3.740%
53	17.357	2419	2426	2443	rVV	2703216	3849279	87.03%	9.004%
54	17.510	2450	2452	2456	rBV5	4973	6882	0.16%	0.016%
55	17.769	2494	2496	2500	rVB5	5160	5159	0.12%	0.012%
56	17.951	2521	2527	2531	rBV	79050	107400	2.43%	0.251%
57	18.169	2559	2564	2570	rBV2	85693	124243	2.81%	0.291%
58	18.251	2575	2578	2582	rVB3	18500	24559	0.56%	0.057%
59	18.463	2611	2614	2617	rBV5	10185	15740	0.36%	0.037%
60	18.645	2642	2645	2650	rBV7	7523	12927	0.29%	0.030%
61	18.975	2698	2701	2709	rVB	32886	49069	1.11%	0.115%
62	19.127	2725	2727	2731	rVB5	13325	13497	0.31%	0.032%
63	19.222	2738	2743	2747	rBV2	39240	54729	1.24%	0.128%
64	19.263	2748	2750	2751	rBV2	8496	6990	0.16%	0.016%
65	19.292	2752	2755	2759	rVB	30593	37811	0.85%	0.088%
66	19.457	2778	2783	2789	rBV2	49992	79857	1.81%	0.187%
67	19.657	2811	2817	2825	rBV	3307146	4422908	100.00%	10.346%
68	21.198	3076	3079	3086	rVB5	49688	72611	1.64%	0.170%
69	21.457	3118	3123	3135	rBV	1175568	1610305	36.41%	3.767%
70	23.668	3492	3499	3511	rBV2	2131521	4369539	98.79%	10.221%
71	23.821	3519	3525	3537	rVB	847489	1714211	38.76%	4.010%




Sum of corrected areas: 42751190

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029863.D
Acq On : 19 Feb 2024 22:41
Operator : MA/JU
Sample : P1402-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

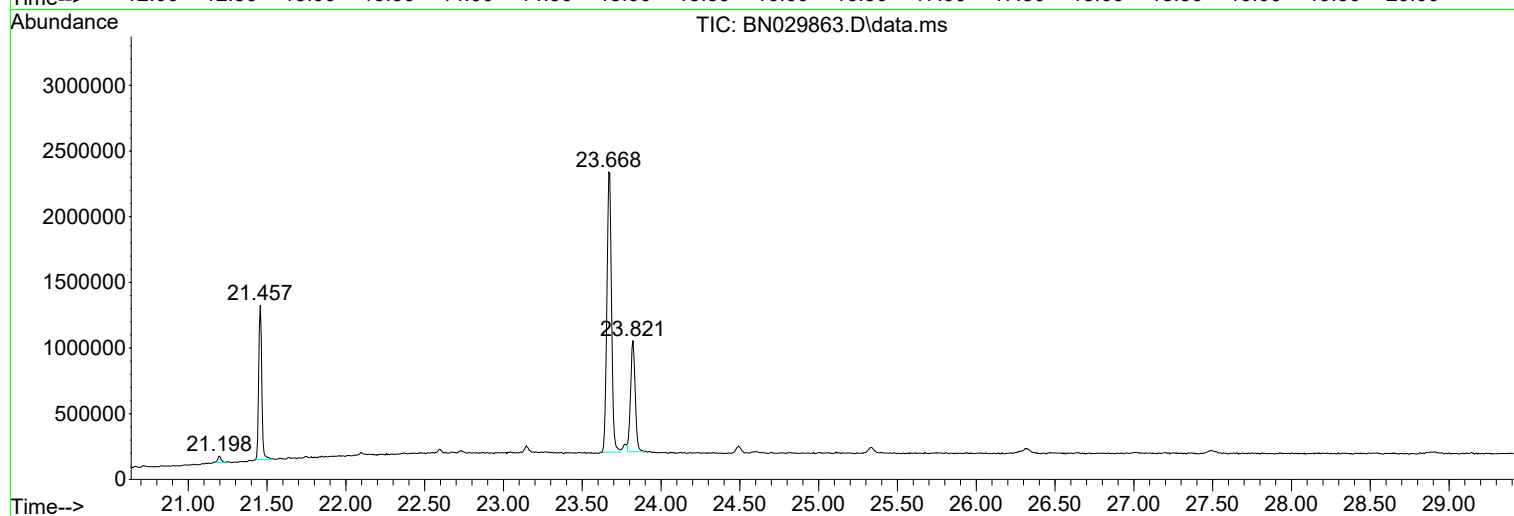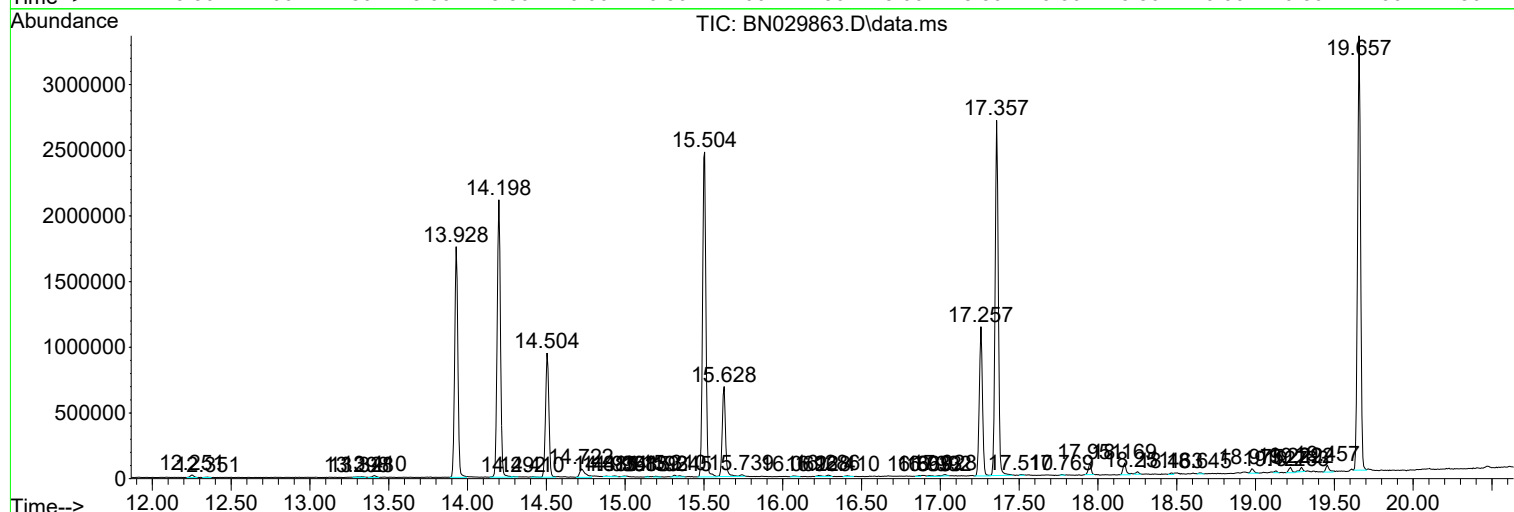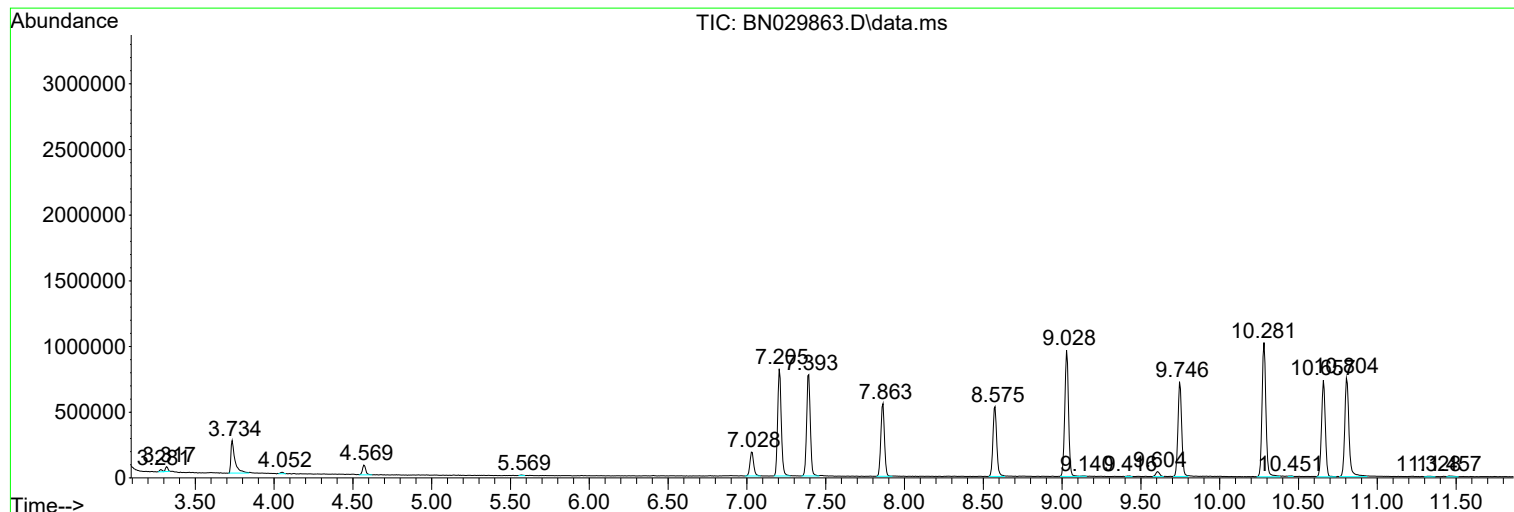

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029863.D
Acq On : 19 Feb 2024 22:41
Operator : MA/JU
Sample : P1402-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029863.D
Acq On : 19 Feb 2024 22:41
Operator : MA/JU
Sample : P1402-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc