

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029864.D
 Acq On : 19 Feb 2024 23:17
 Operator : MA/JU
 Sample : P1402-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	43	rBV	934931	1307127	29.17%	3.007%
2	3.734	106	110	127	rBV	204648	381113	8.50%	0.877%
3	4.052	160	164	169	rVB2	12145	17616	0.39%	0.041%
4	4.570	246	252	264	rVB	383055	549698	12.27%	1.264%
5	7.028	663	670	678	rBV	185915	311423	6.95%	0.716%
6	7.205	693	700	715	rBV	779571	1258862	28.09%	2.896%
7	7.393	723	732	742	rBV	729351	1202100	26.82%	2.765%
8	7.475	742	746	751	rVB7	4987	8952	0.20%	0.021%
9	7.863	805	812	821	rVV	521994	841528	18.78%	1.936%
10	7.934	821	824	829	rVB5	3632	6687	0.15%	0.015%
11	8.575	926	933	943	rBV	508251	857538	19.13%	1.973%
12	9.028	1003	1010	1023	rBV	943011	1545928	34.50%	3.556%
13	9.746	1123	1132	1144	rBV	696744	1165259	26.00%	2.680%
14	10.281	1213	1223	1235	rBV	982970	1638574	36.56%	3.769%
15	10.657	1279	1287	1298	rBV	698428	1171808	26.15%	2.695%
16	10.804	1304	1312	1331	rBV	851036	1571366	35.06%	3.614%
17	11.375	1407	1409	1416	rVB6	3005	5701	0.13%	0.013%
18	12.251	1551	1558	1567	rVB	16540	31981	0.71%	0.074%
19	13.134	1703	1708	1715	rVB4	5798	10446	0.23%	0.024%
20	13.410	1750	1755	1760	rBV	16015	26133	0.58%	0.060%
21	13.928	1836	1843	1855	rBV	1774669	2485608	55.46%	5.717%
22	14.198	1882	1889	1904	rVV	2122712	3053642	68.14%	7.024%
23	14.334	1910	1912	1917	rVB4	3517	5366	0.12%	0.012%
24	14.504	1934	1941	1952	rBV	940726	1363122	30.42%	3.135%
25	14.722	1972	1978	1992	rBV2	55395	156281	3.49%	0.359%
26	15.316	2075	2079	2086	rVB4	5068	8723	0.19%	0.020%
27	15.504	2103	2111	2126	rBV	2508764	3687815	82.29%	8.483%
28	15.628	2126	2132	2145	rVV	688983	989685	22.08%	2.276%
29	15.740	2148	2151	2158	rVB4	10699	18235	0.41%	0.042%
30	16.287	2239	2244	2248	rVB5	7972	11159	0.25%	0.026%
31	17.257	2402	2409	2419	rBV	1107705	1557622	34.76%	3.583%
32	17.357	2419	2426	2445	rVV	2702104	3910775	87.26%	8.996%
33	17.939	2521	2525	2530	rVB6	6359	7911	0.18%	0.018%
34	18.169	2559	2564	2574	rBV3	38960	63890	1.43%	0.147%
35	18.498	2615	2620	2627	rBV4	12836	20772	0.46%	0.048%
36	18.610	2634	2639	2642	rBV6	3204	5752	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029864.D
 Acq On : 19 Feb 2024 23:17
 Operator : MA/JU
 Sample : P1402-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	18.651	2644	2646	2652	rVB7	5487	6508	0.15%	0.015%
38	19.216	2738	2742	2749	rBV3	32171	48387	1.08%	0.111%
39	19.292	2749	2755	2758	rBV	30471	47811	1.07%	0.110%
40	19.451	2779	2782	2790	rVB6	21099	25954	0.58%	0.060%
41	19.610	2806	2809	2811	rBV3	8148	9574	0.21%	0.022%
42	19.657	2811	2817	2826	rVV	3327521	4481560	100.00%	10.309%
43	19.898	2855	2858	2861	rBV4	9478	10708	0.24%	0.025%
44	20.033	2879	2881	2885	rBV5	4445	6657	0.15%	0.015%
45	20.228	2912	2914	2916	rBV3	6034	5067	0.11%	0.012%
46	21.192	3075	3078	3084	rVB6	26466	37655	0.84%	0.087%
47	21.457	3117	3123	3130	rBV2	1149930	1573538	35.11%	3.619%
48	23.669	3492	3499	3510	rBV2	2186815	4338836	96.82%	9.980%
49	23.821	3518	3525	3535	rVB	802638	1625953	36.28%	3.740%




Sum of corrected areas: 43474406

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029864.D
Acq On : 19 Feb 2024 23:17
Operator : MA/JU
Sample : P1402-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

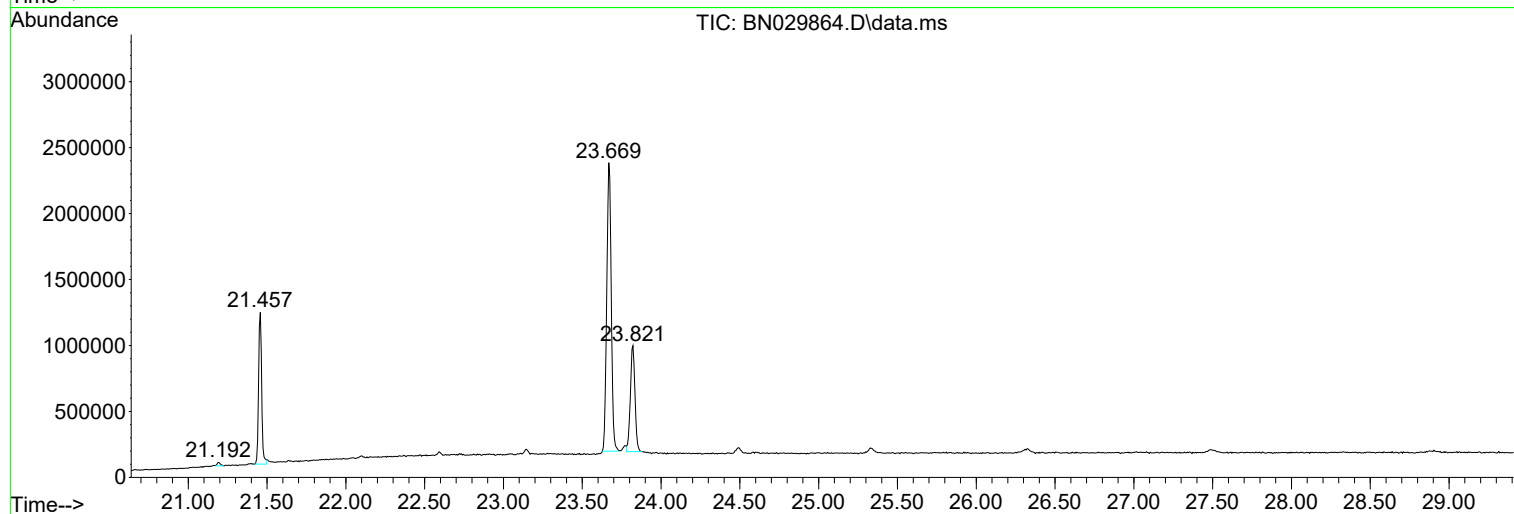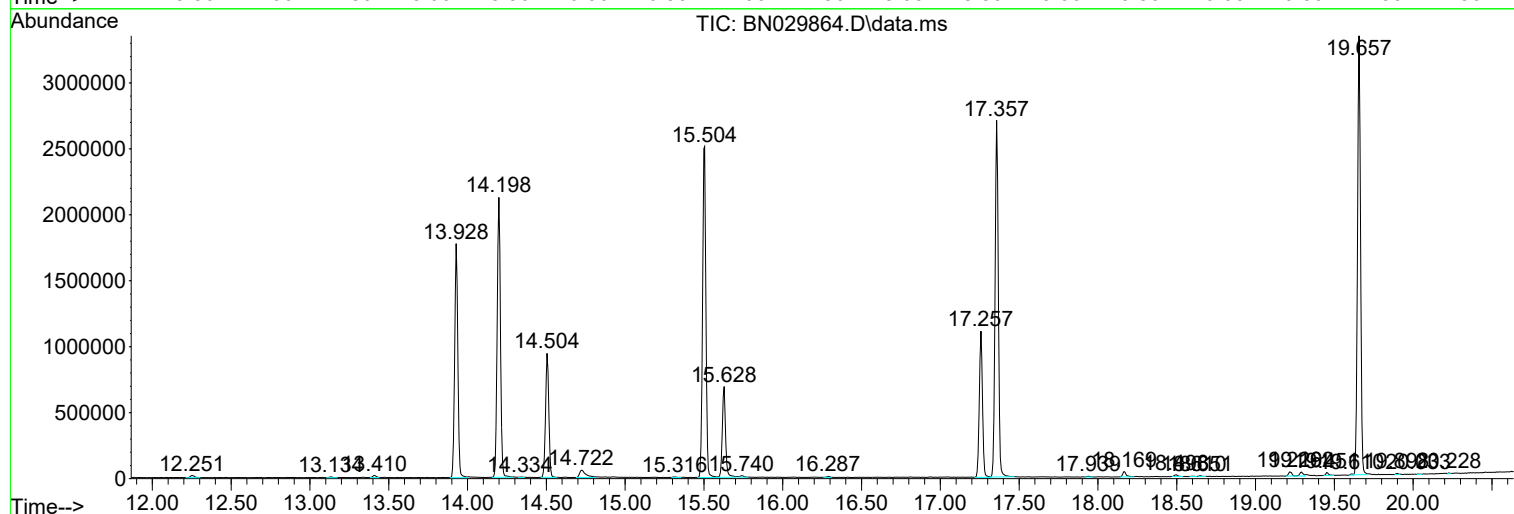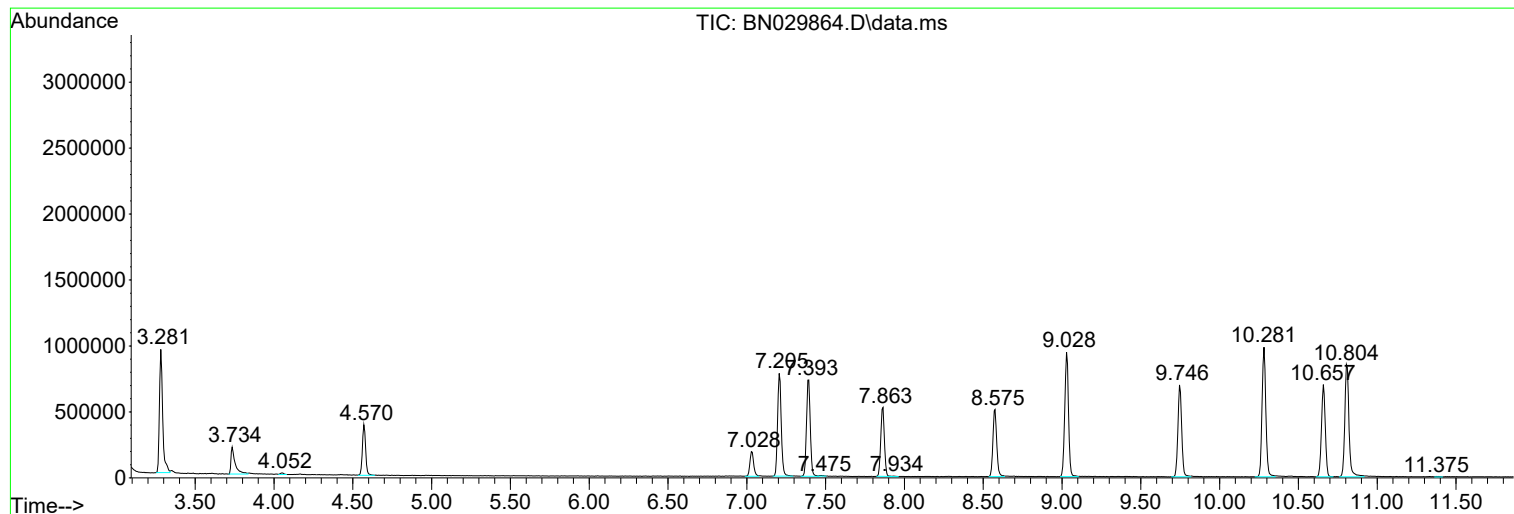

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029864.D
Acq On : 19 Feb 2024 23:17
Operator : MA/JU
Sample : P1402-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029864.D
Acq On : 19 Feb 2024 23:17
Operator : MA/JU
Sample : P1402-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc