

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029865.D
 Acq On : 19 Feb 2024 23:53
 Operator : MA/JU
 Sample : P1436-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH7G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	48	rBV2	39503	58483	1.35%	0.140%
2	3.734	106	110	132	rBV	216424	412657	9.50%	0.985%
3	4.052	160	164	170	rVB	12199	15523	0.36%	0.037%
4	5.864	470	472	478	rVB7	2920	5038	0.12%	0.012%
5	7.028	665	670	680	rBV	164504	272672	6.28%	0.651%
6	7.205	693	700	716	rBV	804307	1273842	29.32%	3.041%
7	7.393	723	732	740	rBV	703335	1143061	26.31%	2.729%
8	7.863	805	812	821	rBV	549192	899216	20.69%	2.147%
9	8.575	926	933	946	rBV	482772	805063	18.53%	1.922%
10	9.028	1002	1010	1025	rBV	945389	1545010	35.56%	3.688%
11	9.140	1025	1029	1032	rVV3	4822	9791	0.23%	0.023%
12	9.410	1073	1075	1083	rVB6	4841	9270	0.21%	0.022%
13	9.746	1125	1132	1145	rBV	691769	1133094	26.08%	2.705%
14	10.281	1215	1223	1240	rBV	958931	1620966	37.31%	3.869%
15	10.657	1280	1287	1297	rBV	752928	1241129	28.56%	2.963%
16	10.804	1303	1312	1327	rBV	767591	1421297	32.71%	3.393%
17	11.422	1408	1417	1423	rBV3	13562	30526	0.70%	0.073%
18	12.251	1551	1558	1564	rBV2	19324	33031	0.76%	0.079%
19	13.246	1720	1727	1729	rBV7	4623	8526	0.20%	0.020%
20	13.334	1736	1742	1746	rBV5	8560	15839	0.36%	0.038%
21	13.404	1746	1754	1759	rVV5	13032	30979	0.71%	0.074%
22	13.475	1764	1766	1770	rVV4	4135	5850	0.13%	0.014%
23	13.510	1770	1772	1777	rVB4	4803	6969	0.16%	0.017%
24	13.928	1836	1843	1853	rBV	1783055	2460195	56.62%	5.873%
25	14.198	1878	1889	1903	rBV	2074369	3065788	70.56%	7.318%
26	14.416	1923	1926	1931	rVB6	6584	9395	0.22%	0.022%
27	14.504	1934	1941	1950	rVV	977546	1434271	33.01%	3.424%
28	14.575	1950	1953	1957	rVV6	5530	10361	0.24%	0.025%
29	14.616	1957	1960	1963	rVB5	2932	4529	0.10%	0.011%
30	14.722	1972	1978	1993	rBV3	51272	132881	3.06%	0.317%
31	14.928	2007	2013	2019	rVB9	8371	15300	0.35%	0.037%
32	15.310	2074	2078	2082	rVB5	6610	9946	0.23%	0.024%
33	15.363	2084	2087	2091	rVB7	8101	8433	0.19%	0.020%
34	15.404	2091	2094	2102	rVB6	4823	9360	0.22%	0.022%
35	15.498	2104	2110	2125	rBV	2410554	3633465	83.62%	8.673%
36	15.628	2125	2132	2144	rVV	656697	941731	21.67%	2.248%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029865.D
 Acq On : 19 Feb 2024 23:53
 Operator : MA/JU
 Sample : P1436-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH7G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.740	2147	2151	2155	rVB4	11979	16770	0.39%	0.040%
38	16.069	2201	2207	2212	rBV8	6684	14147	0.33%	0.034%
39	16.234	2231	2235	2238	rVV5	3749	5150	0.12%	0.012%
40	16.287	2241	2244	2249	rVB3	7856	10281	0.24%	0.025%
41	16.410	2260	2265	2269	rBV6	6925	9188	0.21%	0.022%
42	16.581	2290	2294	2297	rBV6	2691	5051	0.12%	0.012%
43	16.669	2305	2309	2312	rVB6	6319	6337	0.15%	0.015%
44	16.986	2358	2363	2368	rBV7	5553	11135	0.26%	0.027%
45	17.022	2368	2369	2375	rVB4	3270	5663	0.13%	0.014%
46	17.257	2402	2409	2418	rBV	1165057	1637113	37.68%	3.908%
47	17.357	2419	2426	2443	rVV	2746913	3933990	90.54%	9.391%
48	17.563	2458	2461	2465	rVB4	3800	5003	0.12%	0.012%
49	17.663	2474	2478	2485	rVB8	4211	9051	0.21%	0.022%
50	17.775	2494	2497	2499	rBV4	3980	4356	0.10%	0.010%
51	17.945	2519	2526	2529	rBV8	5268	12857	0.30%	0.031%
52	18.039	2540	2542	2545	rBV4	2957	4375	0.10%	0.010%
53	18.169	2559	2564	2571	rBV	81943	118580	2.73%	0.283%
54	18.469	2610	2615	2617	rBV5	7786	12093	0.28%	0.029%
55	18.604	2635	2638	2642	rBV5	11860	12559	0.29%	0.030%
56	18.833	2671	2677	2683	rBV	21527	40212	0.93%	0.096%
57	18.928	2690	2693	2698	rBV6	9488	15198	0.35%	0.036%
58	19.222	2737	2743	2747	rBV2	36827	52748	1.21%	0.126%
59	19.292	2751	2755	2760	rBV	29852	41603	0.96%	0.099%
60	19.363	2765	2767	2774	rVB8	4791	9198	0.21%	0.022%
61	19.451	2779	2782	2786	rBV2	32321	42170	0.97%	0.101%
62	19.604	2806	2808	2811	rBV4	9090	10741	0.25%	0.026%
63	19.657	2811	2817	2824	rVV	3158209	4345143	100.00%	10.372%
64	19.710	2824	2826	2832	rVB6	12604	21261	0.49%	0.051%
65	20.033	2878	2881	2887	rVB3	14419	22243	0.51%	0.053%
66	20.104	2890	2893	2896	rVB4	8508	10225	0.24%	0.024%
67	20.463	2951	2954	2960	rBV5	17062	26107	0.60%	0.062%
68	20.657	2985	2987	2990	rBV4	8555	9008	0.21%	0.022%
69	21.192	3075	3078	3085	rVB4	49527	67339	1.55%	0.161%
70	21.457	3118	3123	3130	rBV	1251432	1577382	36.30%	3.765%
71	23.669	3491	3499	3510	rBV2	2157991	4304530	99.07%	10.275%
72	23.821	3518	3525	3537	rVB	819167	1729510	39.80%	4.129%




Sum of corrected areas: 41891804

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029865.D
Acq On : 19 Feb 2024 23:53
Operator : MA/JU
Sample : P1436-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH7G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

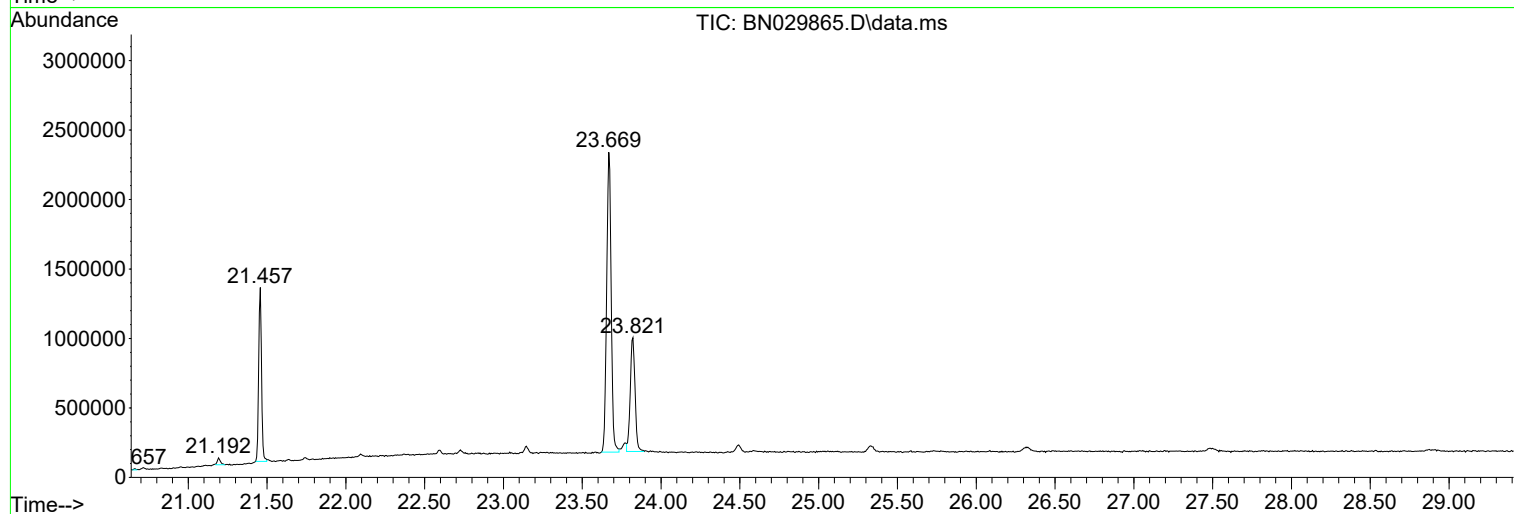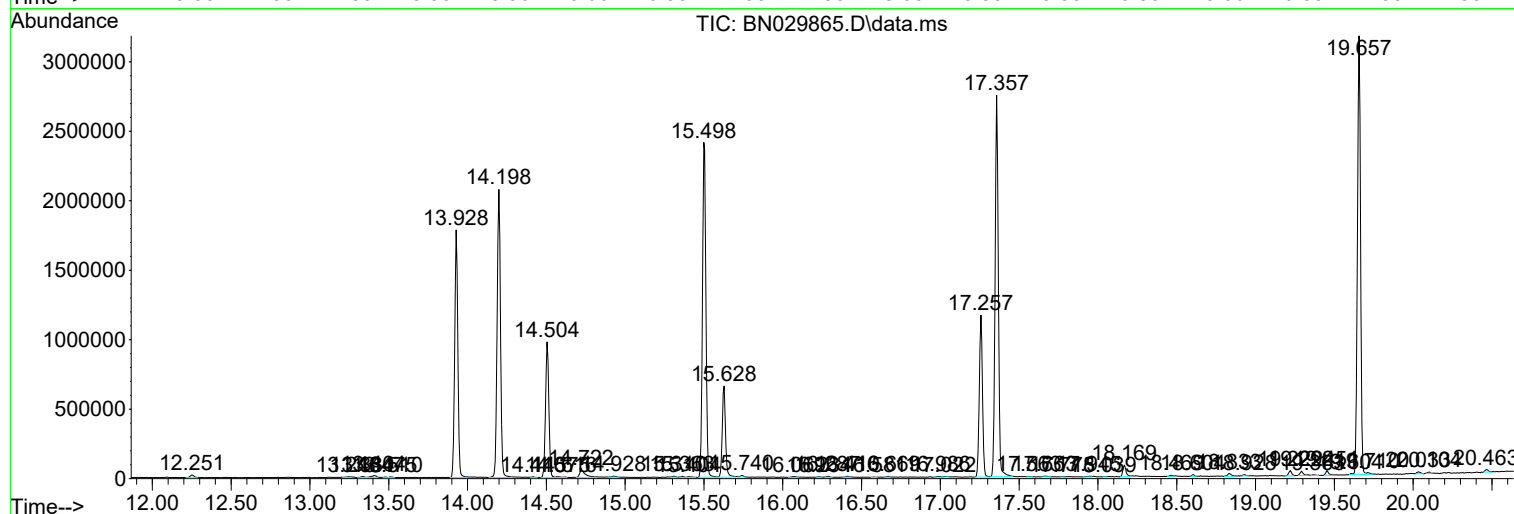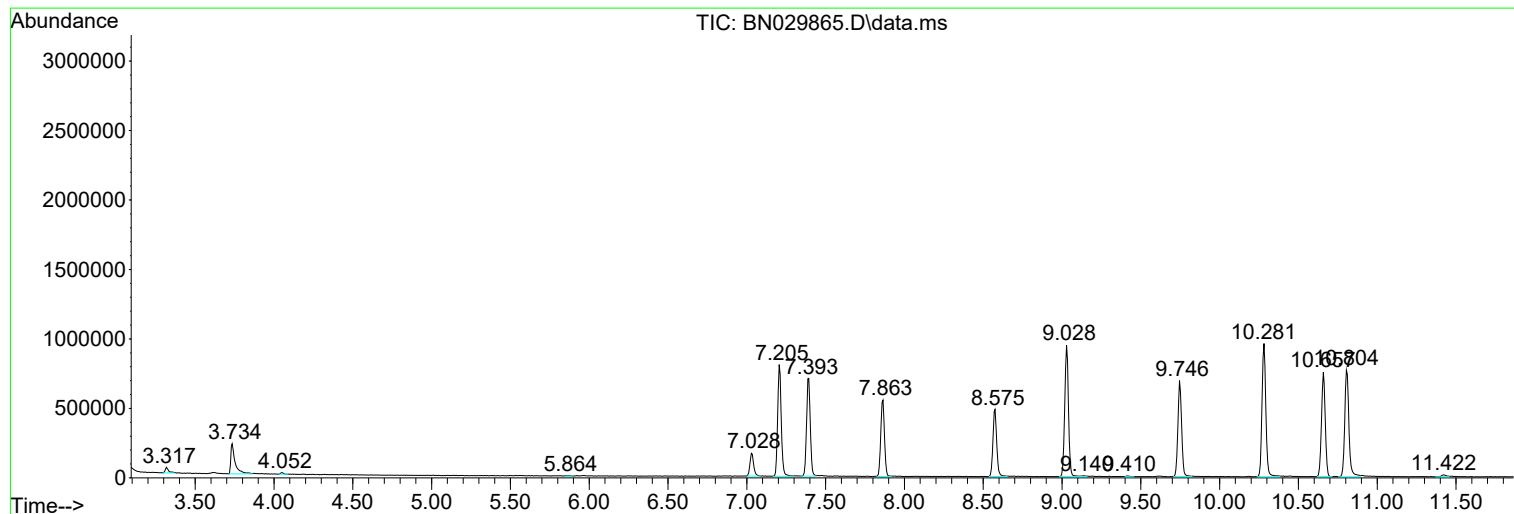

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029865.D
Acq On : 19 Feb 2024 23:53
Operator : MA/JU
Sample : P1436-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH7G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029865.D
Acq On : 19 Feb 2024 23:53
Operator : MA/JU
Sample : P1436-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH7G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc