

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029868.D
Acq On : 20 Feb 2024 06:27
Operator : MA/JU
Sample : P1455-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BN029868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	36	39	45	rVB	33747	41946	0.92%	0.101%
2	4.046	160	163	168	rVB3	13592	18908	0.41%	0.045%
3	4.570	248	252	257	rVB4	21328	29501	0.64%	0.071%
4	5.522	411	414	419	rVB3	6972	8638	0.19%	0.021%
5	7.028	662	670	686	rVB	325326	532866	11.62%	1.279%
6	7.205	693	700	714	rBV	804400	1268008	27.66%	3.042%
7	7.387	724	731	743	rBV	949310	1501389	32.75%	3.602%
8	7.858	804	811	821	rBV	545483	878046	19.15%	2.107%
9	8.569	925	932	948	rBV	770493	1290586	28.15%	3.097%
10	9.028	1003	1010	1022	rBV	932990	1519986	33.16%	3.647%
11	9.193	1034	1038	1045	rVB7	3627	7590	0.17%	0.018%
12	9.422	1072	1077	1081	rVB7	3637	7417	0.16%	0.018%
13	9.746	1124	1132	1145	rBV	719616	1190580	25.97%	2.857%
14	10.281	1215	1223	1242	rBV	1041189	1832525	39.98%	4.397%
15	10.657	1279	1287	1297	rVB	726730	1209806	26.39%	2.903%
16	10.816	1307	1314	1321	rBV2	26327	56207	1.23%	0.135%
17	12.087	1524	1530	1536	rVB8	2319	4634	0.10%	0.011%
18	12.251	1552	1558	1563	rVB2	15580	25665	0.56%	0.062%
19	13.340	1736	1743	1746	rVB9	4164	5710	0.12%	0.014%
20	13.410	1746	1755	1762	rVB4	14521	28681	0.63%	0.069%
21	13.475	1762	1766	1767	rBV3	5217	6152	0.13%	0.015%
22	13.928	1836	1843	1856	rBV	1748467	2436792	53.16%	5.847%
23	14.198	1878	1889	1901	rBV	1920186	2875212	62.72%	6.899%
24	14.504	1934	1941	1951	rBV	950291	1412540	30.81%	3.389%
25	14.722	1971	1978	1996	rBV	133866	327590	7.15%	0.786%
26	14.928	2009	2013	2020	rBV3	34328	53401	1.16%	0.128%
27	15.310	2073	2078	2083	rBV	16587	21695	0.47%	0.052%
28	15.498	2102	2110	2123	rBV	2398730	3563286	77.73%	8.550%
29	15.628	2126	2132	2147	rVV	733450	1072692	23.40%	2.574%
30	15.740	2147	2151	2157	rVB5	10772	18021	0.39%	0.043%
31	16.287	2239	2244	2250	rVB5	7670	11618	0.25%	0.028%
32	16.934	2350	2354	2357	rVB5	4517	6131	0.13%	0.015%
33	17.257	2402	2409	2419	rBV	1150017	1640174	35.78%	3.935%
34	17.357	2419	2426	2438	rBV	2781524	3959961	86.38%	9.501%
35	17.934	2520	2524	2530	rVB5	21255	27238	0.59%	0.065%
36	18.163	2559	2563	2569	rBV4	30405	41891	0.91%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029868.D
Acq On : 20 Feb 2024 06:27
Operator : MA/JU
Sample : P1455-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	18.245	2573	2577	2582	rVB5	5973	6854	0.15%	0.016%
38	18.657	2641	2647	2650	rBV8	4070	7391	0.16%	0.018%
39	19.028	2707	2710	2712	rBV4	6367	7486	0.16%	0.018%
40	19.216	2738	2742	2749	rBV2	36819	53748	1.17%	0.129%
41	19.292	2750	2755	2759	rVV	29436	44325	0.97%	0.106%
42	19.328	2759	2761	2765	rVV5	5583	6729	0.15%	0.016%
43	19.451	2777	2782	2790	rBV5	33532	55616	1.21%	0.133%
44	19.533	2794	2796	2799	rVB4	4669	4601	0.10%	0.011%
45	19.610	2806	2809	2810	rBV3	9082	8738	0.19%	0.021%
46	19.657	2810	2817	2826	rVV2	3240951	4568351	99.66%	10.961%
47	21.457	3118	3123	3130	rBV	1278540	1625923	35.47%	3.901%
48	23.669	3491	3499	3512	rBV	2306223	4584111	100.00%	10.999%
49	23.821	3518	3525	3536	rVB	853123	1770571	38.62%	4.248%




Sum of corrected areas: 41677527

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029868.D
Acq On : 20 Feb 2024 06:27
Operator : MA/JU
Sample : P1455-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

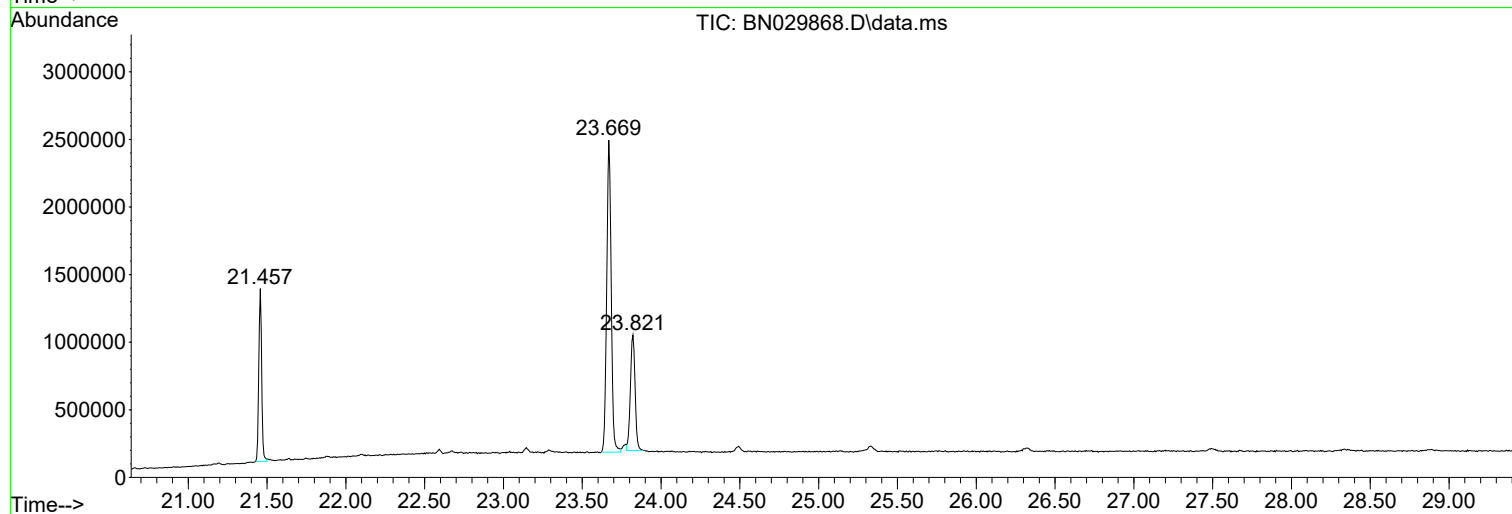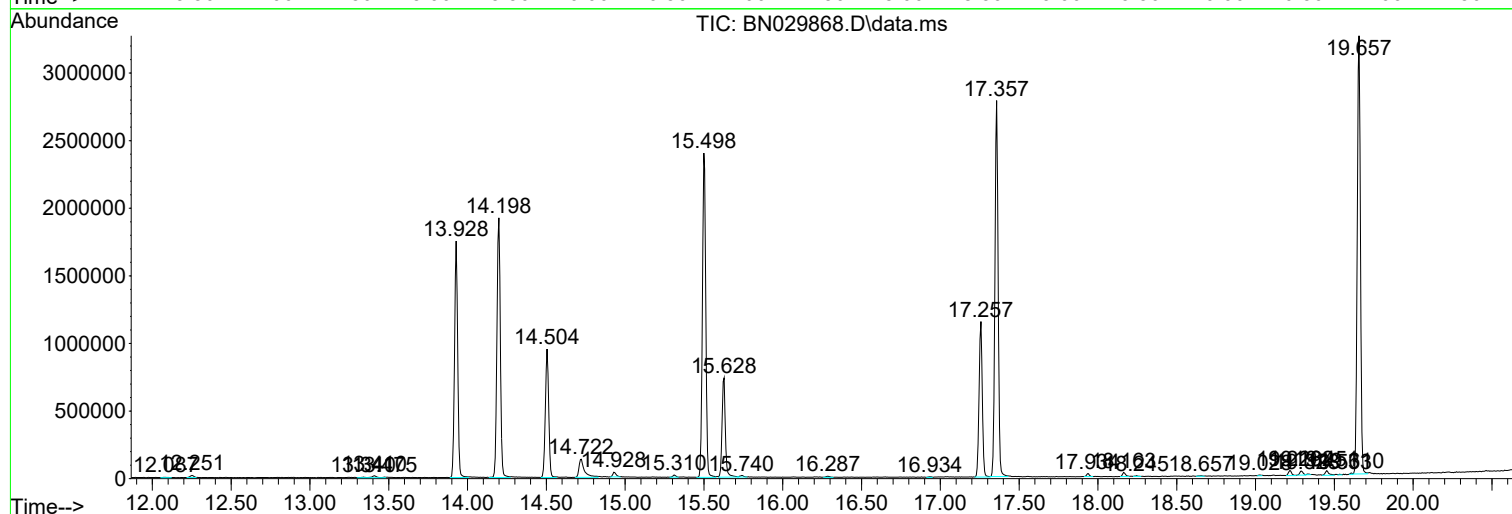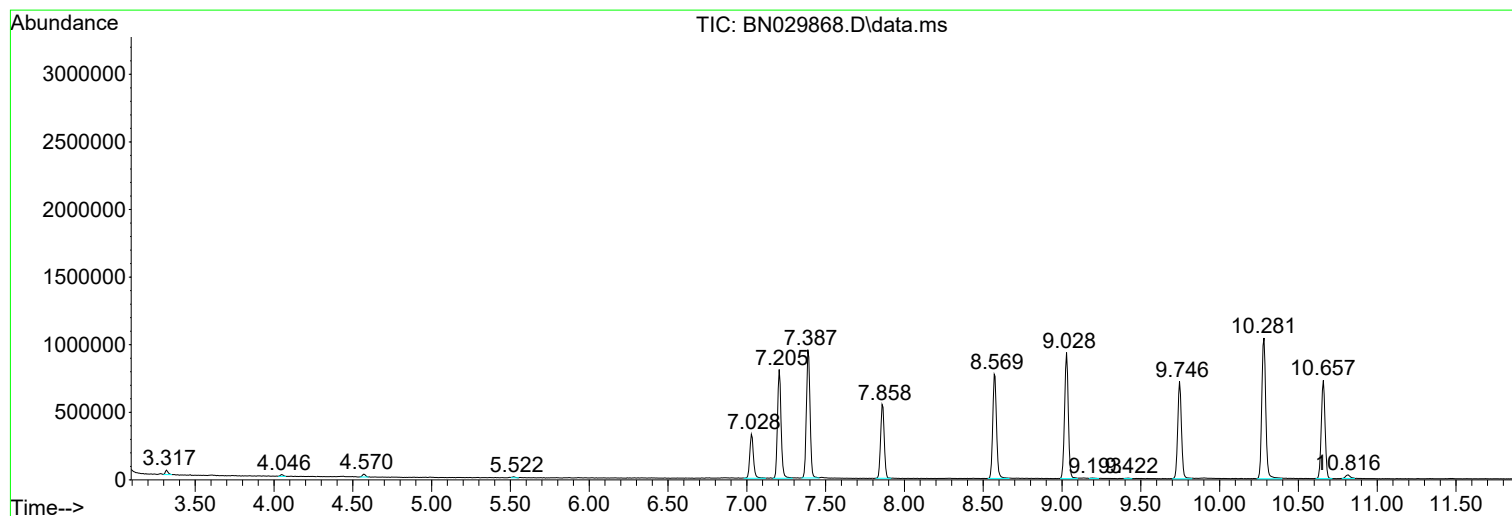

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029868.D
Acq On : 20 Feb 2024 06:27
Operator : MA/JU
Sample : P1455-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029868.D
Acq On : 20 Feb 2024 06:27
Operator : MA/JU
Sample : P1455-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------