

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029870.D
 Acq On : 20 Feb 2024 08:15
 Operator : MA/JU
 Sample : PB159060BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	35	39	48	rVB	67094	86213	2.10%	0.183%
2	3.728	105	109	126	rBV	709111	1167296	28.42%	2.480%
3	4.046	158	163	168	rBV5	31335	52141	1.27%	0.111%
4	4.222	190	193	198	rVB3	7467	9565	0.23%	0.020%
5	4.275	198	202	209	rVB4	12690	17952	0.44%	0.038%
6	4.428	224	228	235	rVB6	10951	15739	0.38%	0.033%
7	4.552	247	249	254	rBV5	5609	6596	0.16%	0.014%
8	4.611	254	259	264	rVV	44763	62314	1.52%	0.132%
9	4.663	265	268	277	rVB2	14604	30560	0.74%	0.065%
10	5.758	450	454	456	rBV5	5320	6222	0.15%	0.013%
11	6.181	523	526	533	rVB7	4506	10146	0.25%	0.022%
12	7.028	663	670	687	rBV	946761	1496473	36.44%	3.180%
13	7.205	694	700	712	rBV	732482	1160554	28.26%	2.466%
14	7.387	724	731	744	rVB	940756	1493655	36.37%	3.174%
15	7.569	758	762	768	rVB9	6198	11714	0.29%	0.025%
16	7.857	804	811	818	rBV	687741	1093521	26.63%	2.323%
17	8.099	848	852	857	rBV8	6510	13613	0.33%	0.029%
18	8.569	925	932	946	rBV	1056669	1760817	42.87%	3.741%
19	9.028	1001	1010	1021	rBV	857291	1408171	34.29%	2.992%
20	9.746	1125	1132	1147	rBV	681574	1127134	27.44%	2.395%
21	10.028	1174	1180	1182	rBV6	3410	7539	0.18%	0.016%
22	10.281	1215	1223	1243	rBV	1028042	1745629	42.50%	3.709%
23	10.534	1259	1266	1269	rVB8	4294	8340	0.20%	0.018%
24	10.657	1277	1287	1295	rBV	926934	1526045	37.16%	3.242%
25	10.804	1305	1312	1328	rBV	985348	1785444	43.47%	3.794%
26	11.298	1392	1396	1397	rBV4	4644	4779	0.12%	0.010%
27	11.340	1401	1403	1408	rVV5	4311	7089	0.17%	0.015%
28	11.416	1412	1416	1421	rVV6	4762	6896	0.17%	0.015%
29	12.251	1553	1558	1563	rBV3	17878	29065	0.71%	0.062%
30	13.410	1749	1755	1758	rBV4	11036	18489	0.45%	0.039%
31	13.928	1836	1843	1858	rBV	1629573	2305151	56.13%	4.898%
32	14.198	1882	1889	1904	rBV	1920961	2814516	68.53%	5.980%
33	14.504	1934	1941	1949	rBV	1251510	1826501	44.47%	3.881%
34	14.716	1967	1977	1994	rBV	550441	1087667	26.48%	2.311%
35	15.498	2104	2110	2124	rBV	2411410	3429077	83.49%	7.286%
36	15.628	2125	2132	2141	rBV	605720	881950	21.47%	1.874%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
 Data File : BN029870.D
 Acq On : 20 Feb 2024 08:15
 Operator : MA/JU
 Sample : PB159060BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.739	2147	2151	2157	rVB3	11740	18652	0.45%	0.040%
38	16.286	2241	2244	2248	rVB4	7041	9127	0.22%	0.019%
39	16.645	2301	2305	2310	rBV8	2550	5273	0.13%	0.011%
40	17.257	2402	2409	2417	rVV	1519810	2140754	52.12%	4.548%
41	17.357	2419	2426	2441	rVV	2560710	3689927	89.85%	7.840%
42	18.169	2559	2564	2570	rBV9	4550	8518	0.21%	0.018%
43	18.704	2651	2655	2656	rBV4	3511	4387	0.11%	0.009%
44	19.216	2737	2742	2747	rBV	30361	43252	1.05%	0.092%
45	19.286	2750	2754	2759	rVV	25800	33562	0.82%	0.071%
46	19.604	2806	2808	2810	rBV3	6028	6826	0.17%	0.015%
47	19.657	2811	2817	2832	rVB	2912526	4106970	100.00%	8.726%
48	21.457	3117	3123	3138	rBV	1646384	2211002	53.84%	4.698%
49	23.668	3491	3499	3511	rBV2	1958550	4011617	97.68%	8.523%
50	23.821	3518	3525	3539	rVB	1069178	2261044	55.05%	4.804%




Sum of corrected areas: 47065484

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029870.D
Acq On : 20 Feb 2024 08:15
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

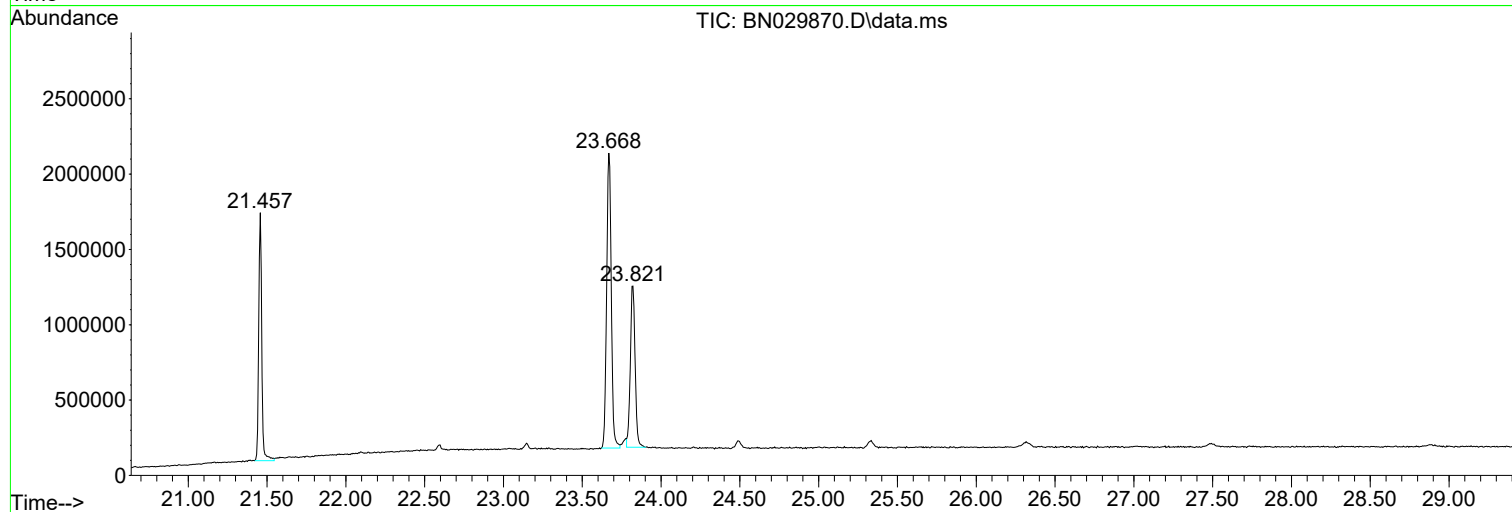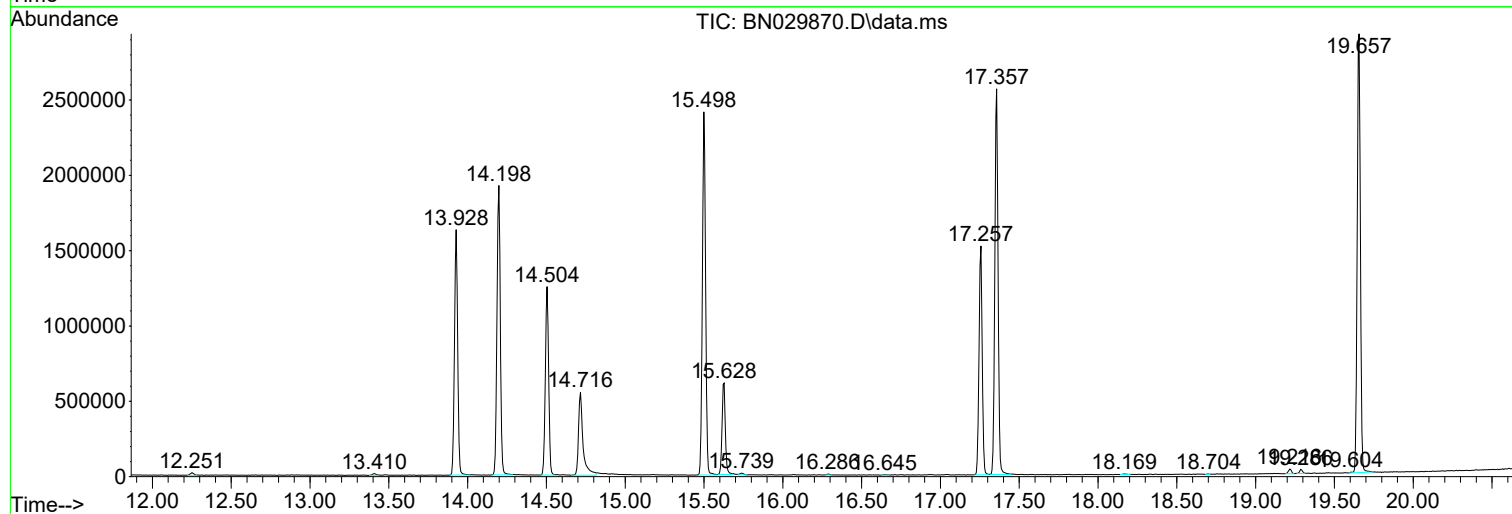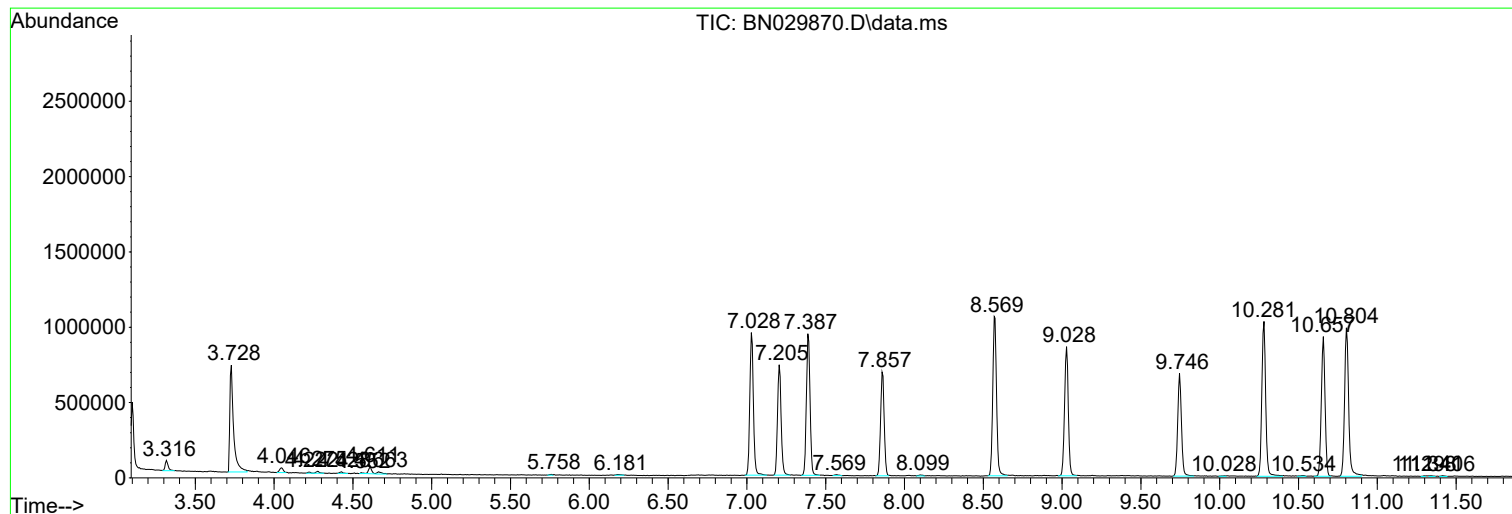

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029870.D
Acq On : 20 Feb 2024 08:15
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021924\
Data File : BN029870.D
Acq On : 20 Feb 2024 08:15
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc