




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021925\
Data File : BN036470.D
Acq On : 19 Feb 2025 14:57
Operator : RC/JU
Sample : Q1226-22DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZL9DL

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:01:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2025
Supervised By :mohammad ahmed 02/20/2025

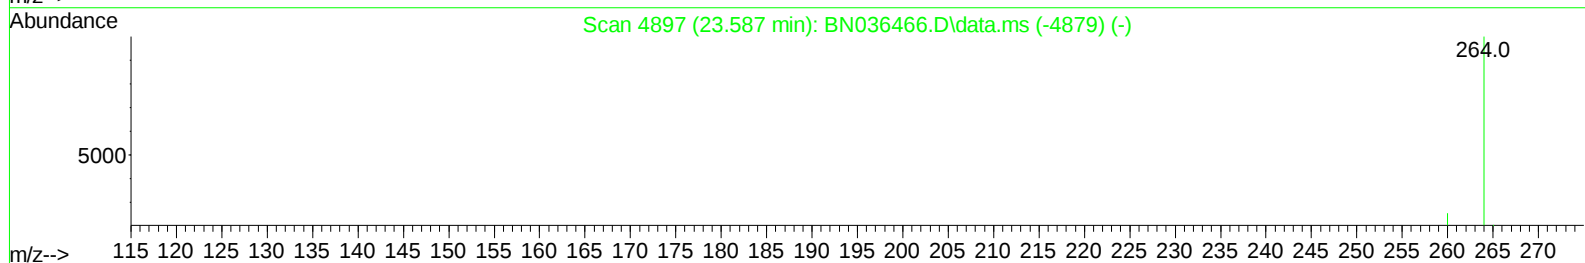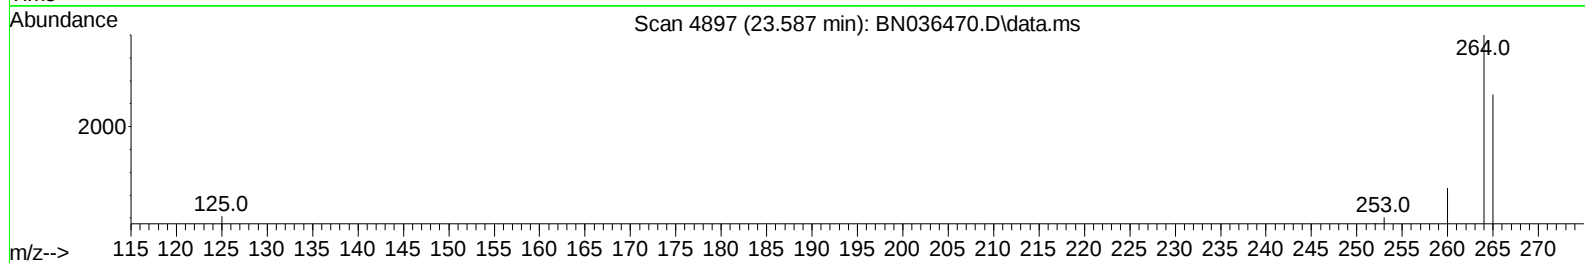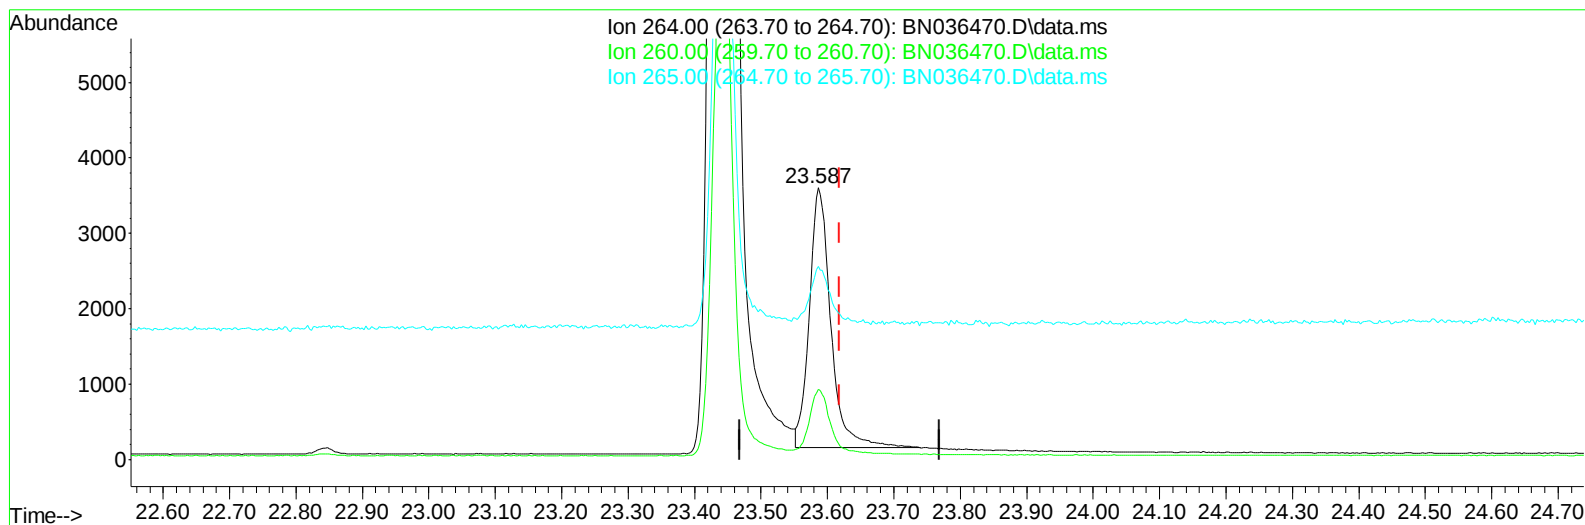

TIC: BN036470.D\data.ms

(23) Perylene-d12 (I)

23.587min (-0.032) 0.40 ng/u1

response 7697

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.82
265.00	53.20	70.99#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021925\
Data File : BN036470.D
Acq On : 19 Feb 2025 14:57
Operator : RC/JU
Sample : Q1226-22DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZL9DL

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:01:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2025
Supervised By :mohammad ahmed 02/20/2025

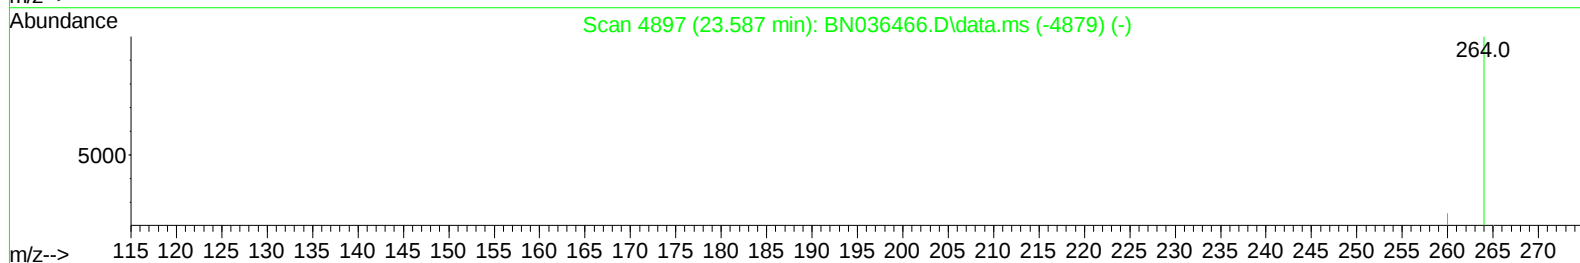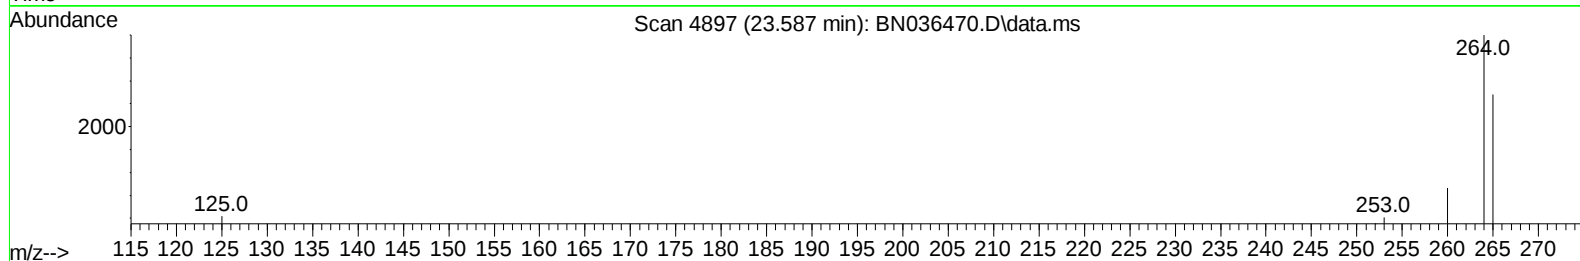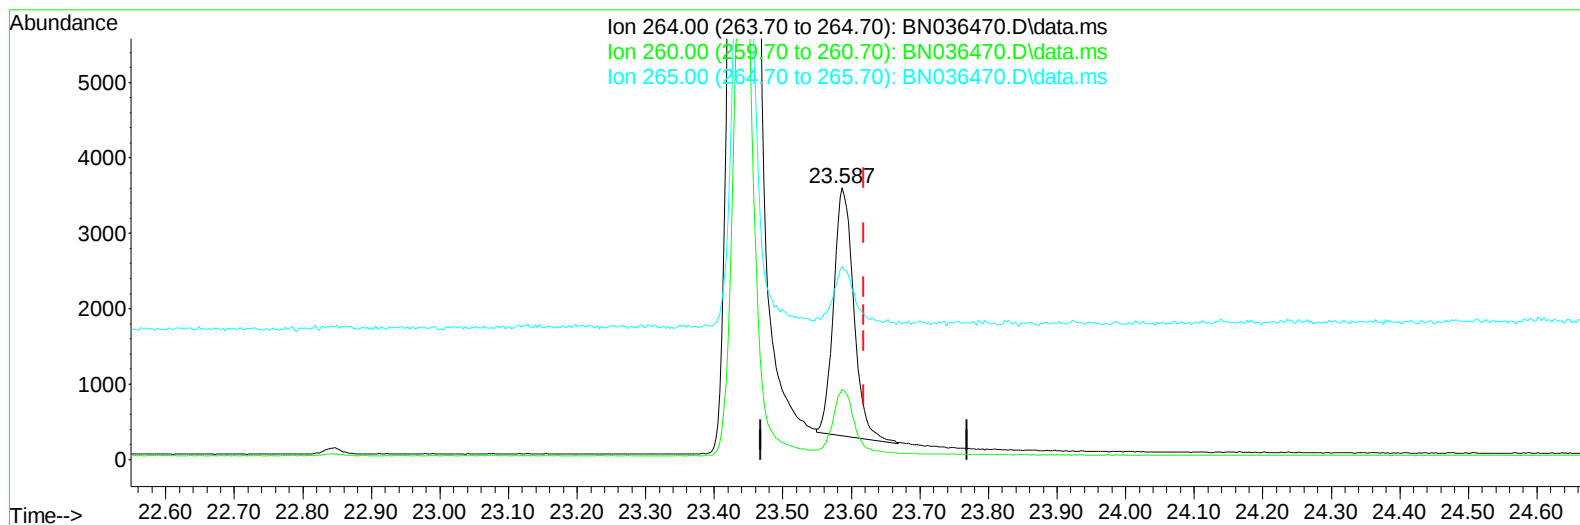

TIC: BN036470.D\data.ms

(23) Perylene-d12 (I)

23.587min (-0.032) 0.40 ng/ul m

response 6705

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.82
265.00	53.20	70.99#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021925\
 Data File : BN036470.D
 Acq On : 19 Feb 2025 14:57
 Operator : RC/JU
 Sample : Q1226-22DL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCZL9DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/20/2025
 Supervised By :mohammad ahmed 02/20/2025

Quant Time: Feb 19 18:01:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 07 11:25:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	2058	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.535	136	5209	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.386	164	3495	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.133	188	7561	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.322	240	6843	0.400	ng/ul	#-0.02
23) Perylene-d12	23.587	264	6705m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.227	96	606	0.269	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	12.135	152	243	0.037	ng/ul	-0.02
18) Fluoranthene-d10	19.165	212	819	0.044	ng/ul	-0.02
Target Compounds						
14) Pentachlorophenol	16.787	266	3042	1.148	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021925\
Data File : BN036470.D
Acq On : 19 Feb 2025 14:57
Operator : RC/JU
Sample : Q1226-22DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCZL9DL

Manual IntegrationsAPPROVED

Quant Time: Feb 19 18:01:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 07 11:25:57 2025
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/20/2025
Supervised By :mohammad ahmed 02/20/2025

