


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
Data File : BN013687.D
Acq On : 20 Feb 2021 12:21
Operator : CG/JU
Sample : PB134659BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK59

Manual Integrations
APPROVED

mohammad
2/22/2021 2:10:55 PM

Quant Time: Feb 22 02:36:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 02:30:08 2021
Response via : Initial Calibration

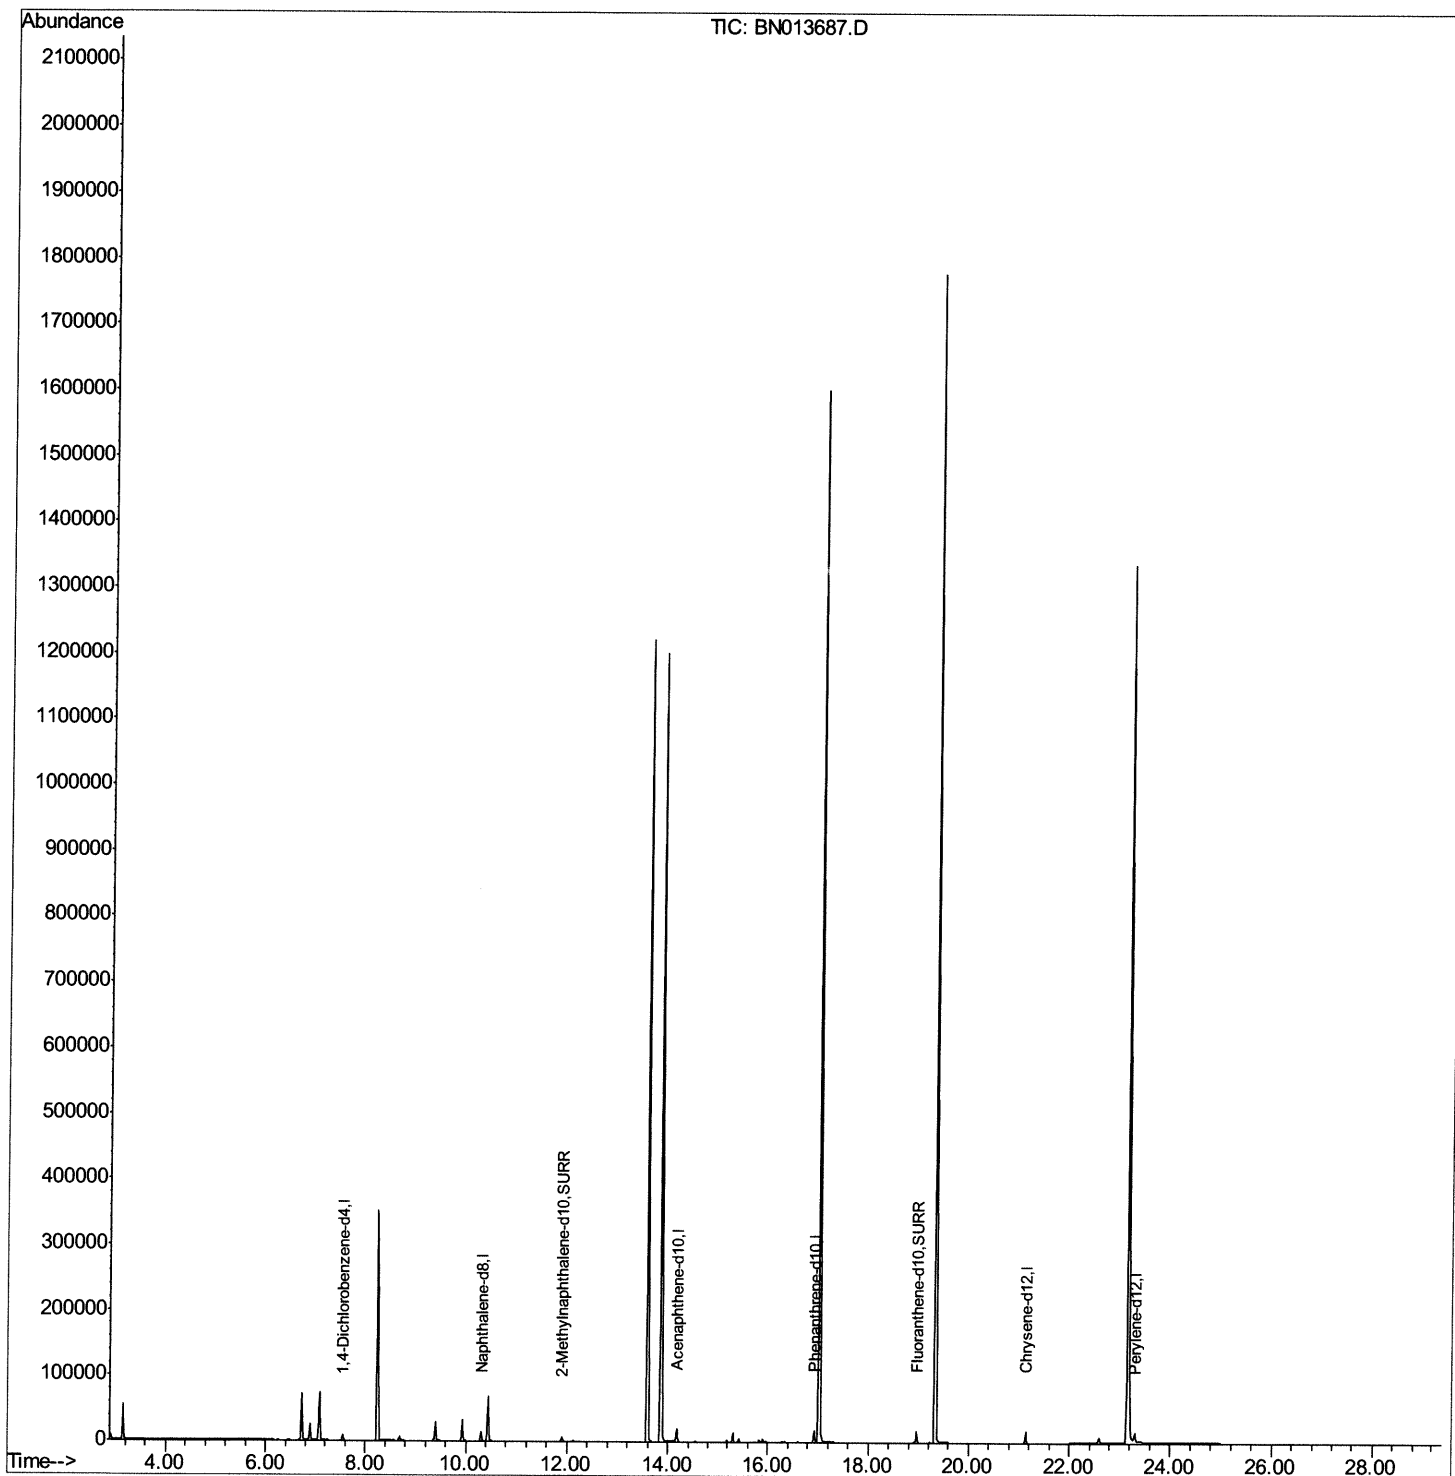

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
 Data File : BN013687.D
 Acq On : 20 Feb 2021 12:21
 Operator : CG/JU
 Sample : PB134659BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK59

Manual Integrations
APPROVED

mohammad
 2/22/2021 2:10:55 PM

Quant Time: Feb 22 02:35:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 02:30:08 2021
 Response via : Initial Calibration

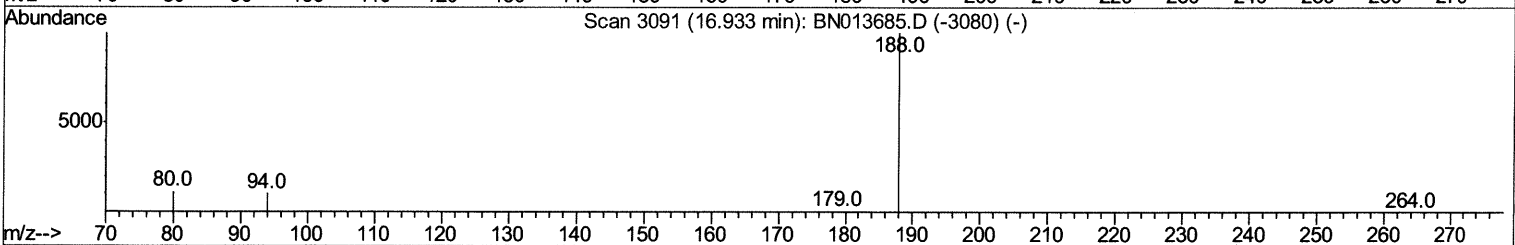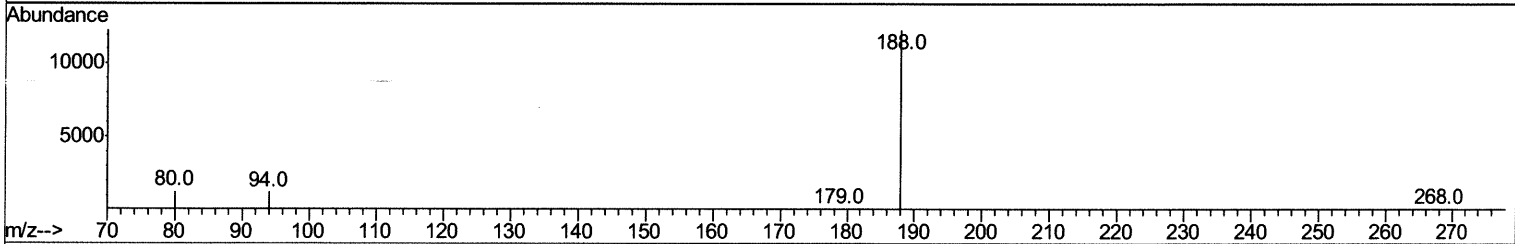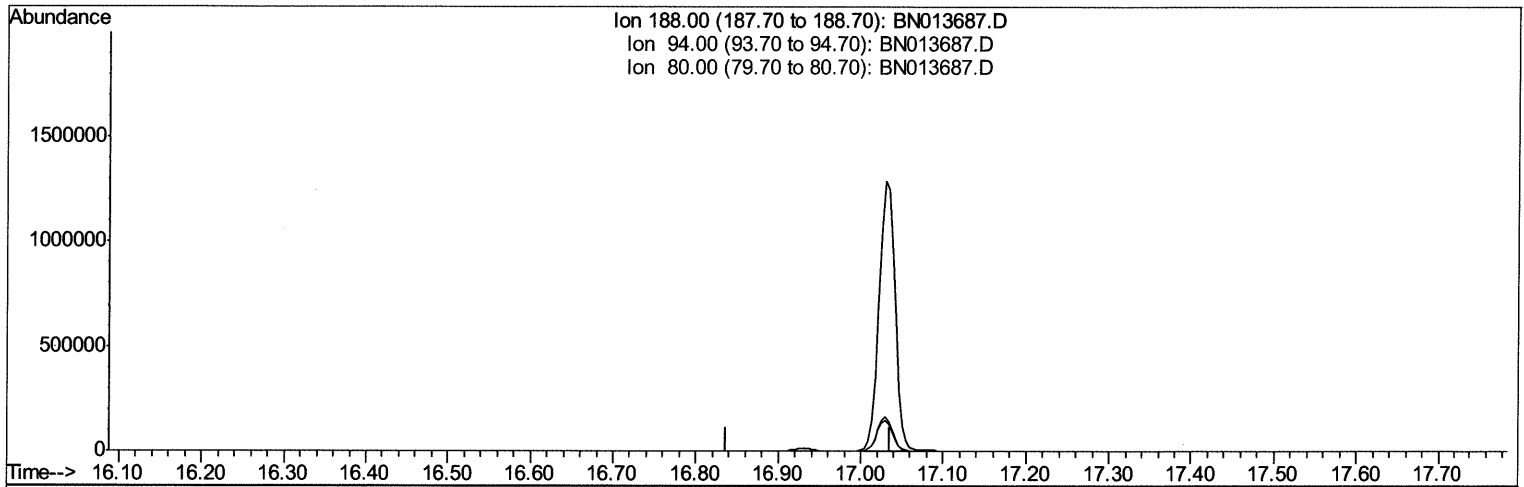

TIC: BN013687.D

(10) Phenanthrene-d10 (I)

16.937min (-16.937) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
 Data File : BN013687.D
 Acq On : 20 Feb 2021 12:21
 Operator : CG/JU
 Sample : PB134659BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK59

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:10:55 PM

Quant Time: Feb 22 02:35:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 02:30:08 2021
 Response via : Initial Calibration

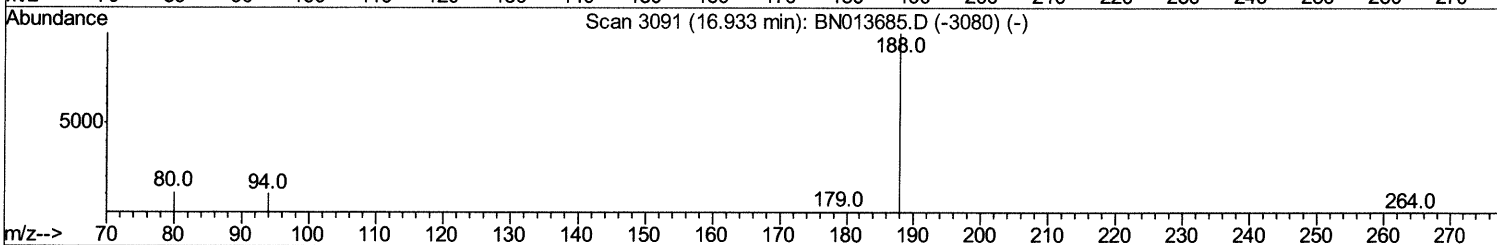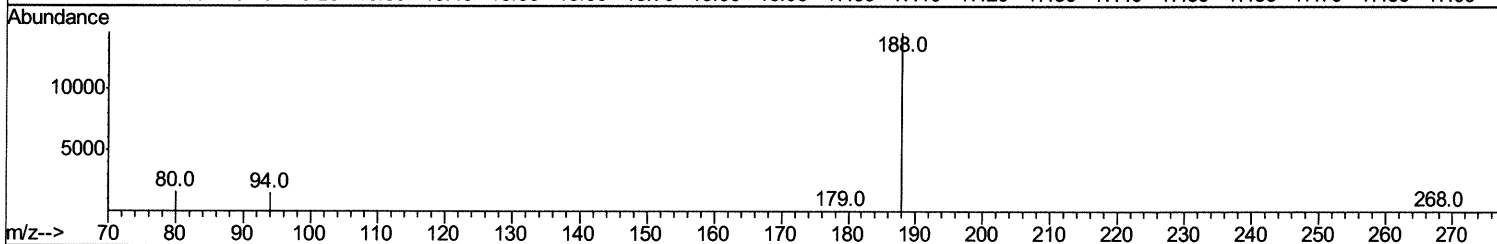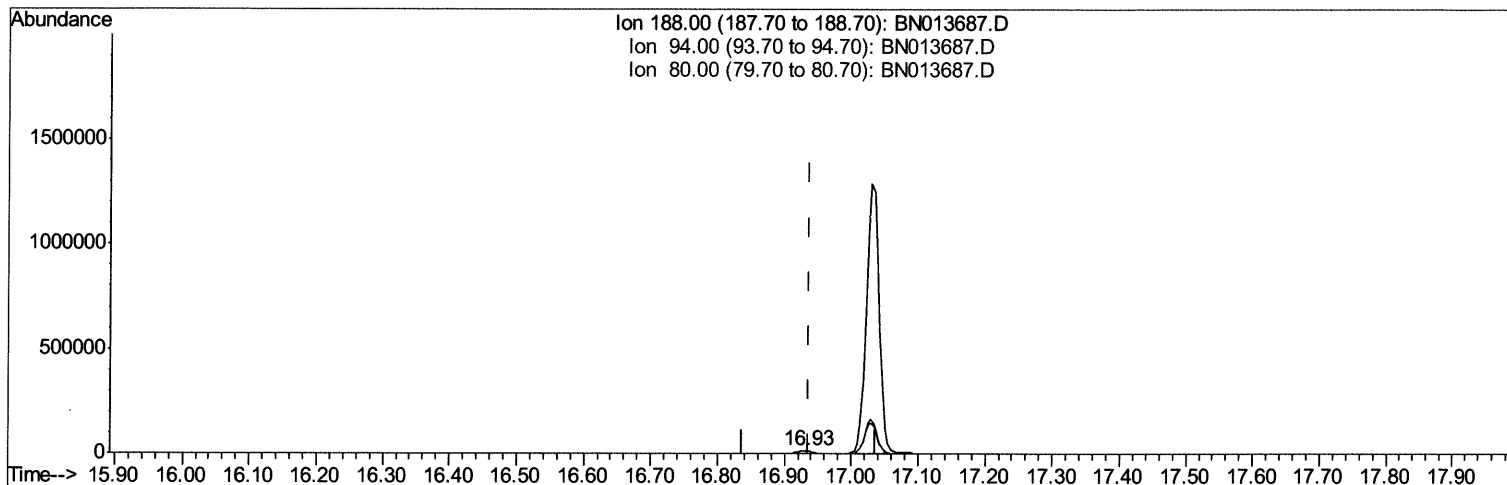

TIC: BN013687.D

(10) Phenanthrene-d10 (I)

16.933min (-0.004) 0.40ng/ul m 02/22/21 JU

response 20153

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	10.45
80.00	11.30	11.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
Data File : BN013687.D
Acq On : 20 Feb 2021 12:21
Operator : CG/JU
Sample : PB134659BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK59

Manual Integrations
APPROVED

mohammad
2/22/2021 2:10:55 PM

Quant Time: Feb 22 02:36:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 02:30:08 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	4539	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	17786	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	10400	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	20153m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.14	240	16553	0.40	ng/ul	0.00
20) Perylene-d12	23.30	264	16857	0.40	ng/ul	0.00

02/22/21 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.90	152	9941	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	19060	0.39	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed