


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
Data File : BN013688.D
Acq On : 20 Feb 2021 12:57
Operator : CG/JU
Sample : PB134731BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK31

Manual Integrations
APPROVED

mohammad
2/22/2021 2:10:57 PM

Quant Time: Feb 22 02:38:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 22 02:30:08 2021
Response via : Initial Calibration

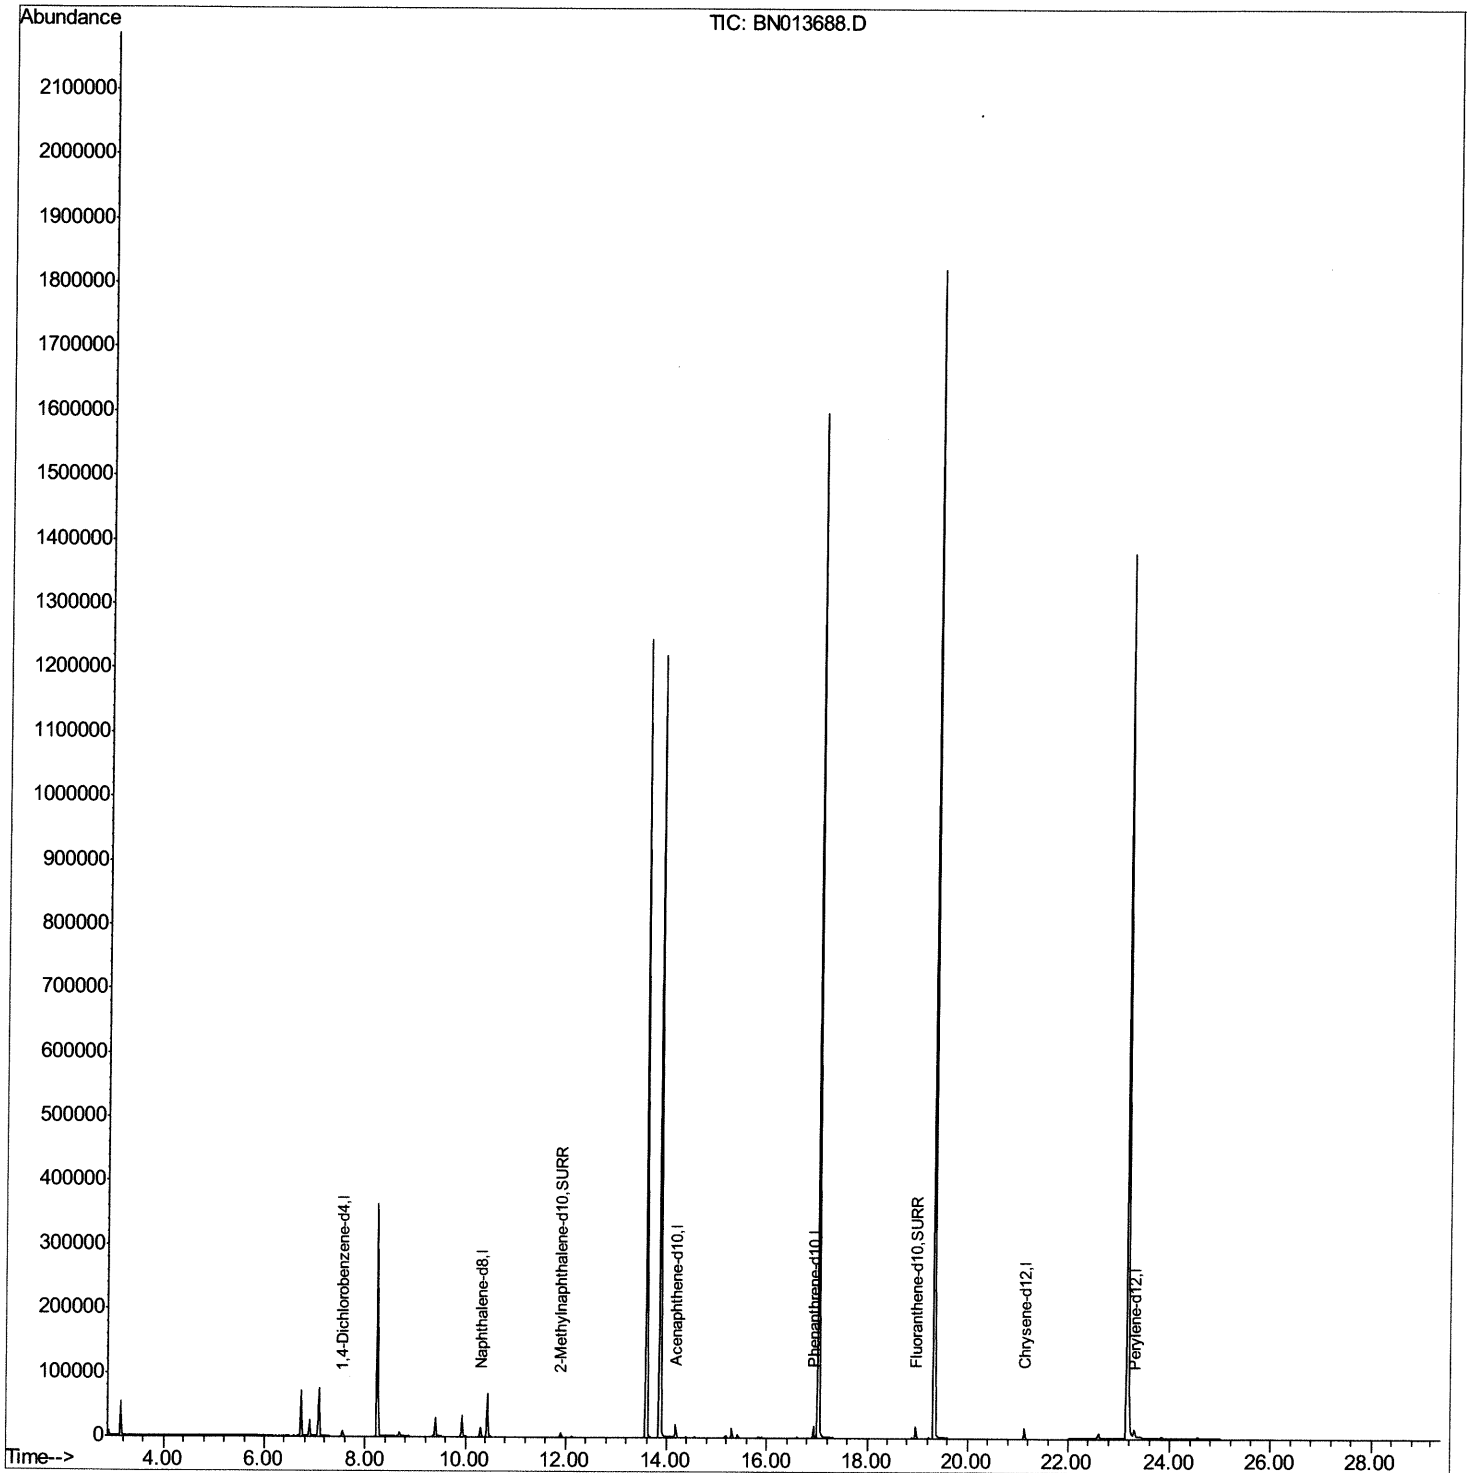

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
 Data File : BN013688.D
 Acq On : 20 Feb 2021 12:57
 Operator : CG/JU
 Sample : PB134731BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK31

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:10:57 PM

Quant Time: Feb 22 02:37:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 02:30:08 2021
 Response via : Initial Calibration

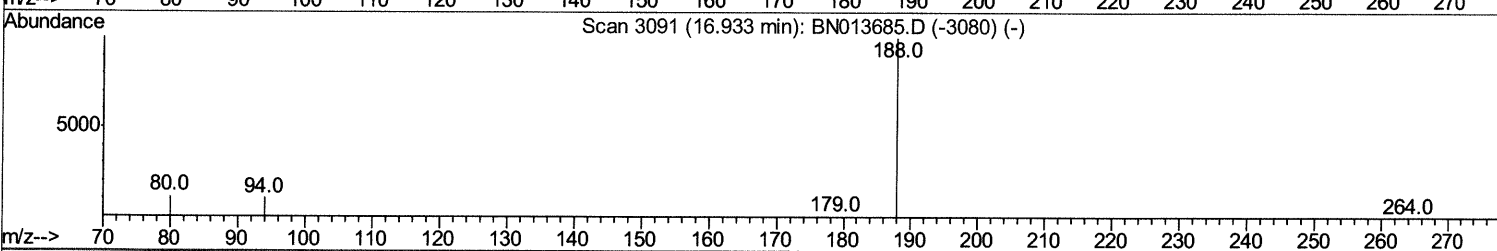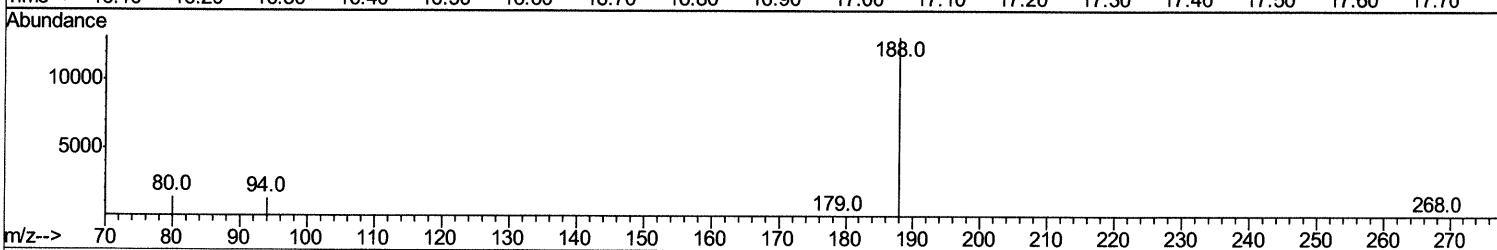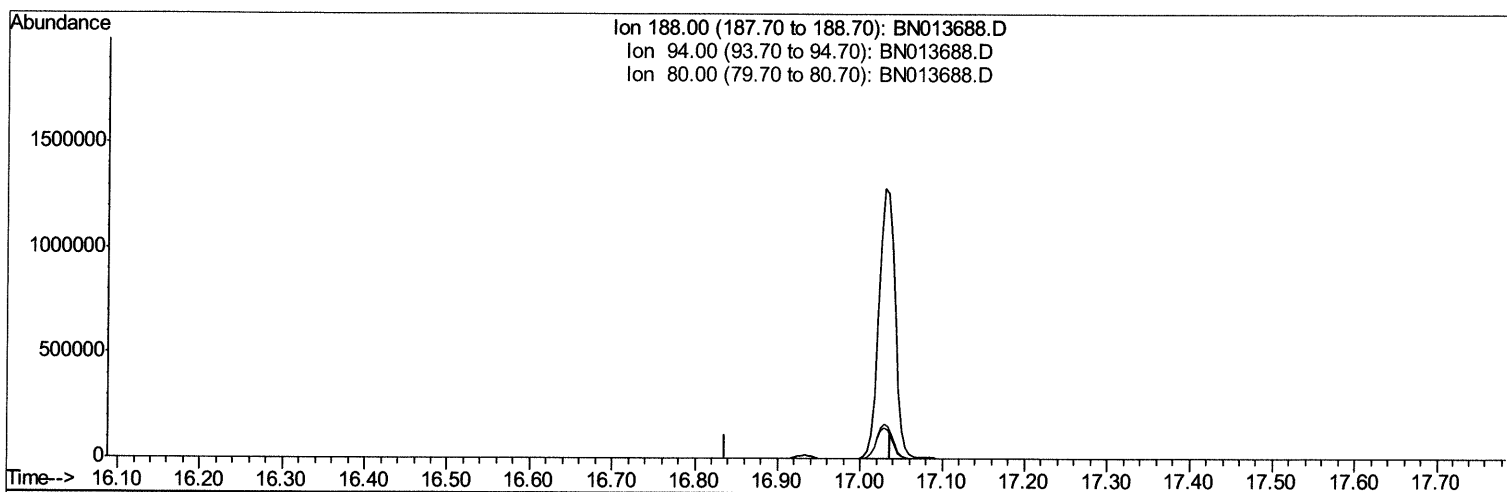

TIC: BN013688.D

(10) Phenanthrene-d10 (I)

16.937min (-16.937) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
 Data File : BN013688.D
 Acq On : 20 Feb 2021 12:57
 Operator : CG/JU
 Sample : PB134731BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK31

Manual Integrations
APPROVED

mohammad
 2/22/2021 2:10:57 PM

Quant Time: Feb 22 02:37:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 02:30:08 2021
 Response via : Initial Calibration

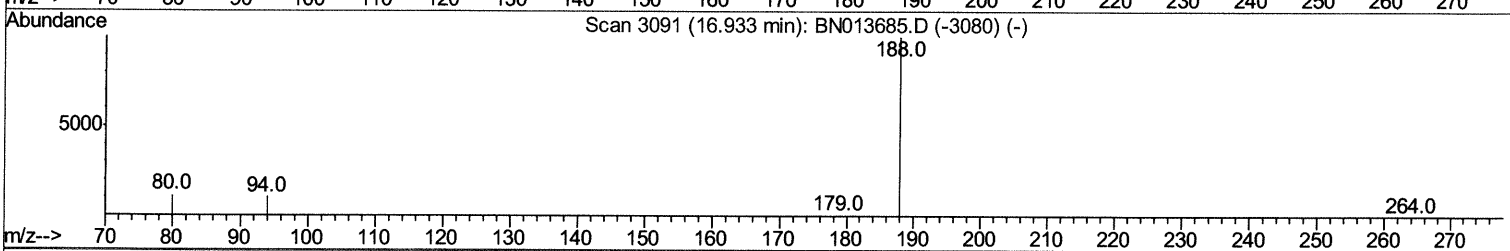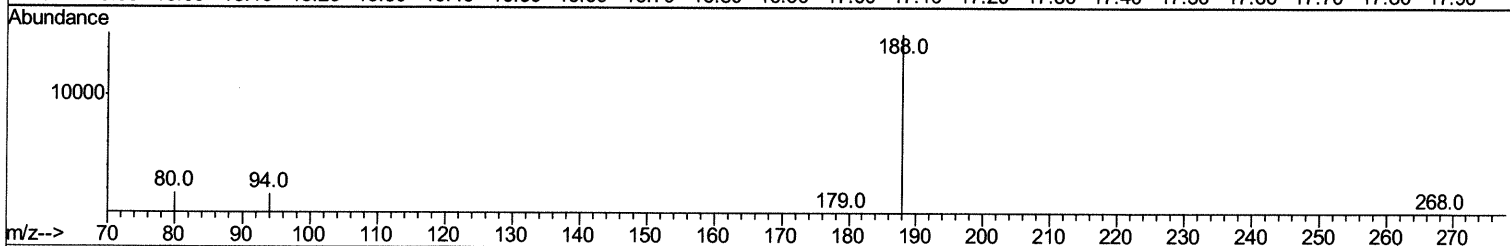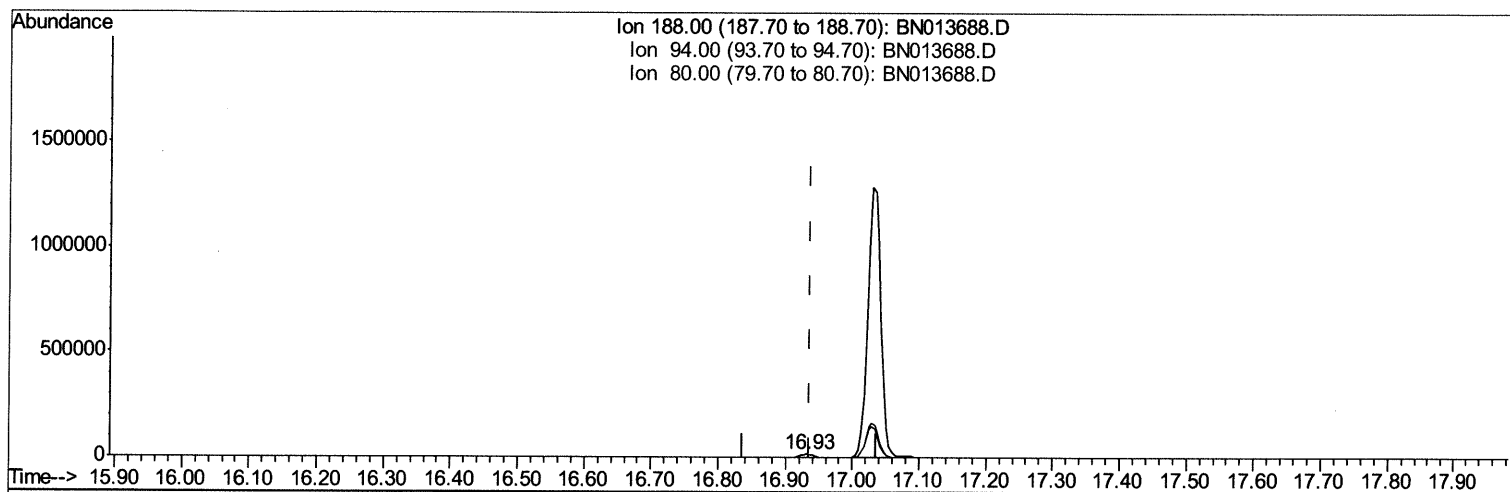

TIC: BN013688.D

(10) Phenanthrene-d10 (I)

16.932min (-0.004) 0.40ng/ul m 02/22/21JU

response 20490

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	10.75
80.00	11.30	11.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN022021\
 Data File : BN013688.D
 Acq On : 20 Feb 2021 12:57
 Operator : CG/JU
 Sample : PB134731BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK31

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:10:57 PM

Quant Time: Feb 22 02:38:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 22 02:30:08 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	4628	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	18028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	10508	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	20490m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.14	240	16360	0.40	ng/ul	0.00
20) Perylene-d12	23.30	264	17473	0.40	ng/ul	0.00

02/22/2021

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.90	152	10057	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	19374	0.39	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed