
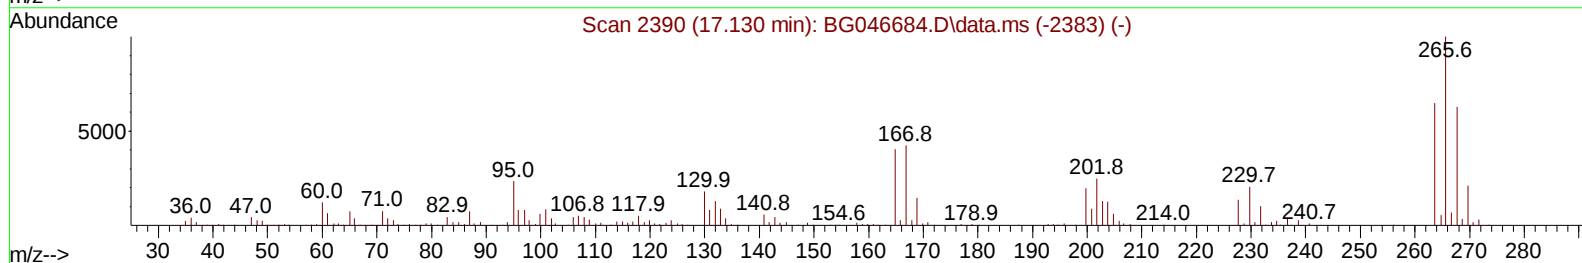
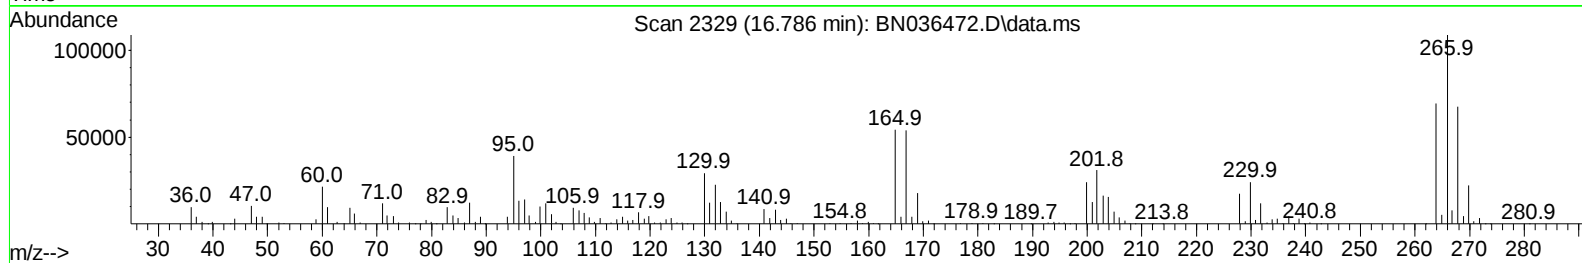


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022025\
Data File : BN036472.D
Acq On : 20 Feb 2025 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 02:03:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

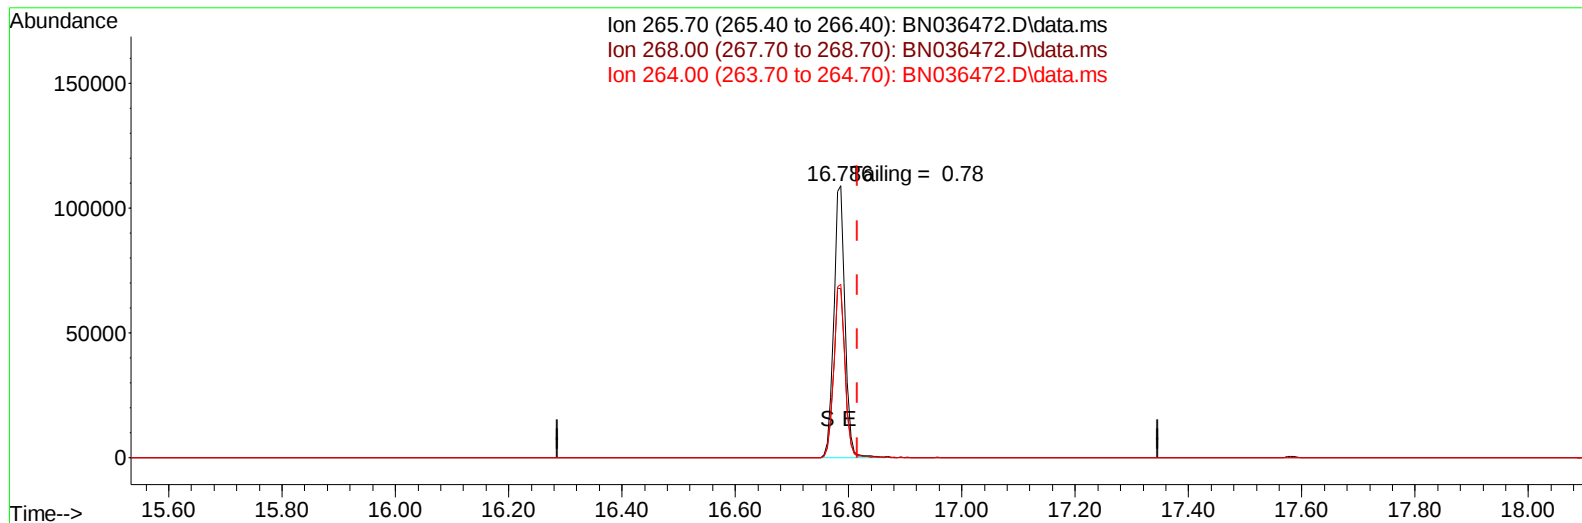

TIC: BN036472.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.030) 19225.56 ng

response 150123

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.22
264.00	61.60	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022025\
Data File : BN036472.D
Acq On : 20 Feb 2025 09:32
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 02:03:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

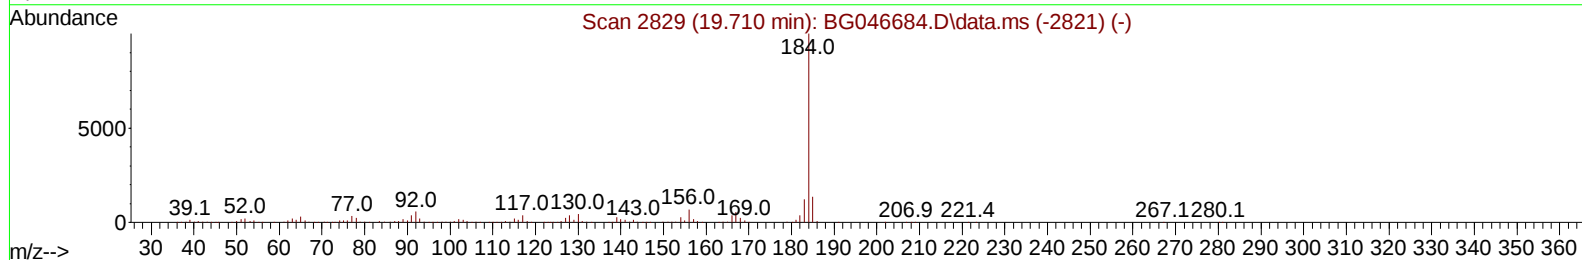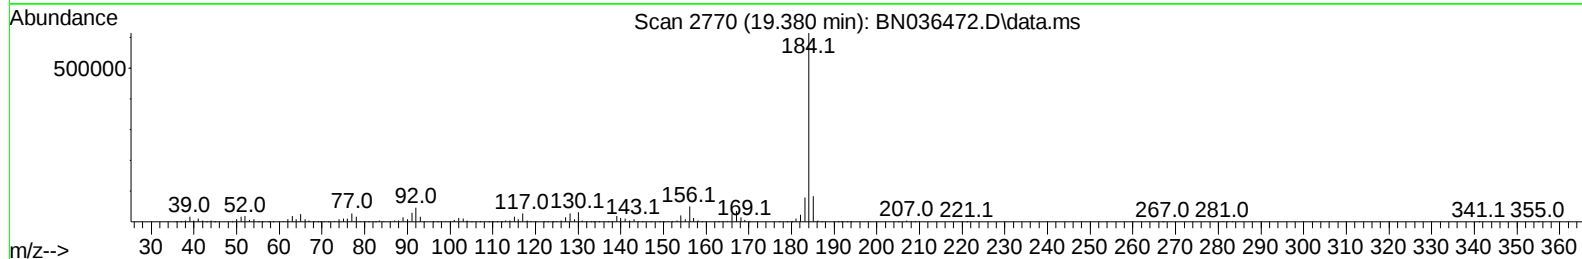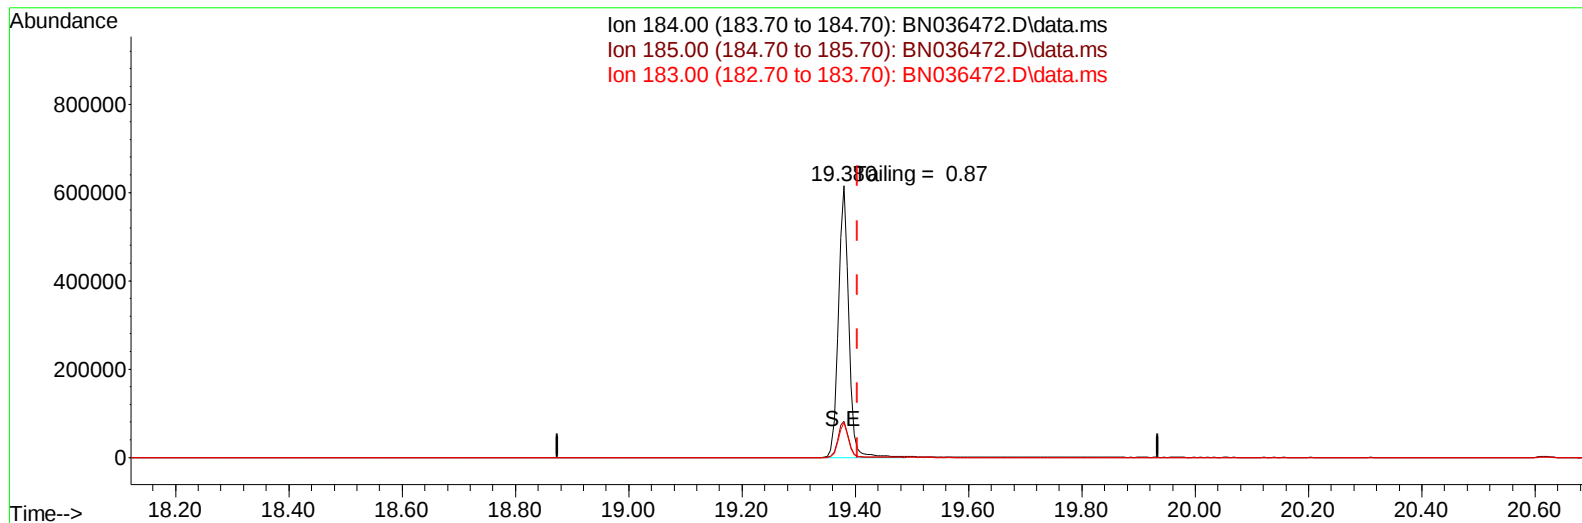

TIC: BN036472.D\data.ms

(77) Benzidine**19.380min (-0.024) 0.00 ng****response 787833**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.45
183.00	13.20	12.84
0.00	0.00	0.00