




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Manual IntegrationsAPPROVED

Quant Time: Feb 22 01:04:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

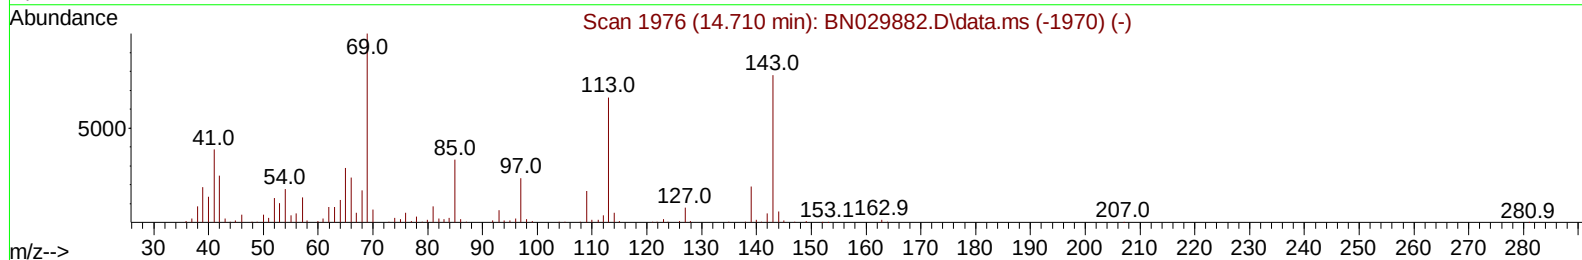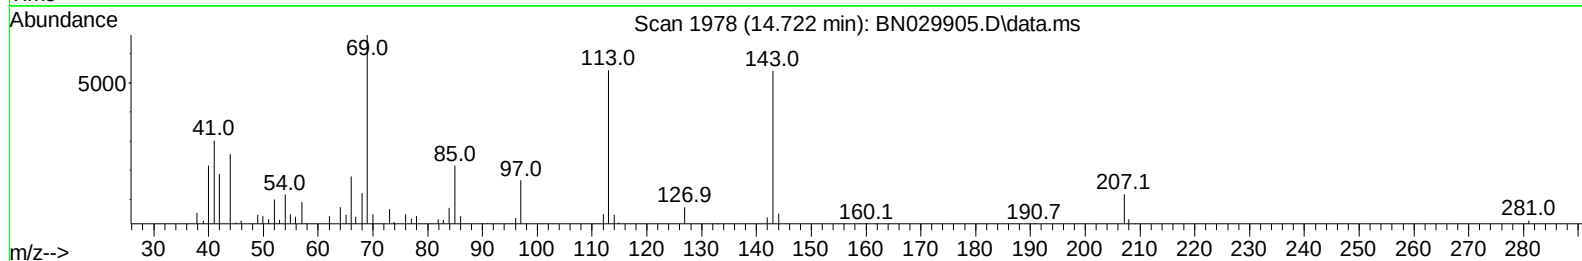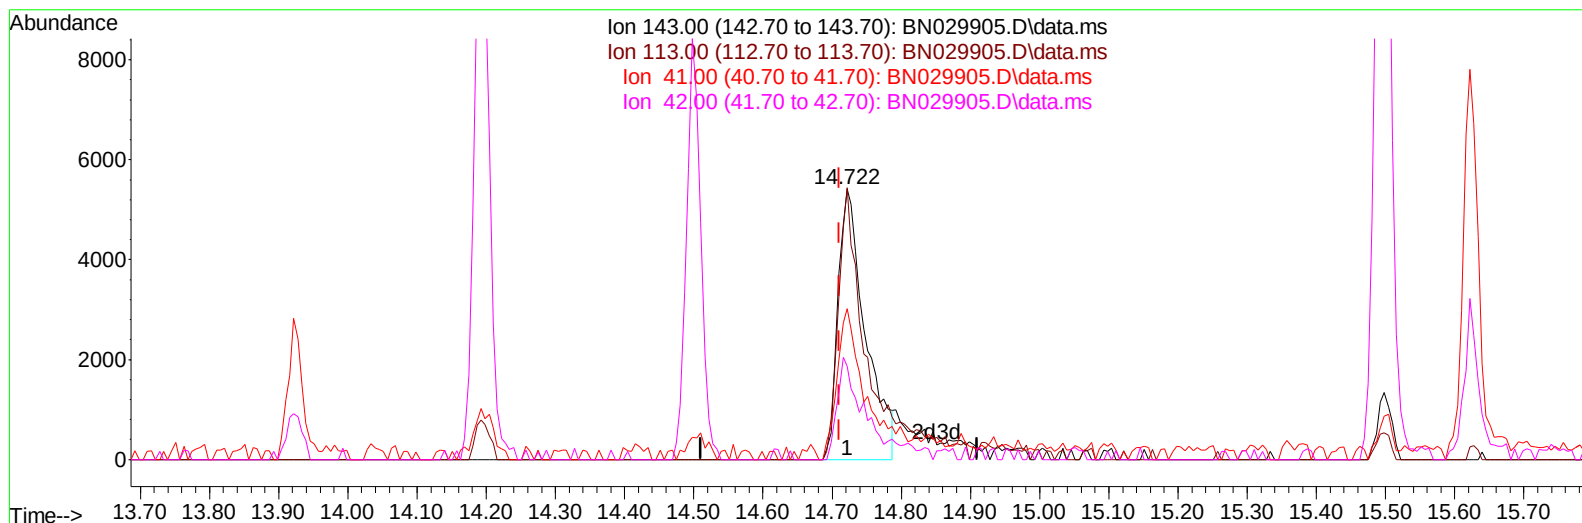

TIC: BN029905.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 3.46 ng/ul

response 14831

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	100.30
41.00	45.90	55.65#
42.00	28.40	34.50#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029905.D
 Acq On : 22 Feb 2024 00:38
 Operator : MA/JU
 Sample : P1493-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W9

Manual IntegrationsAPPROVED

Quant Time: Feb 22 01:04:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

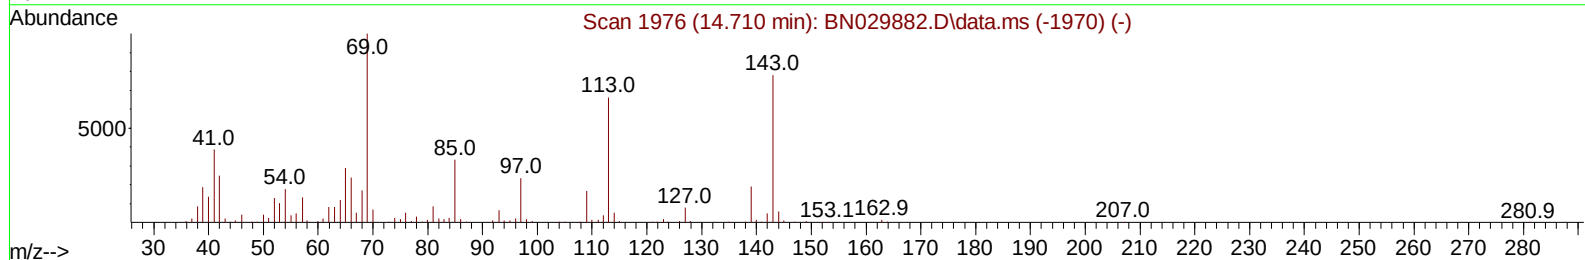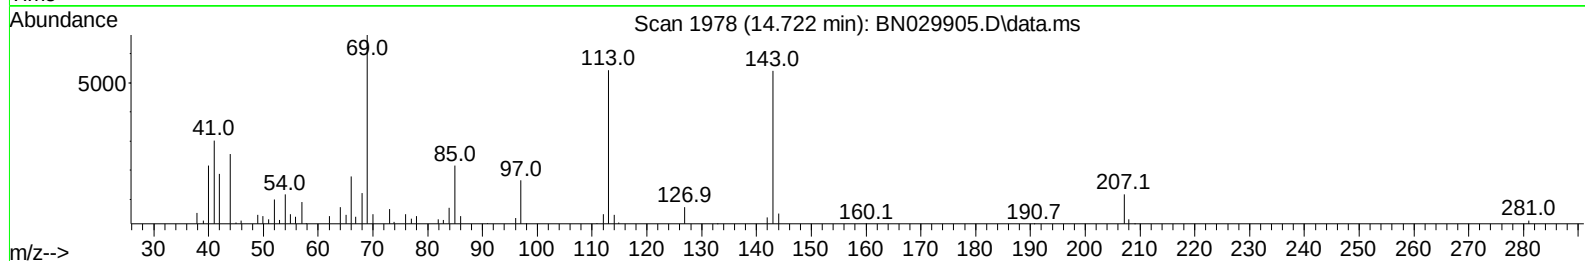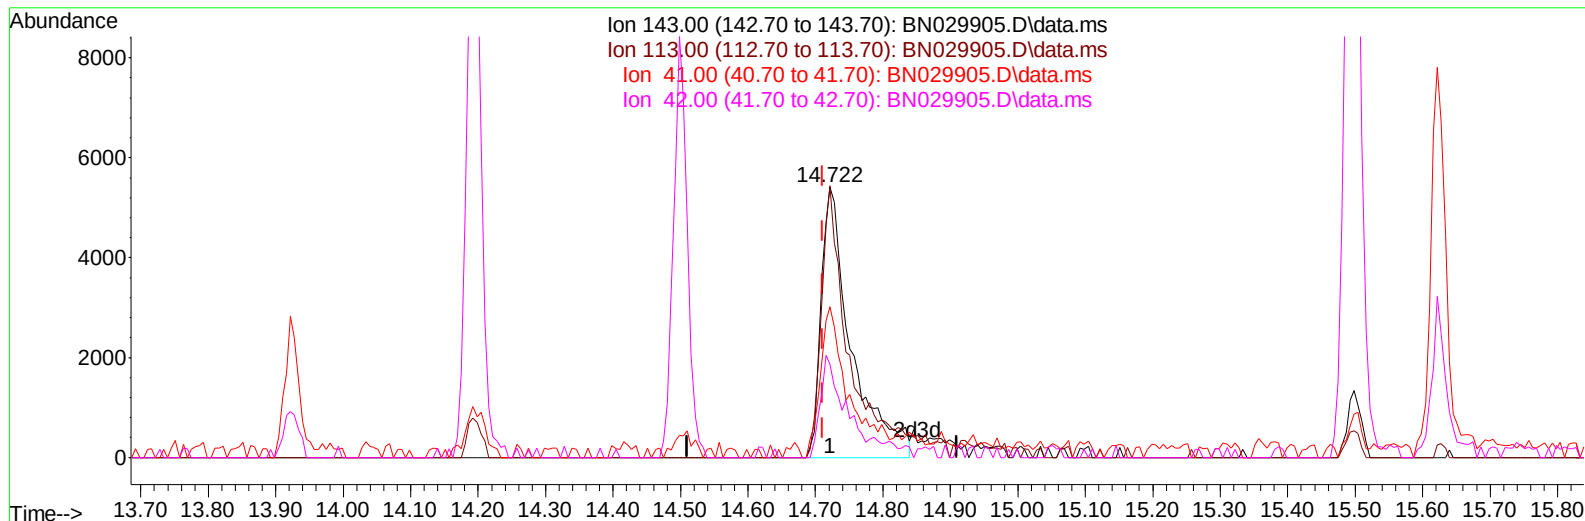

TIC: BN029905.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 3.92 ng/ul m

response 16773

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	100.30
41.00	45.90	55.65#
42.00	28.40	34.50#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029905.D
 Acq On : 22 Feb 2024 00:38
 Operator : MA/JU
 Sample : P1493-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 01:04:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	137940	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	563965	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	303065	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	646147	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	536860	20.000	ng/ul	0.00
88) Perylene-d12	23.815	264	585836	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	15847	3.779	ng/uL	0.00
4) Pyridine-d5	3.746	84	40434	3.615	ng/ul	0.02
7) Phenol-d5	7.028	99	90307	6.999	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	335619	38.976	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	292069	31.239	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	171530	17.826	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	188806	43.135	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	175076	45.926	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	285944	38.002	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	316032	24.619	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	928511	41.151	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1132498	42.264	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	16773m	3.917	ng/ul	0.01
60) Fluorene-d10	15.498	176	838194	43.667	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	98066	31.148	ng/ul	0.00
73) Anthracene-d10	17.351	188	1332103	43.990	ng/ul	0.00
81) Pyrene-d10	19.651	212	1468781	45.590	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1355422	46.237	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 01:04:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

