




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029907.D
Acq On : 22 Feb 2024 01:50
Operator : MA/JU
Sample : P1493-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X1

Manual IntegrationsAPPROVED

Quant Time: Feb 22 02:31:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

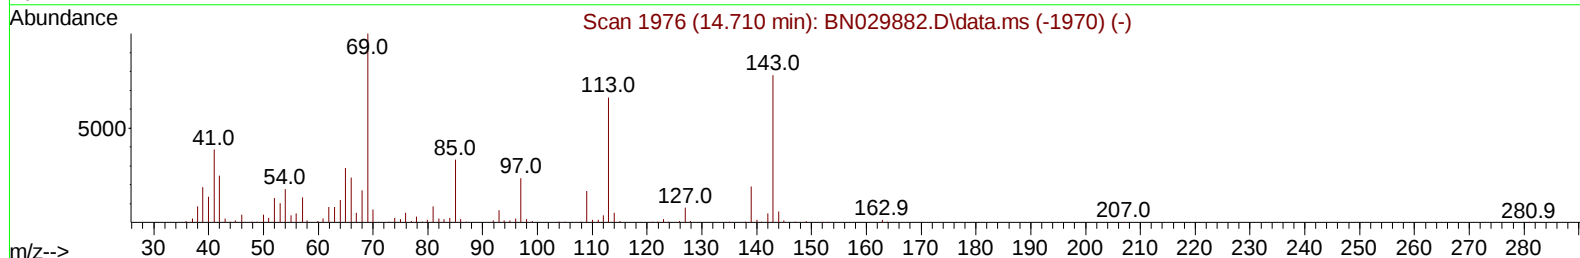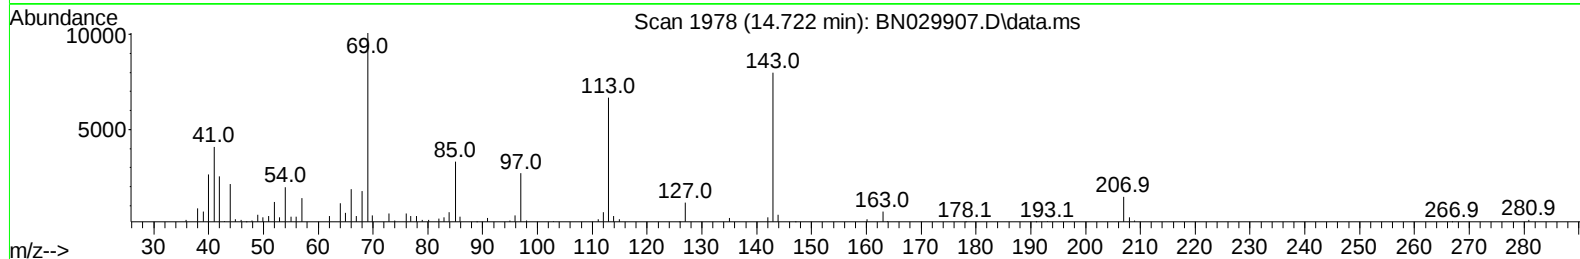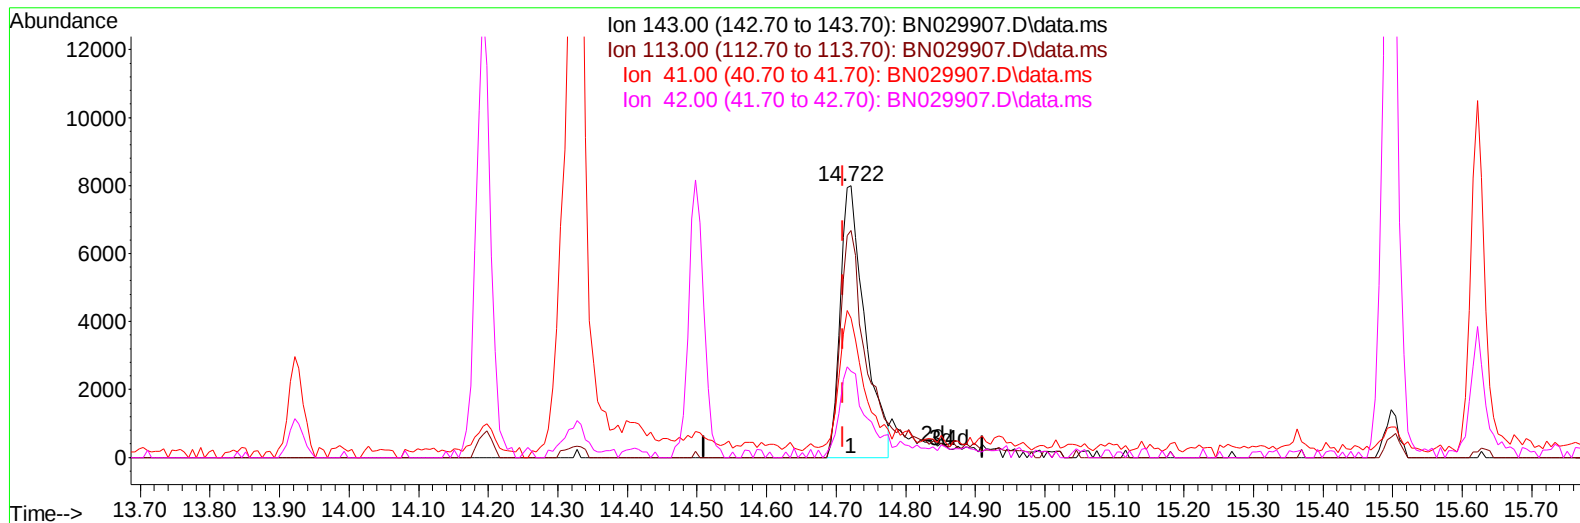

TIC: BN029907.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 4.52 ng/u1

response 19454

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	83.68
41.00	45.90	51.21
42.00	28.40	31.79




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029907.D
Acq On : 22 Feb 2024 01:50
Operator : MA/JU
Sample : P1493-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X1

Manual IntegrationsAPPROVED

Quant Time: Feb 22 02:31:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

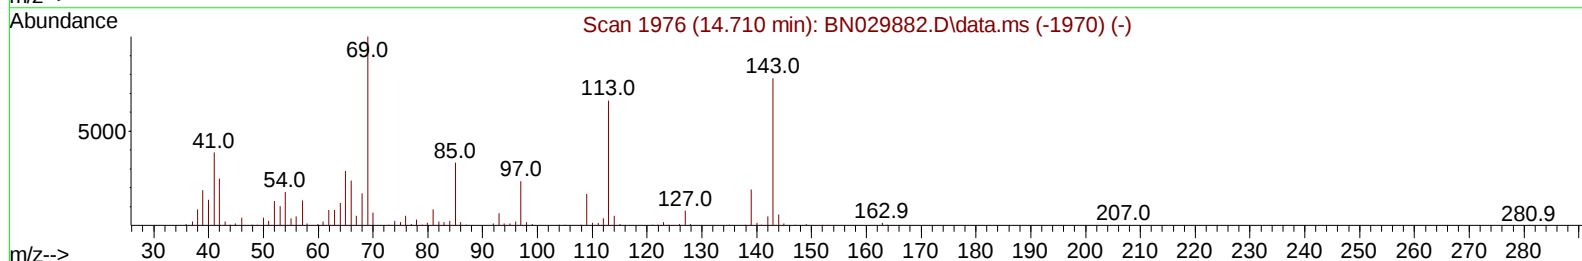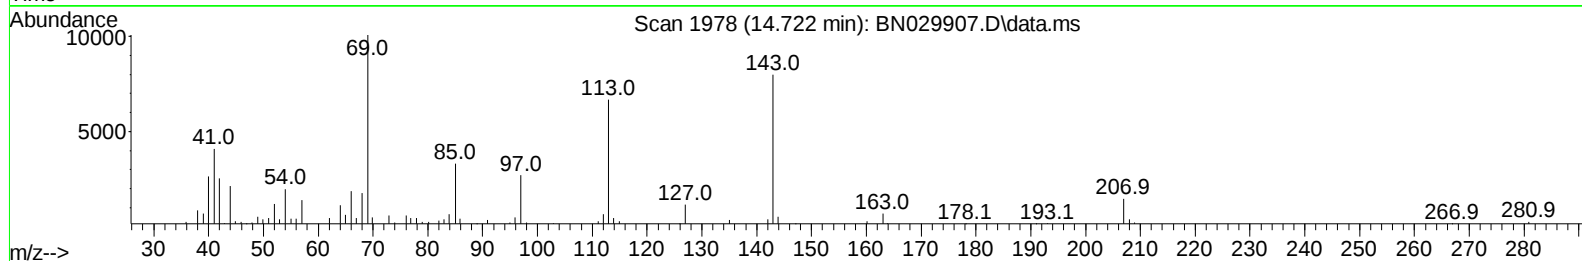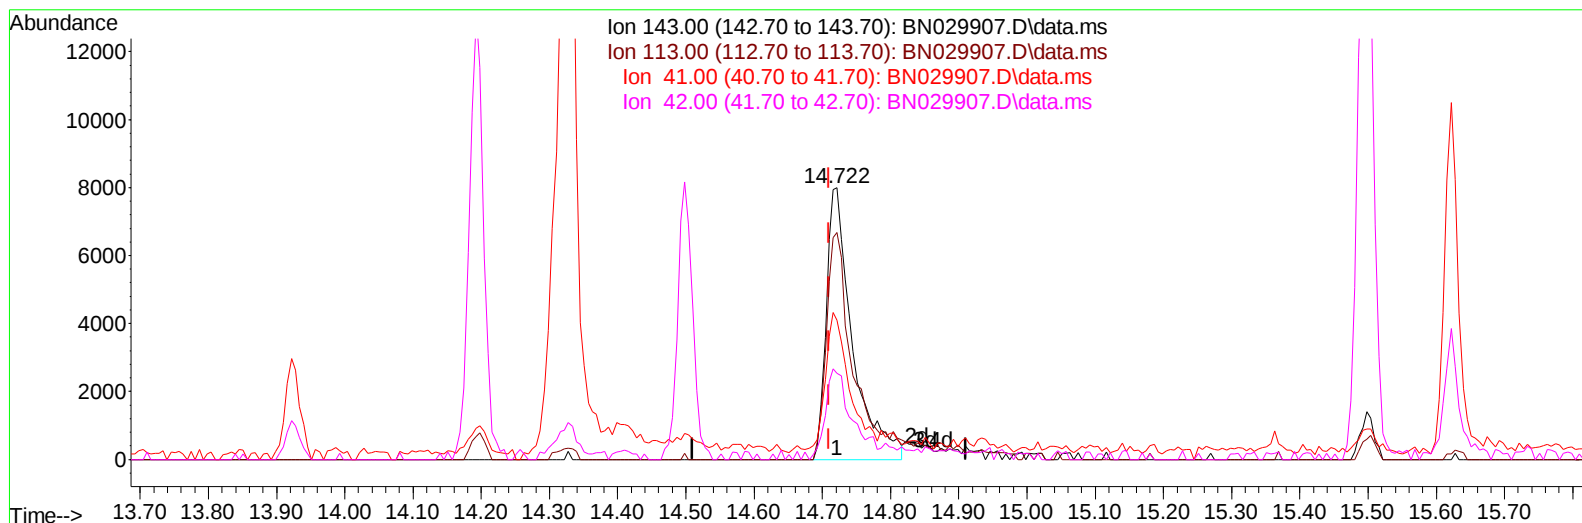

TIC: BN029907.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 4.93 ng/ul m

response 21201

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	83.68
41.00	45.90	51.21
42.00	28.40	31.79

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029907.D
 Acq On : 22 Feb 2024 01:50
 Operator : MA/JU
 Sample : P1493-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3X1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 02:32:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	140584	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	571069	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	304397	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	630643	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	563298	20.000	ng/ul	0.00
88) Perylene-d12	23.810	264	644926	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	16829	3.937	ng/uL	0.00
4) Pyridine-d5	3.734	84	69054	6.058	ng/ul	0.00
7) Phenol-d5	7.028	99	91211	6.936	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	358552	40.856	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	308751	32.402	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	176322	17.980	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	200260	45.183	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	193427	50.109	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	314802	41.316	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	392470	30.193	ng/ul	0.00
46) Dimethylphthalate-d6	13.928	166	1044201	46.076	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1260150	46.822	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	21201m	4.929	ng/ul	0.01
60) Fluorene-d10	15.498	176	936568	48.579	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	117929	38.378	ng/ul	0.00
73) Anthracene-d10	17.351	188	1493262	50.524	ng/ul	0.00
81) Pyrene-d10	19.651	212	1713169	50.680	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.662	264	1612038	49.953	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029907.D
Acq On : 22 Feb 2024 01:50
Operator : MA/JU
Sample : P1493-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 02:32:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

