




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 04:03:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

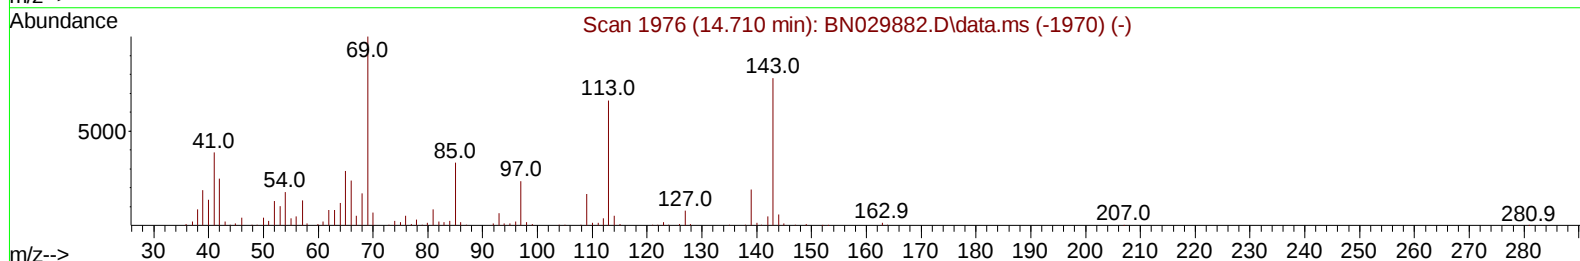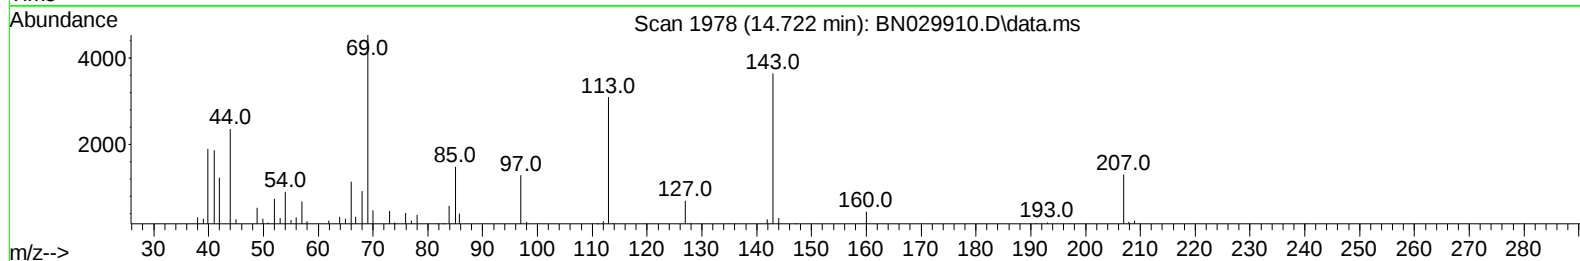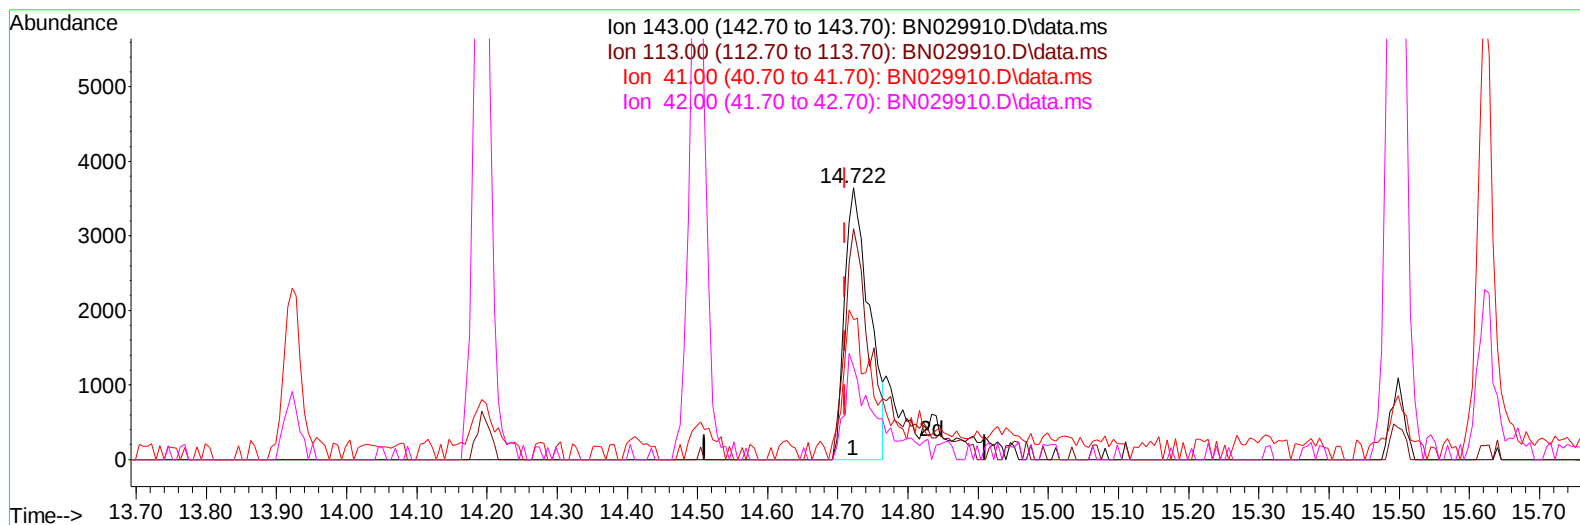

TIC: BN029910.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 2.05 ng/u1

response 8855

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	84.99
41.00	45.90	51.51
42.00	28.40	34.03




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 04:03:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

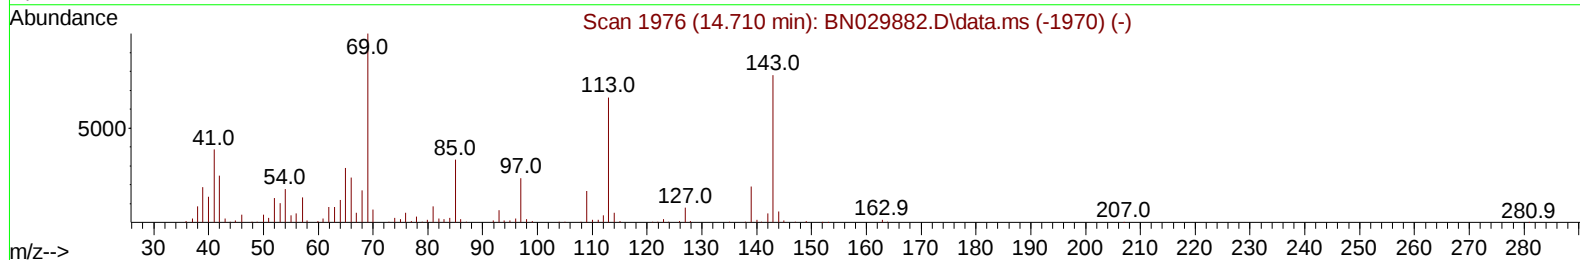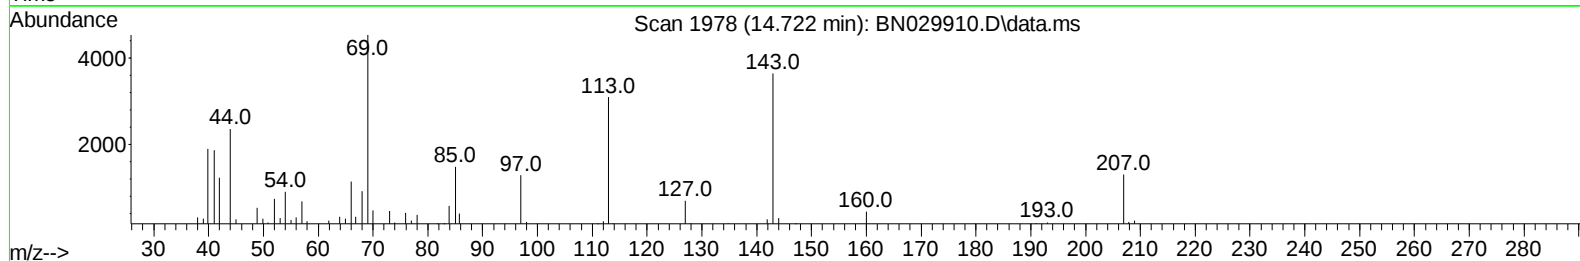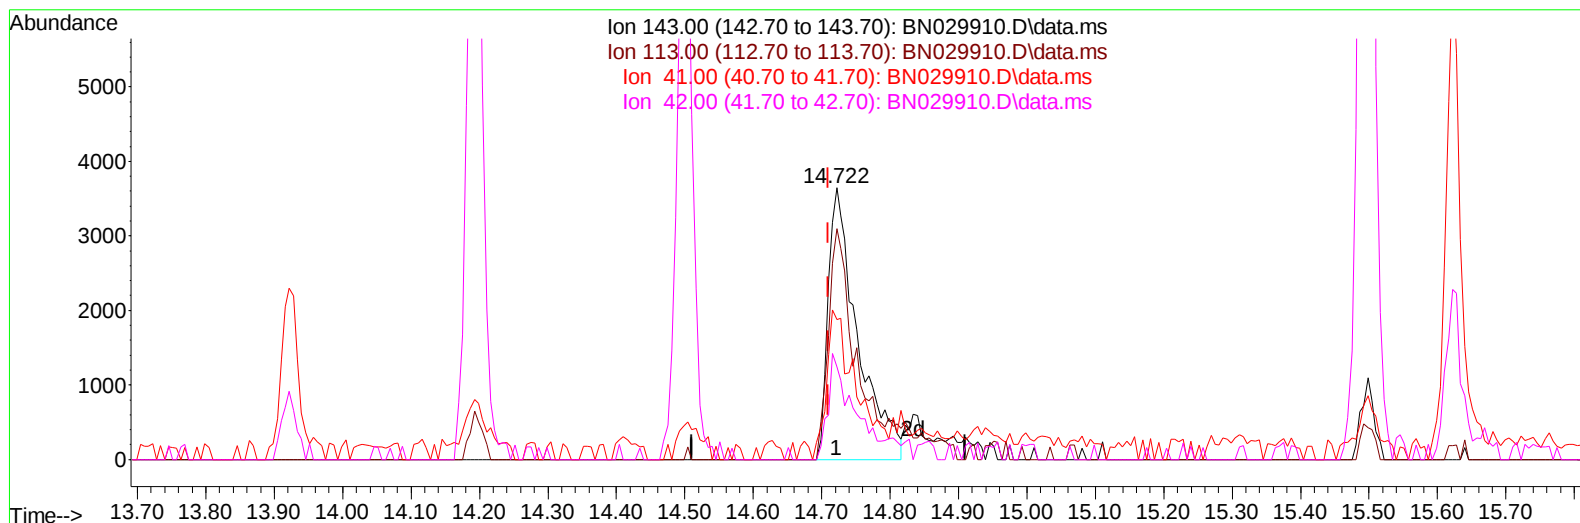

TIC: BN029910.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (+ 0.012) 2.52 ng/ul m

response 10871

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	84.99
41.00	45.90	51.51
42.00	28.40	34.03

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029910.D
 Acq On : 22 Feb 2024 03:38
 Operator : MA/JU
 Sample : P1493-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 04:05:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.858	152		141699	20.000	ng/ul	0.00
20) Naphthalene-d8	10.652	136		579847	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164		305555	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188		619933	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240		520020	20.000	ng/ul	0.00
88) Perylene-d12	23.816	264		571452	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.317	96		17323	4.021	ng/uL	0.00
4) Pyridine-d5	3.734	84		78199	6.806	ng/ul	0.00
7) Phenol-d5	7.028	99		71339	5.382	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67		297416	33.623	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132		246316	25.646	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113		135422	13.700	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128		161414	35.867	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143		147034	37.514	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165		243271	31.445	ng/ul	0.00
31) 4-Chloroaniline-d4	10.799	131		438269	33.206	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166		824635	36.250	ng/ul	0.00
49) Acenaphthylene-d8	14.193	160		989018	36.609	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143		10871m	2.518	ng/ul	0.01
60) Fluorene-d10	15.498	176		713413	36.864	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200		76278	25.252	ng/ul	0.00
73) Anthracene-d10	17.351	188		1080571	37.192	ng/ul	0.00
81) Pyrene-d10	19.651	212		1201413	38.498	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.669	264		1082911	37.871	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 04:05:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

