




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029911.D
 Acq On : 22 Feb 2024 04:14
 Operator : MA/JU
 Sample : P1493-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W5

Manual Integrations APPROVED

Quant Time: Feb 22 05:18:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

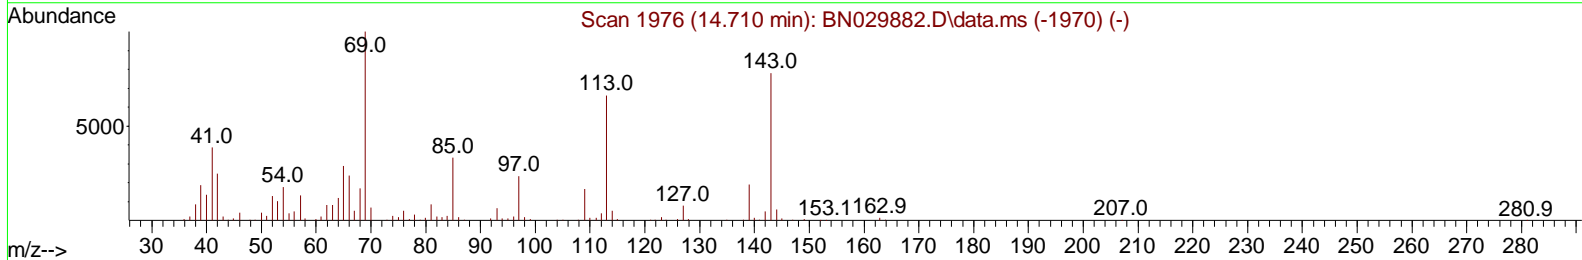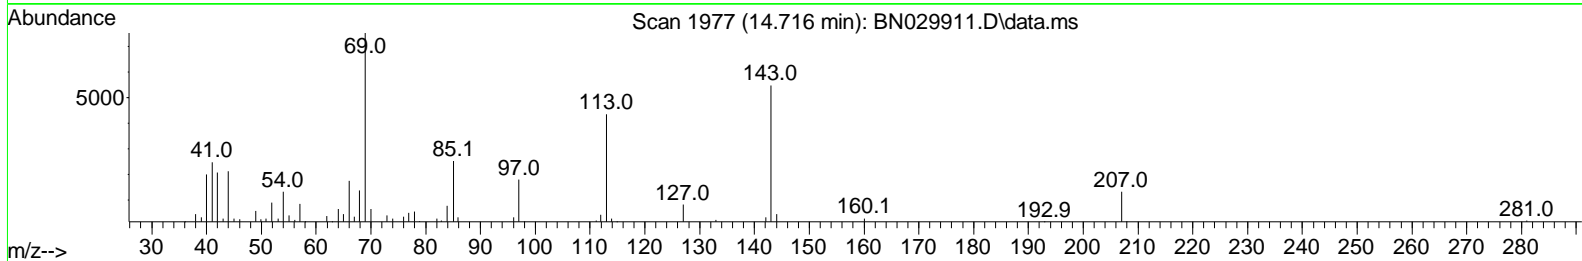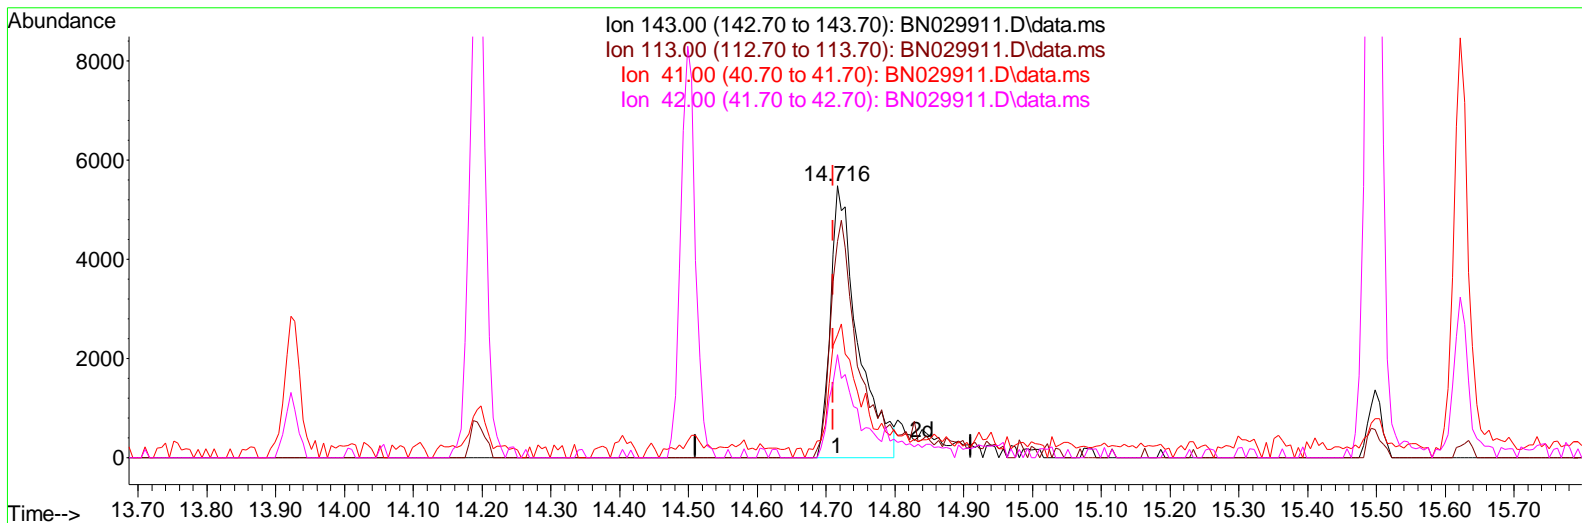

TIC: BN029911.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.006) 3.43 ng/ul

response 14920

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	79.46
41.00	45.90	45.21
42.00	28.40	37.94#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029911.D
 Acq On : 22 Feb 2024 04:14
 Operator : MA/JU
 Sample : P1493-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W5

Manual Integrations APPROVED

Quant Time: Feb 22 05:18:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

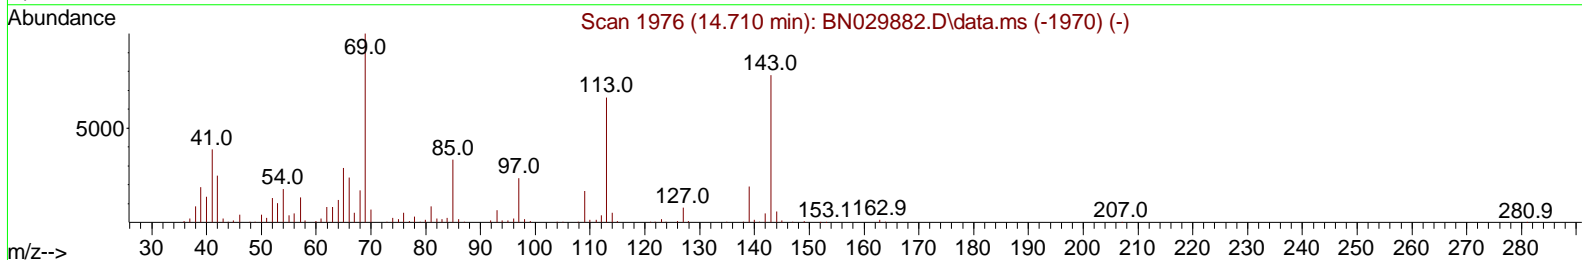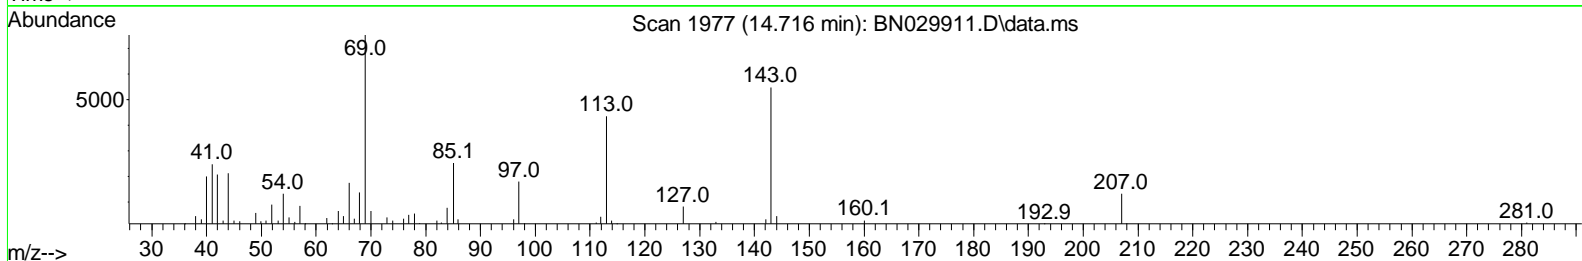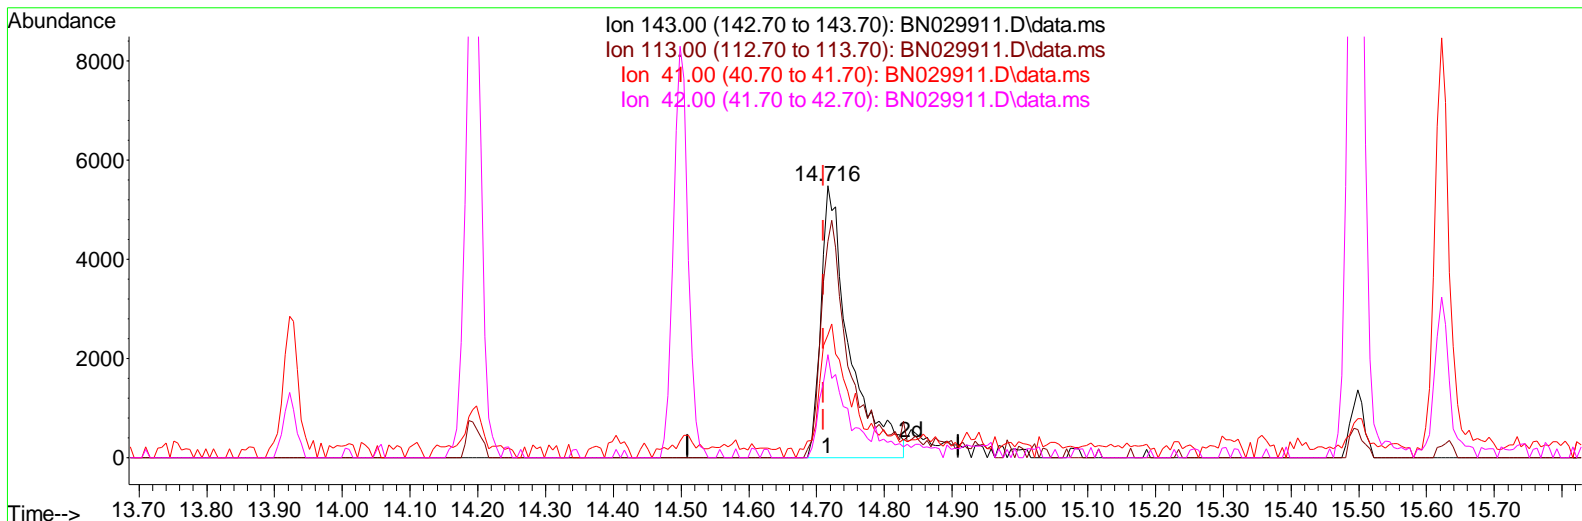

TIC: BN029911.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.006) 3.64 ng/ul m

response	15872	
Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	79.46
41.00	45.90	45.21
42.00	28.40	37.94#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BNO22124\
 Data File : BNO29911.D
 Acq On : 22 Feb 2024 04:14
 Operator : MA/JU
 Sample : P1493-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 BH3W5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 05:19:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BNO20724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	143196	20.000	ng/ul	0.00
20) Naphthalene-d8	10.652	136	581792	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	308246	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	654358	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	564736	20.000	ng/ul	0.00
88) Perylene-d12	23.816	264	638298	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	16126	3.704	ng/uL	0.00
4) Pyridine-d5	3.734	84	84905	7.313	ng/ul	0.00
7) Phenol-d5	7.028	99	84015	6.273	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	324362	36.286	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	282422	29.098	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	162779	16.296	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	185769	41.141	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	167207	42.518	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	281232	36.230	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	390912	29.519	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	973695	42.428	ng/ul	0.00
49) Acenaphthylene-d8	14.193	160	1155981	42.415	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	15872m	3.644	ng/ul	0.00
60) Fluorene-d10	15.498	176	866157	44.365	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	98769	30.977	ng/ul	0.00
73) Anthracene-d10	17.351	188	1388675	45.282	ng/ul	0.00
81) Pyrene-d10	19.651	212	1572157	46.390	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	1448672	45.357	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029911.D
 Acq On : 22 Feb 2024 04:14
 Operator : MA/JU
 Sample : P1493-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 BH3W5

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 02/22/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 05:19:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

