




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 13:03:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/23/2024
Supervised By :mohammad ahmed 02/24/2024

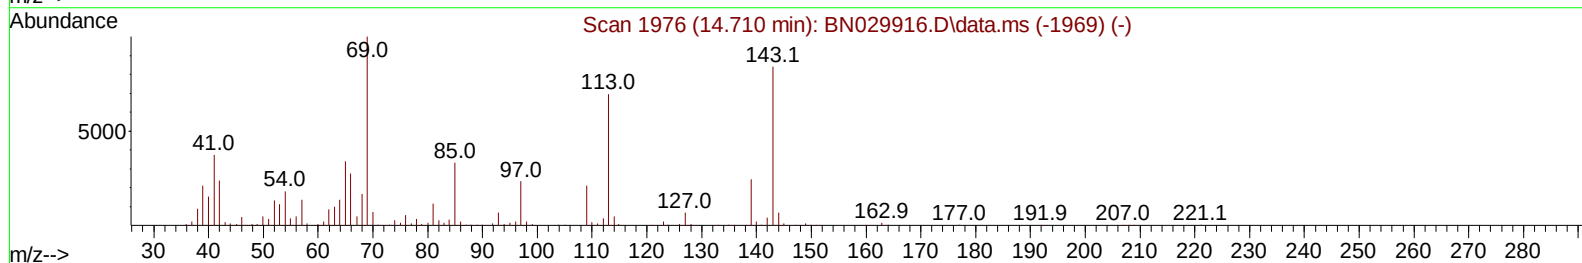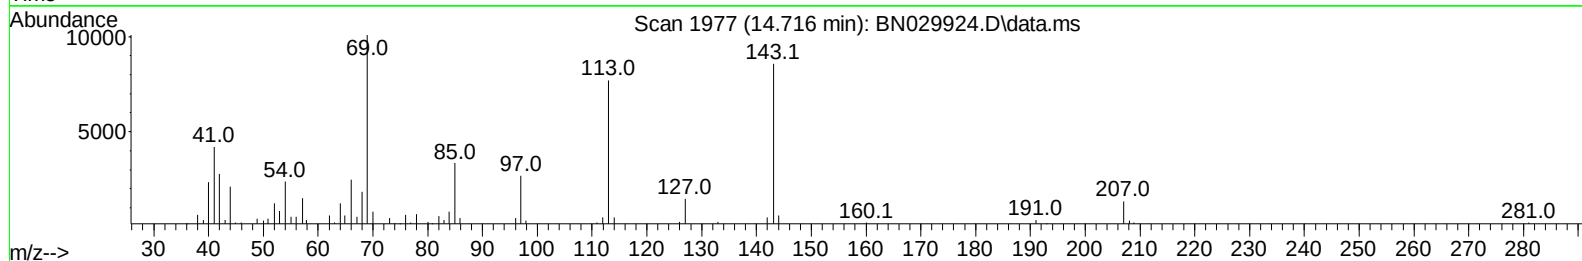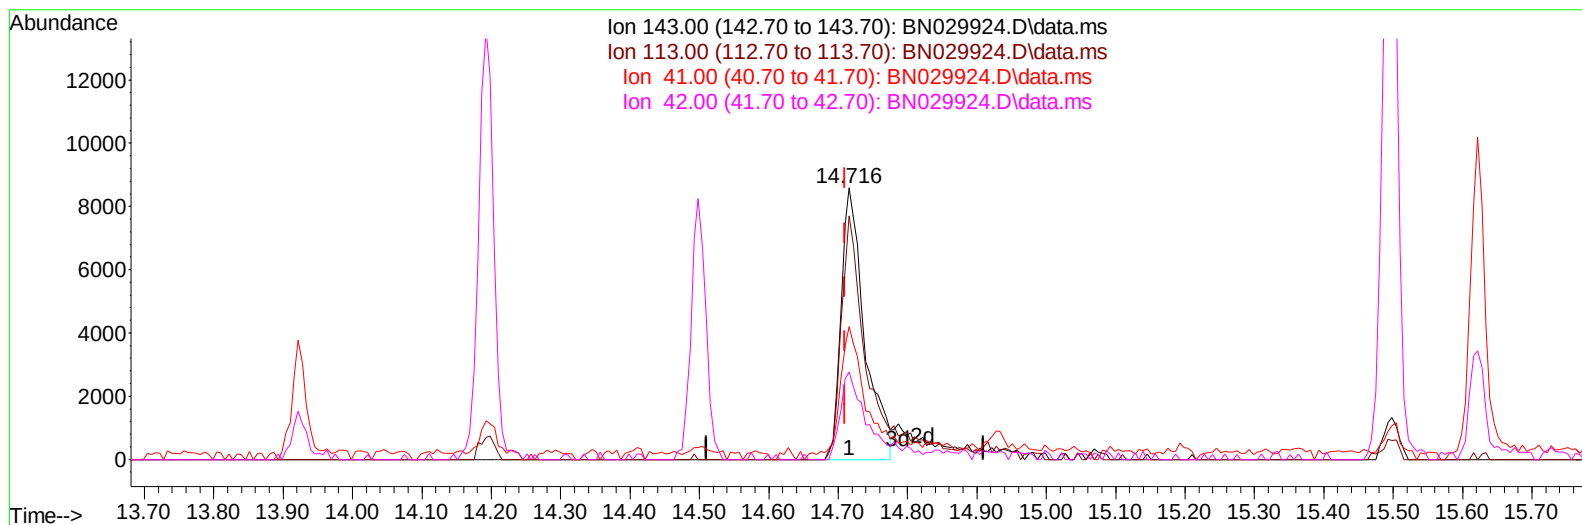

TIC: BN029924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.006) 4.63 ng/u1

response 20164

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	89.67
41.00	45.90	49.05
42.00	28.40	32.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 13:03:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/23/2024
Supervised By :mohammad ahmed 02/24/2024

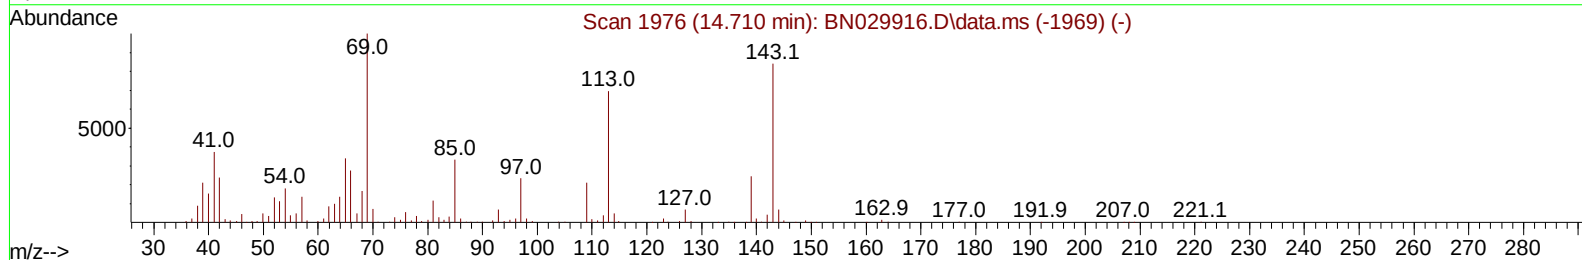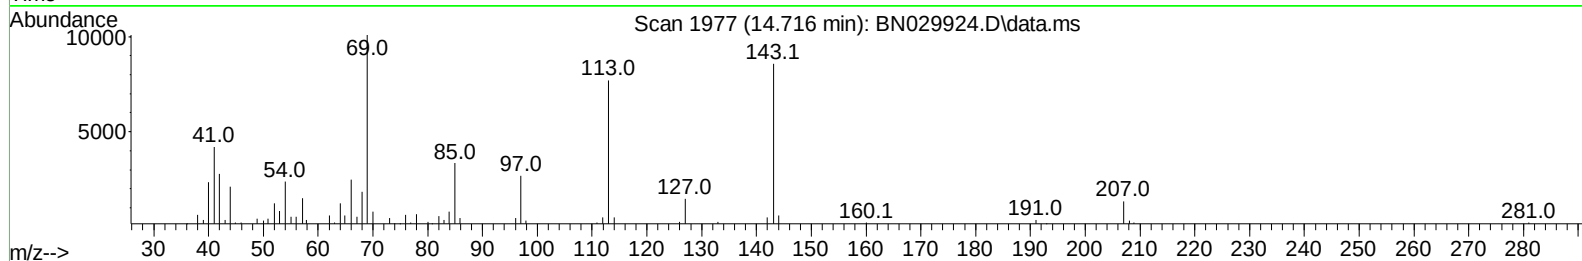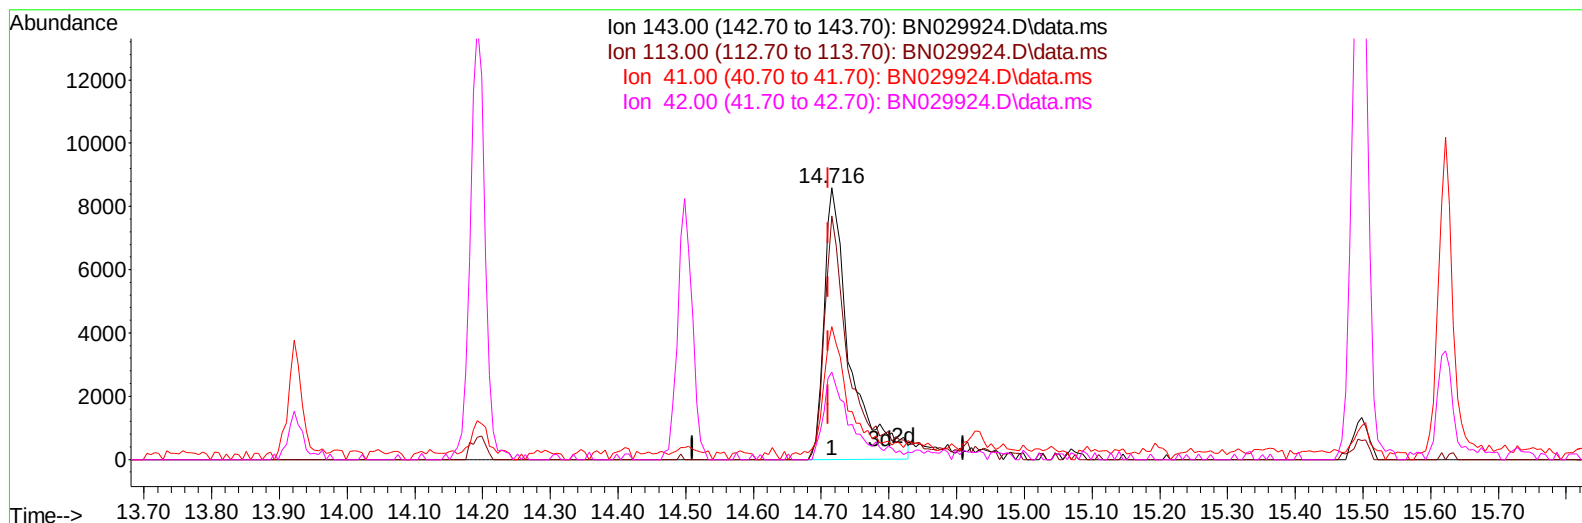

TIC: BN029924.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.006) 5.18 ng/ul m

response 22567

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	89.67
41.00	45.90	49.05
42.00	28.40	32.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029924.D
 Acq On : 22 Feb 2024 12:38
 Operator : MA/JU
 Sample : P1493-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/23/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 23:11:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	146475	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	595189	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	308221	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	625064	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240	528061	20.000	ng/ul	0.00
88) Perylene-d12	23.815	264	580646	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	21620	4.855	ng/uL	0.00
4) Pyridine-d5	3.734	84	145194	12.226	ng/ul	0.00
7) Phenol-d5	7.022	99	121803	8.890	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	405565	44.355	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	358799	36.140	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	223970	21.920	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	226830	49.103	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	208484	51.821	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	348337	43.865	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	518581	38.278	ng/ul	0.00
46) Dimethylphthalate-d6	13.928	166	1126667	49.098	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160	1360568	49.926	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	22567m	5.181	ng/ul	0.00
60) Fluorene-d10	15.498	176	979451	50.173	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	121691	39.955	ng/ul	0.00
73) Anthracene-d10	17.351	188	1537036	52.469	ng/ul	0.00
81) Pyrene-d10	19.651	212	1762357	55.614	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	1595142	54.901	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/23/2024
Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 23:11:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

