




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029929.D
Acq On : 22 Feb 2024 15:39
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 16:38:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/23/2024
Supervised By :mohammad ahmed 02/24/2024

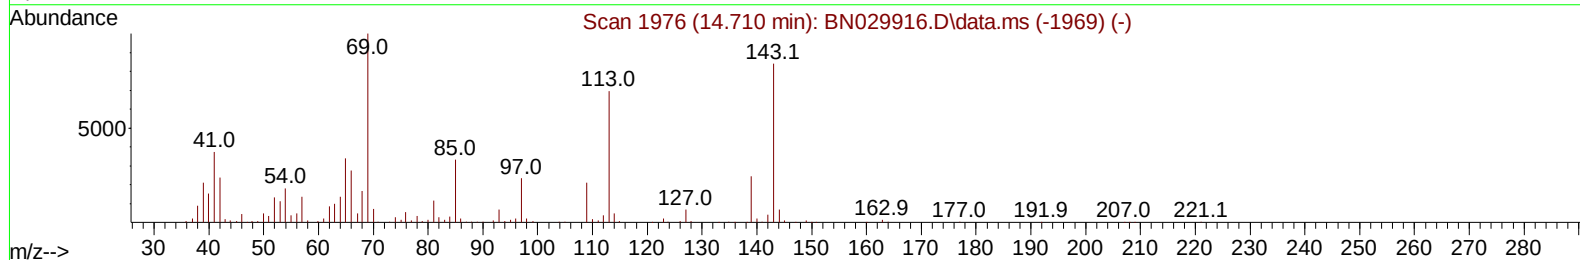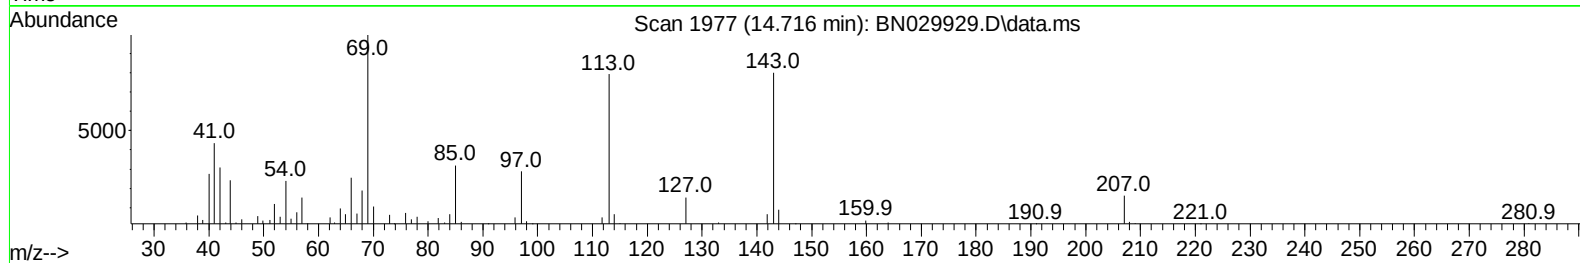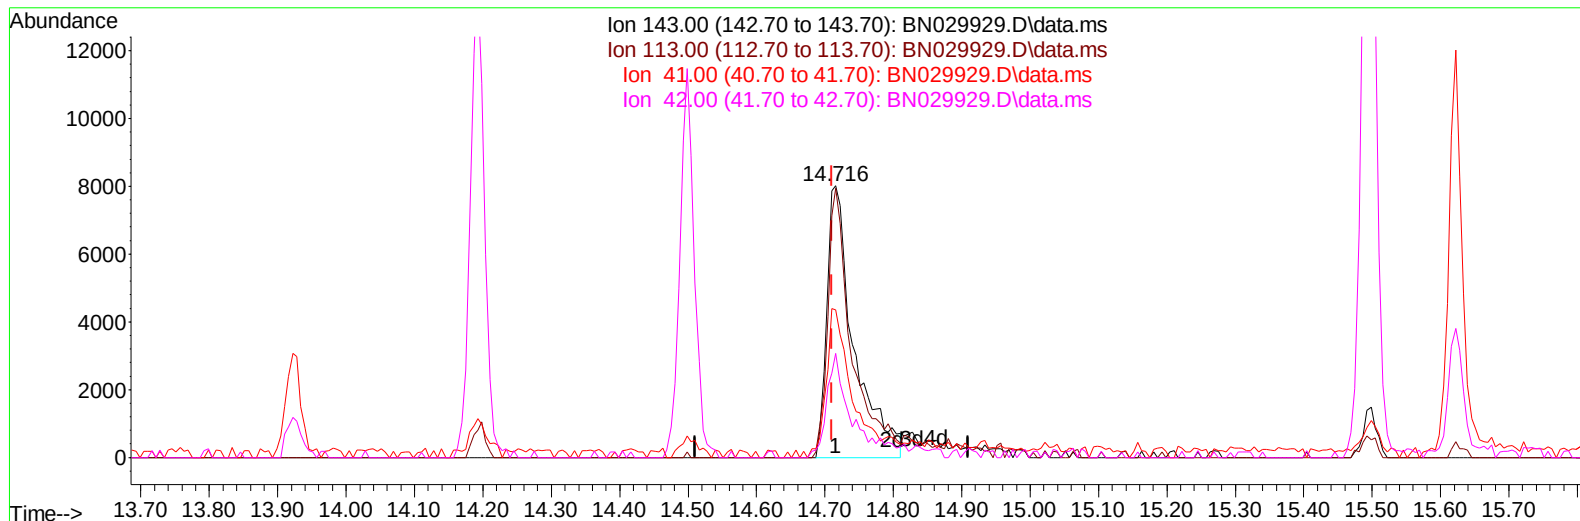

TIC: BN029929.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.716min (+ 0.006) 3.74 ng/ul m

response 21914

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	99.04
41.00	45.90	54.36
42.00	28.40	38.40#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029929.D
 Acq On : 22 Feb 2024 15:39
 Operator : MA/JU
 Sample : P1494-03
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/23/2024
 Supervised By :mohammad ahmed 02/24/2024

Quant Time: Feb 22 23:18:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 21 22:34:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	191631	20.000	ng/ul	0.00
20) Naphthalene-d8	10.652	136	800726	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	414171	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.251	188	860409	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240	722423	20.000	ng/ul	0.00
88) Perylene-d12	23.816	264	829813	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	20651	3.545	ng/uL	0.00
4) Pyridine-d5	3.734	84	95704	6.160	ng/ul	0.00
7) Phenol-d5	7.022	99	120912	6.746	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	396998	33.187	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	361650	27.843	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	214909	16.077	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	226065	36.376	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	209233	38.657	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	343642	32.166	ng/ul	0.00
31) 4-Chloroaniline-d4	10.804	131	478129	26.233	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1124836	36.479	ng/ul	0.00
49) Acenaphthylene-d8	14.193	160	1329545	36.307	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	21914m	3.744	ng/ul	0.00
60) Fluorene-d10	15.498	176	982067	37.438	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.622	200	127201	30.341	ng/ul	0.00
73) Anthracene-d10	17.351	188	1609128	39.905	ng/ul	0.00
81) Pyrene-d10	19.651	212	1818298	41.942	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1701614	40.980	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029929.D
Acq On : 22 Feb 2024 15:39
Operator : MA/JU
Sample : P1494-03
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y4

Manual IntegrationsAPPROVED

Quant Time: Feb 22 23:18:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 21 22:34:54 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/23/2024
Supervised By :mohammad ahmed 02/24/2024

