

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029883.D
 Acq On : 21 Feb 2024 10:53
 Operator : MA/JU
 Sample : PB159060BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	50	rVB	121375	163923	2.31%	0.203%
2	3.593	82	86	90	rBV5	7024	13287	0.19%	0.016%
3	3.717	104	107	127	rBV	1260929	2073321	29.19%	2.573%
4	4.040	157	162	171	rVB3	52040	88485	1.25%	0.110%
5	4.211	188	191	196	rBV2	10487	13218	0.19%	0.016%
6	4.270	196	201	212	rBV2	58132	83891	1.18%	0.104%
7	4.417	223	226	231	rVB2	18280	22702	0.32%	0.028%
8	4.558	246	250	253	rVB4	6595	8477	0.12%	0.011%
9	4.599	253	257	262	rBV	75319	108087	1.52%	0.134%
10	4.658	263	267	268	rBV	21256	27194	0.38%	0.034%
11	5.752	448	453	459	rBV6	12232	20543	0.29%	0.025%
12	6.181	520	526	530	rBV7	8377	18743	0.26%	0.023%
13	7.022	661	669	686	rBV	1723725	2767581	38.96%	3.434%
14	7.199	692	699	709	rBV	1385629	2157801	30.38%	2.678%
15	7.381	723	730	746	rVV	1731769	2743194	38.62%	3.404%
16	7.558	756	760	764	rBV7	9714	16757	0.24%	0.021%
17	7.852	804	810	819	rVB	1049696	1652850	23.27%	2.051%
18	8.016	835	838	843	rBV7	5797	8801	0.12%	0.011%
19	8.093	843	851	856	rBV5	8112	16727	0.24%	0.021%
20	8.569	924	932	946	rBV	1977459	3232138	45.50%	4.011%
21	8.675	948	950	957	rVB8	4345	7468	0.11%	0.009%
22	9.022	1001	1009	1026	rBV	1622198	2651479	37.33%	3.290%
23	9.410	1072	1075	1083	rVB9	3722	7807	0.11%	0.010%
24	9.740	1123	1131	1157	rBV	1293401	2154306	30.33%	2.673%
25	10.028	1173	1180	1182	rBV8	4836	10639	0.15%	0.013%
26	10.275	1213	1222	1232	rBV	1905693	3164456	44.55%	3.927%
27	10.522	1258	1264	1270	rVB4	7409	14134	0.20%	0.018%
28	10.652	1278	1286	1294	rBV	1363238	2321604	32.68%	2.881%
29	10.799	1303	1311	1331	rBV	1715342	3209441	45.18%	3.983%
30	11.305	1392	1397	1399	rBV6	6631	8618	0.12%	0.011%
31	11.328	1399	1401	1410	rVB5	7366	13989	0.20%	0.017%
32	11.416	1410	1416	1421	rBV5	7557	12853	0.18%	0.016%
33	11.863	1488	1492	1497	rBV8	3920	7240	0.10%	0.009%
34	12.110	1527	1534	1536	rBV7	3398	7406	0.10%	0.009%
35	12.246	1549	1557	1564	rBV2	31679	54883	0.77%	0.068%
36	13.404	1745	1754	1761	rBV2	27411	44778	0.63%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029883.D
Acq On : 21 Feb 2024 10:53
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	13.469	1761	1765	1770	rBV6	4294	7153	0.10%	0.009%
38	13.928	1836	1843	1855	rBV	2975204	4109273	57.85%	5.099%
39	14.193	1881	1888	1903	rBV2	3373052	5084636	71.58%	6.310%
40	14.504	1934	1941	1953	rBV	1808015	2673148	37.63%	3.317%
41	14.710	1969	1976	1996	rBV	1135584	2003000	28.20%	2.486%
42	15.498	2102	2110	2124	rBV	4222555	5945167	83.69%	7.378%
43	15.628	2125	2132	2145	rVV	1203849	1767011	24.87%	2.193%
44	15.740	2147	2151	2155	rVB3	20700	29412	0.41%	0.036%
45	16.287	2239	2244	2248	rVB5	13701	21453	0.30%	0.027%
46	17.257	2402	2409	2419	rBV	2117750	3048936	42.92%	3.784%
47	17.357	2419	2426	2439	rVV	4319099	6213630	87.47%	7.711%
48	18.163	2557	2563	2567	rBV8	7884	12289	0.17%	0.015%
49	18.498	2615	2620	2627	rVB10	5872	11653	0.16%	0.014%
50	18.651	2639	2646	2652	rBV10	5743	12369	0.17%	0.015%
51	19.222	2738	2743	2747	rBV	46957	64525	0.91%	0.080%
52	19.292	2750	2755	2763	rBV	42970	66537	0.94%	0.083%
53	19.457	2778	2783	2784	rBV5	7133	7890	0.11%	0.010%
54	19.610	2806	2809	2811	rBV3	12314	14680	0.21%	0.018%
55	19.657	2811	2817	2826	rVV	5194050	6982868	98.30%	8.665%
56	21.457	3118	3123	3136	rBV	2281699	3047291	42.90%	3.782%
57	23.674	3491	3500	3512	rBV2	3500658	7103634	100.00%	8.815%
58	23.769	3514	3516	3519	rVV	107758	174828	2.46%	0.217%
59	23.821	3519	3525	3538	rVB	1588022	3253764	45.80%	4.038%




Sum of corrected areas: 80583968

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029883.D
Acq On : 21 Feb 2024 10:53
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

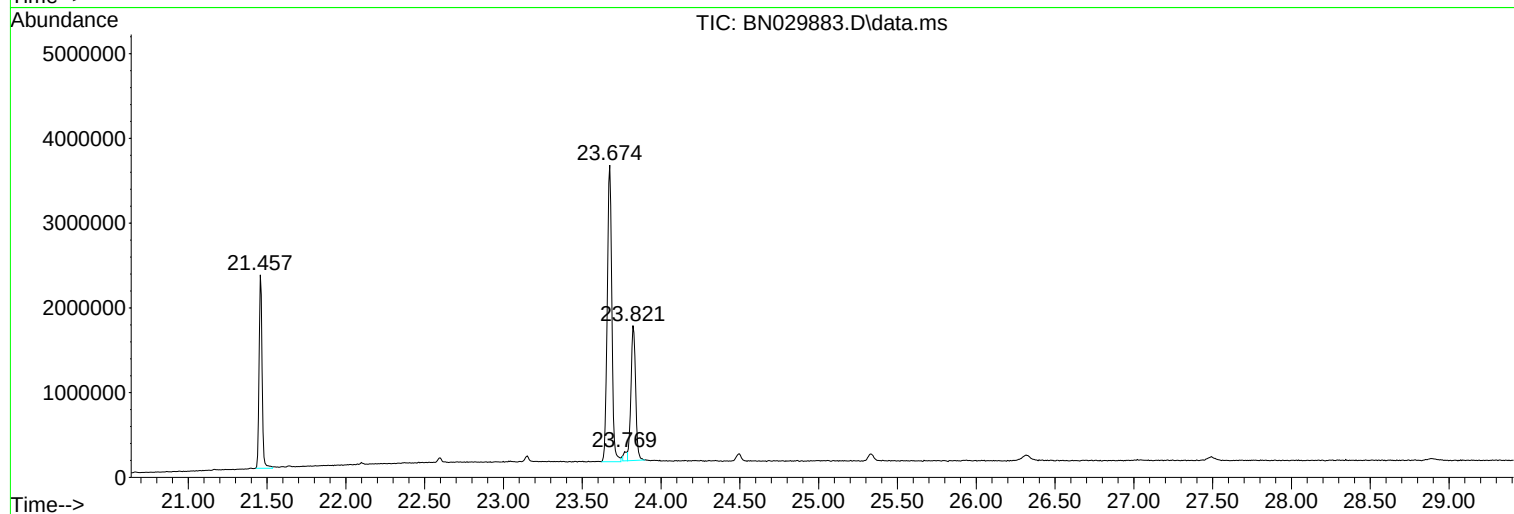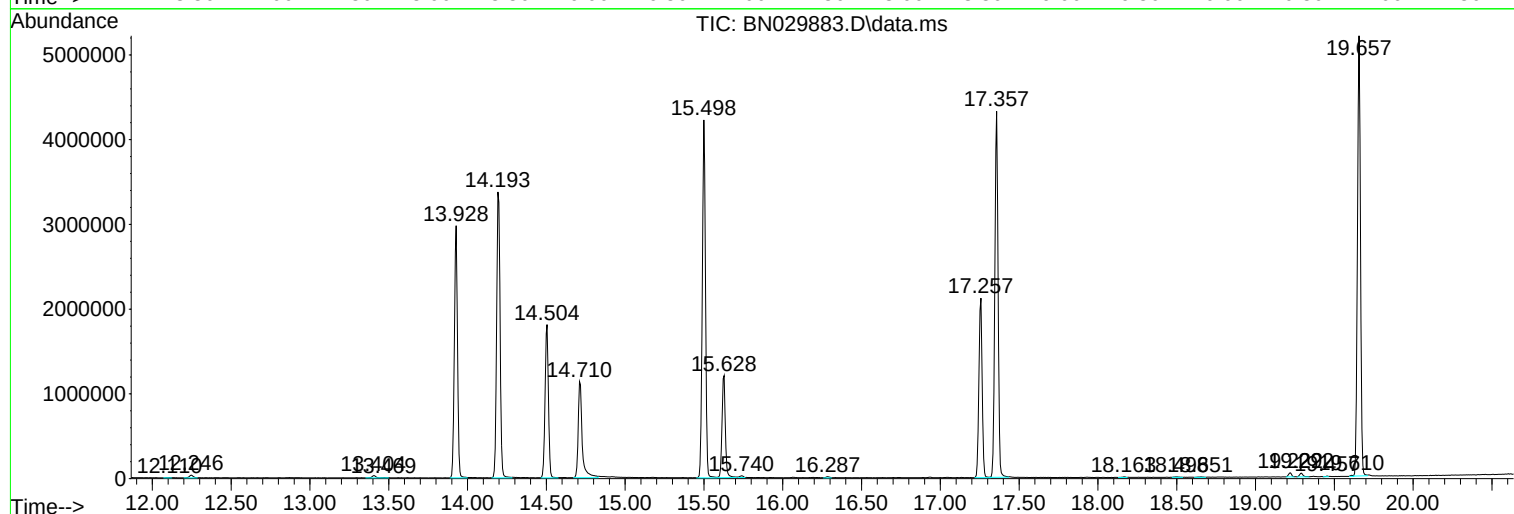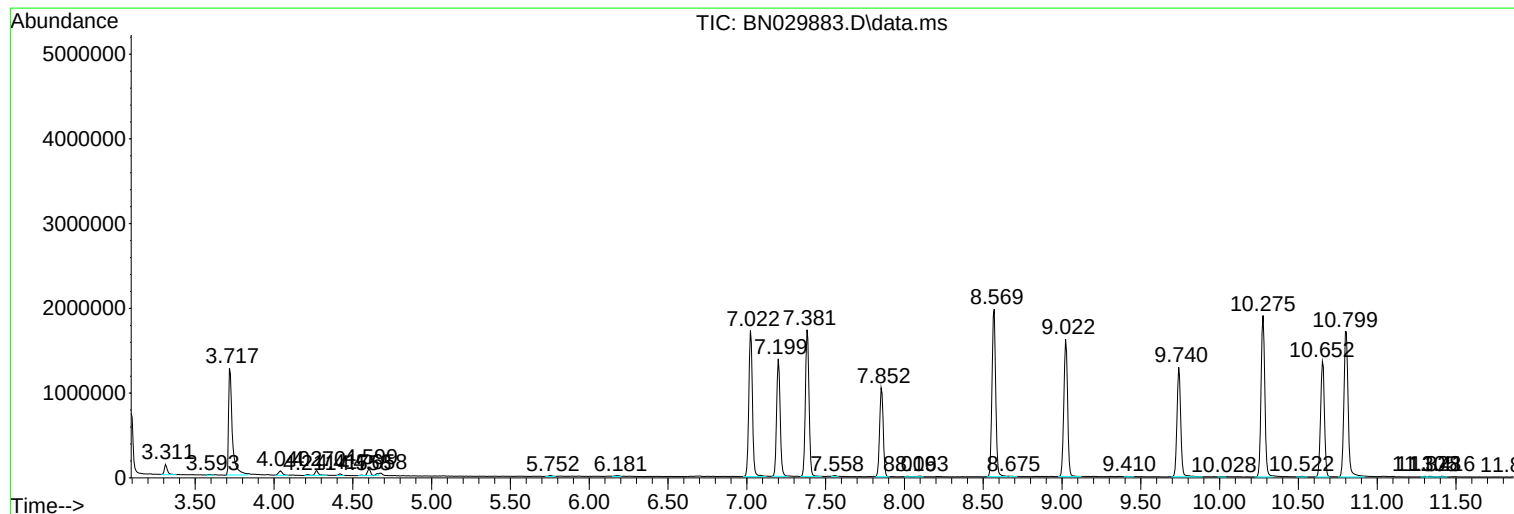

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029883.D
Acq On : 21 Feb 2024 10:53
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029883.D
Acq On : 21 Feb 2024 10:53
Operator : MA/JU
Sample : PB159060BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------