

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029900.D
 Acq On : 21 Feb 2024 21:38
 Operator : MA/JU
 Sample : PB159092BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	35	39	47	rVB	62073	79637	2.11%	0.177%
2	3.728	105	109	133	rBV	648404	1118020	29.63%	2.483%
3	4.046	159	163	169	rVB3	33966	53431	1.42%	0.119%
4	4.222	191	193	195	rVB2	6735	4816	0.13%	0.011%
5	4.275	198	202	207	rVB3	15465	22269	0.59%	0.049%
6	4.422	224	227	232	rVB3	12742	17217	0.46%	0.038%
7	4.604	253	258	265	rBV	41543	62232	1.65%	0.138%
8	4.663	265	268	279	rVB3	14500	30857	0.82%	0.069%
9	5.751	451	453	459	rVB6	5846	9946	0.26%	0.022%
10	7.028	658	670	679	rBV	896541	1429602	37.88%	3.175%
11	7.204	693	700	714	rBV	708717	1115032	29.55%	2.477%
12	7.387	723	731	740	rBV	923399	1444445	38.28%	3.208%
13	7.569	758	762	767	rVB7	5611	9642	0.26%	0.021%
14	7.857	804	811	821	rBV	767764	1201298	31.83%	2.668%
15	8.016	834	838	842	rBV6	4609	7791	0.21%	0.017%
16	8.104	847	853	857	rVB7	5350	10248	0.27%	0.023%
17	8.569	925	932	948	rBV	1031920	1664611	44.11%	3.697%
18	8.839	972	978	983	rBV9	2757	6014	0.16%	0.013%
19	8.892	983	987	990	rVV6	2966	4702	0.12%	0.010%
20	9.028	1001	1010	1021	rBV	805695	1357310	35.97%	3.015%
21	9.745	1124	1132	1148	rBV	633964	1079153	28.60%	2.397%
22	10.016	1175	1178	1182	rBV6	2804	4704	0.12%	0.010%
23	10.275	1213	1222	1240	rBV	957604	1647176	43.65%	3.659%
24	10.528	1259	1265	1270	rVB5	5119	9471	0.25%	0.021%
25	10.657	1279	1287	1297	rVB	974299	1660024	43.99%	3.687%
26	10.804	1304	1312	1331	rBV	926650	1698962	45.02%	3.774%
27	11.310	1392	1398	1399	rBV5	3053	5264	0.14%	0.012%
28	11.739	1468	1471	1475	rBV6	2504	4252	0.11%	0.009%
29	12.251	1550	1558	1565	rBV	15373	25535	0.68%	0.057%
30	13.404	1748	1754	1760	rBV4	13203	23664	0.63%	0.053%
31	13.474	1762	1766	1768	rBV5	3418	5010	0.13%	0.011%
32	13.927	1836	1843	1858	rBV	1496303	2166668	57.42%	4.813%
33	14.027	1858	1860	1868	rVB8	3630	6628	0.18%	0.015%
34	14.192	1881	1888	1902	rBV	1732238	2648509	70.19%	5.883%
35	14.504	1934	1941	1951	rBV	1292665	1944599	51.53%	4.319%
36	14.710	1968	1976	1998	rBV	440086	970039	25.71%	2.155%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029900.D
 Acq On : 21 Feb 2024 21:38
 Operator : MA/JU
 Sample : PB159092BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK092

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.186	2051	2057	2058	rBV6	2959	3829	0.10%	0.009%
38	15.498	2102	2110	2124	rBV	2228149	3161863	83.79%	7.023%
39	15.621	2124	2131	2142	rVV	564797	808137	21.42%	1.795%
40	15.739	2147	2151	2155	rVB4	10992	15307	0.41%	0.034%
41	16.063	2203	2206	2211	rBV5	3895	6086	0.16%	0.014%
42	16.286	2239	2244	2247	rBV6	5872	9901	0.26%	0.022%
43	17.251	2402	2408	2418	rBV	1500540	2211012	58.59%	4.911%
44	17.351	2419	2425	2442	rVB2	2275521	3361477	89.08%	7.467%
45	19.215	2738	2742	2748	rBV2	26449	35370	0.94%	0.079%
46	19.286	2749	2754	2758	rBV2	22751	34172	0.91%	0.076%
47	19.609	2806	2809	2810	rBV3	5543	5918	0.16%	0.013%
48	19.651	2810	2816	2827	rVV	2708704	3773542	100.00%	8.382%
49	21.456	3117	3123	3135	rBV	1608243	2196694	58.21%	4.879%
50	23.662	3491	3498	3510	rBV2	1763625	3579013	94.84%	7.950%
51	23.815	3518	3524	3538	rVB	1090417	2269557	60.14%	5.041%




Sum of corrected areas: 45020656

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029900.D
Acq On : 21 Feb 2024 21:38
Operator : MA/JU
Sample : PB159092BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

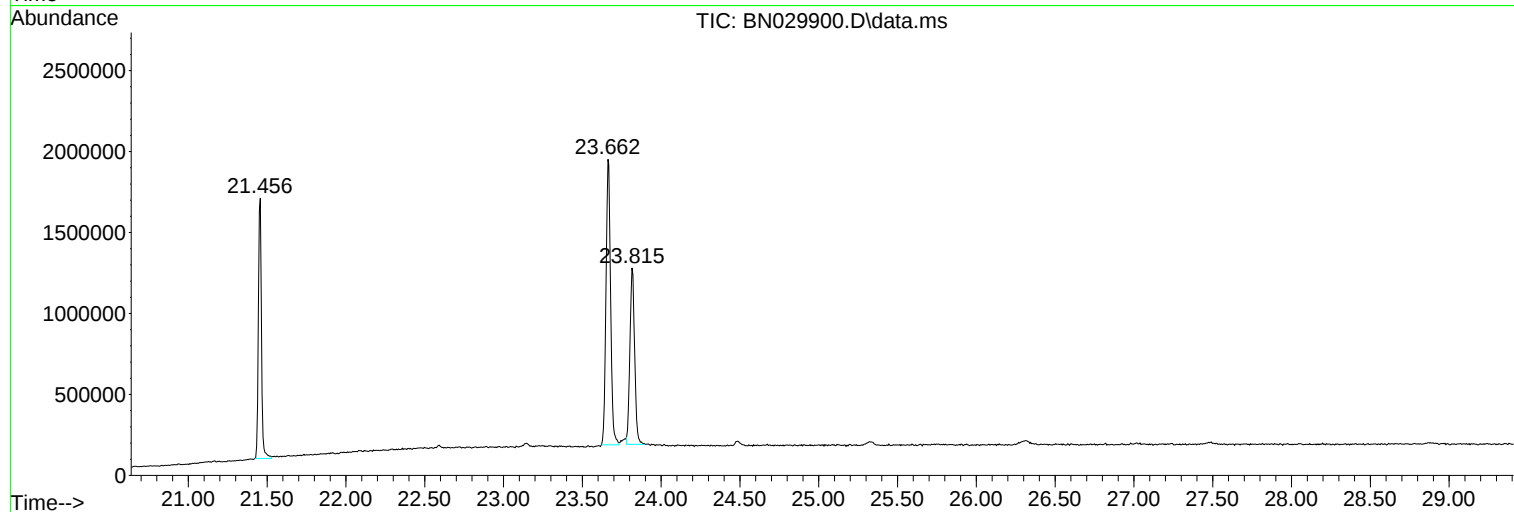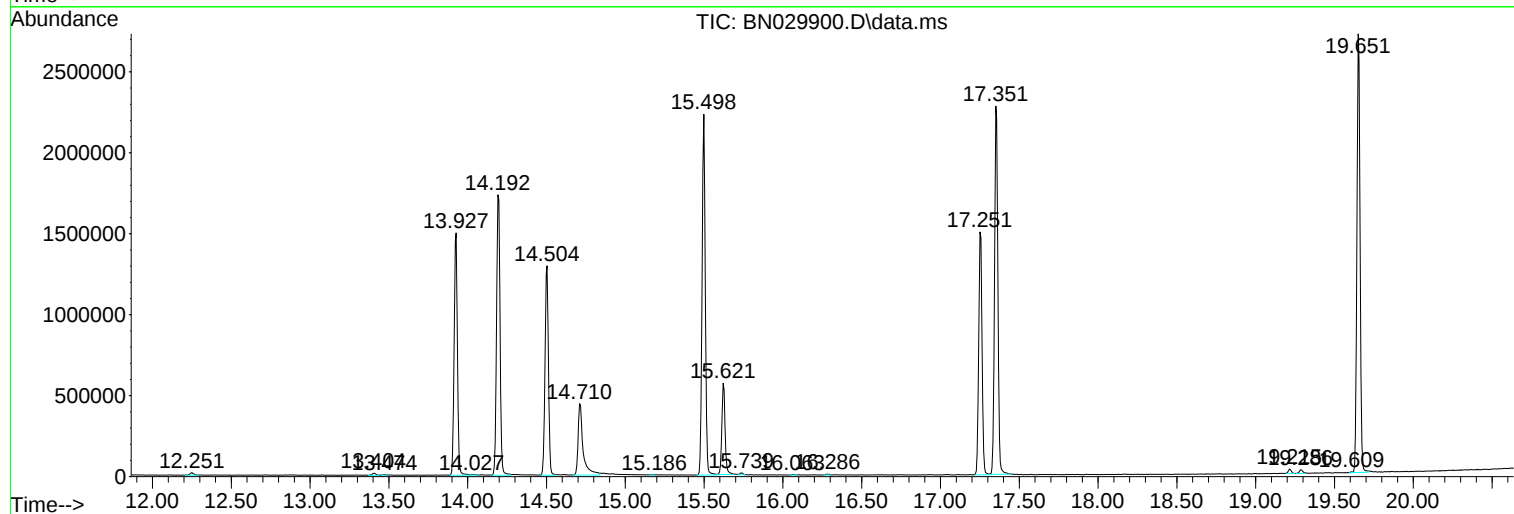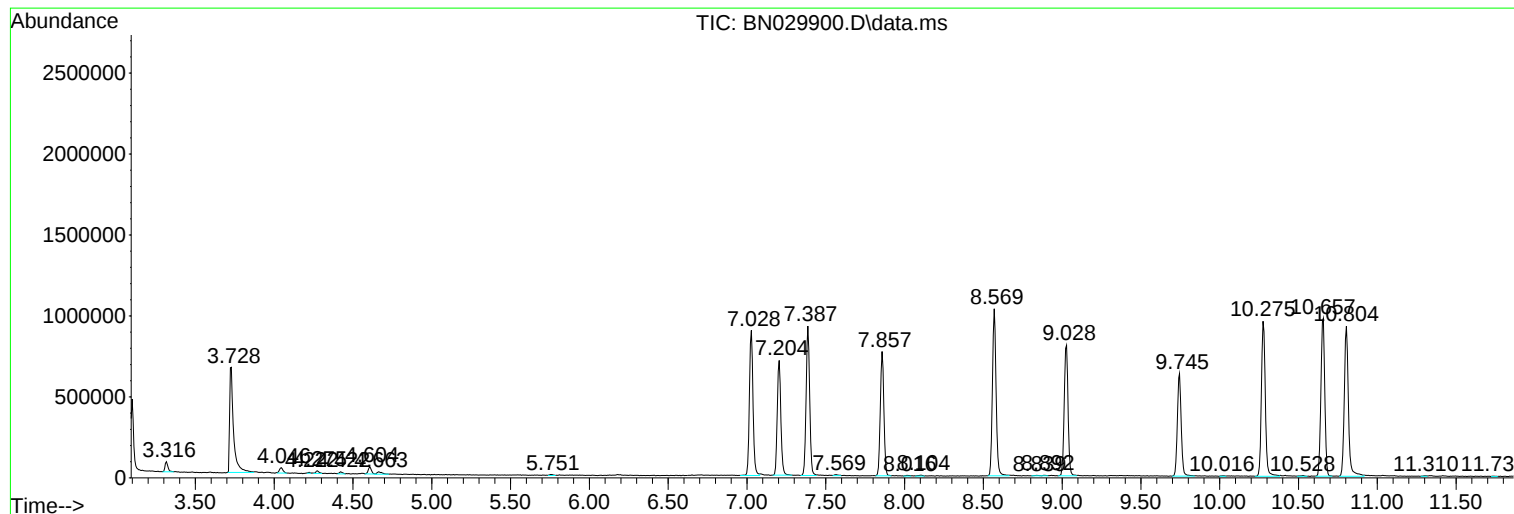

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029900.D
Acq On : 21 Feb 2024 21:38
Operator : MA/JU
Sample : PB159092BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029900.D
Acq On : 21 Feb 2024 21:38
Operator : MA/JU
Sample : PB159092BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------