

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029901.D
 Acq On : 21 Feb 2024 22:14
 Operator : MA/JU
 Sample : PB159094BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	35	39	50	rVB	62517	89068	2.41%	0.216%
2	3.728	105	109	128	rBV	627554	1085791	29.42%	2.634%
3	4.046	159	163	171	rVB4	29234	51739	1.40%	0.125%
4	4.275	198	202	206	rBV3	15081	21314	0.58%	0.052%
5	4.422	224	227	233	rVB8	9456	14602	0.40%	0.035%
6	4.605	254	258	264	rVV	41989	57404	1.56%	0.139%
7	4.663	264	268	277	rVB2	14740	31646	0.86%	0.077%
8	5.758	450	454	457	rBV5	4789	6385	0.17%	0.015%
9	6.657	601	607	610	rBV7	4699	10446	0.28%	0.025%
10	7.028	663	670	679	rBV	853449	1361772	36.90%	3.303%
11	7.205	693	700	713	rVB	680114	1059953	28.72%	2.571%
12	7.387	724	731	745	rBV	863167	1364675	36.98%	3.310%
13	7.563	758	761	769	rVB7	5898	10583	0.29%	0.026%
14	7.857	804	811	819	rVB	607503	943335	25.56%	2.288%
15	8.028	835	840	841	rBV4	2842	4422	0.12%	0.011%
16	8.099	849	852	857	rBV5	4717	4592	0.12%	0.011%
17	8.569	925	932	944	rBV	974844	1583985	42.92%	3.842%
18	8.840	974	978	980	rBV5	3002	3811	0.10%	0.009%
19	9.028	1001	1010	1023	rBV	770199	1299542	35.21%	3.152%
20	9.328	1059	1061	1064	rBV4	3889	4940	0.13%	0.012%
21	9.746	1121	1132	1149	rBV	602958	1027048	27.83%	2.491%
22	10.034	1176	1181	1187	rBV7	2139	5166	0.14%	0.013%
23	10.275	1214	1222	1232	rBV	896458	1545687	41.88%	3.749%
24	10.528	1259	1265	1269	rVB8	3442	6106	0.17%	0.015%
25	10.651	1279	1286	1295	rBV	764605	1307006	35.41%	3.170%
26	10.804	1303	1312	1334	rBV	868409	1619764	43.89%	3.929%
27	11.340	1402	1403	1409	rVV5	3470	4297	0.12%	0.010%
28	11.416	1412	1416	1423	rVB7	4333	7978	0.22%	0.019%
29	12.245	1551	1557	1565	rBV3	14295	24219	0.66%	0.059%
30	13.410	1748	1755	1758	rBV4	12281	19975	0.54%	0.048%
31	13.481	1762	1767	1769	rBV5	2524	3957	0.11%	0.010%
32	13.922	1835	1842	1857	rBV	1402425	2049320	55.53%	4.971%
33	14.192	1881	1888	1904	rBV	1658464	2483465	67.29%	6.024%
34	14.504	1933	1941	1948	rBV	1015662	1517163	41.11%	3.680%
35	14.604	1957	1958	1965	rVB6	2442	4260	0.12%	0.010%
36	14.710	1968	1976	1993	rBV	433180	909426	24.64%	2.206%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029901.D
Acq On : 21 Feb 2024 22:14
Operator : MA/JU
Sample : PB159094BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	14.922	2010	2012	2019	rVB7	5131	6722	0.18%	0.016%
38	15.498	2103	2110	2124	rBV	2057352	3017292	81.76%	7.318%
39	15.622	2124	2131	2143	rVV	557657	789619	21.40%	1.915%
40	15.733	2147	2150	2156	rVB5	9507	14695	0.40%	0.036%
41	16.069	2203	2207	2210	rBV5	2674	4303	0.12%	0.010%
42	16.286	2241	2244	2248	rVB6	6217	7563	0.20%	0.018%
43	16.939	2352	2355	2357	rBV4	3060	3799	0.10%	0.009%
44	17.251	2402	2408	2418	rBV	1215921	1763767	47.79%	4.278%
45	17.351	2419	2425	2441	rVB2	2221999	3270103	88.61%	7.932%
46	18.763	2661	2665	2670	rBV7	2304	4456	0.12%	0.011%
47	19.222	2738	2743	2747	rBV4	25030	36985	1.00%	0.090%
48	19.286	2751	2754	2759	rVV	19385	27965	0.76%	0.068%
49	19.651	2810	2816	2833	rBV	2636050	3690598	100.00%	8.951%
50	21.457	3117	3123	3134	rBV2	1268953	1794670	48.63%	4.353%
51	23.662	3491	3498	3510	rBV2	1711517	3493602	94.66%	8.474%
52	23.815	3517	3524	3534	rVB2	863292	1758205	47.64%	4.264%




Sum of corrected areas: 41229186

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029901.D
Acq On : 21 Feb 2024 22:14
Operator : MA/JU
Sample : PB159094BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

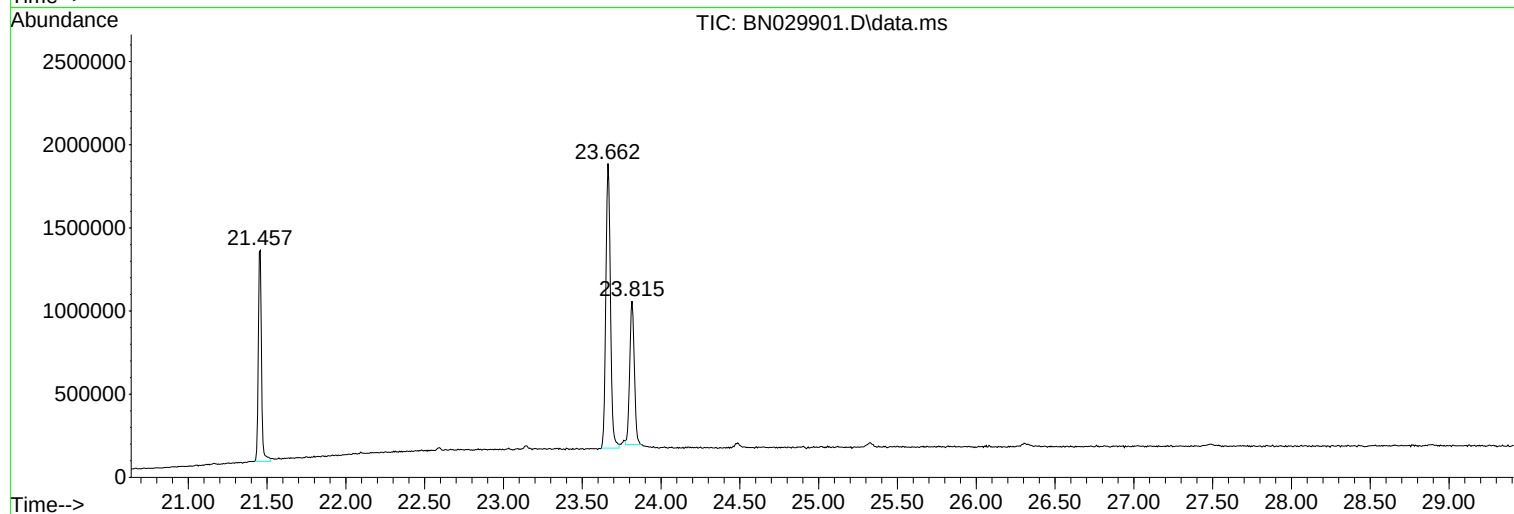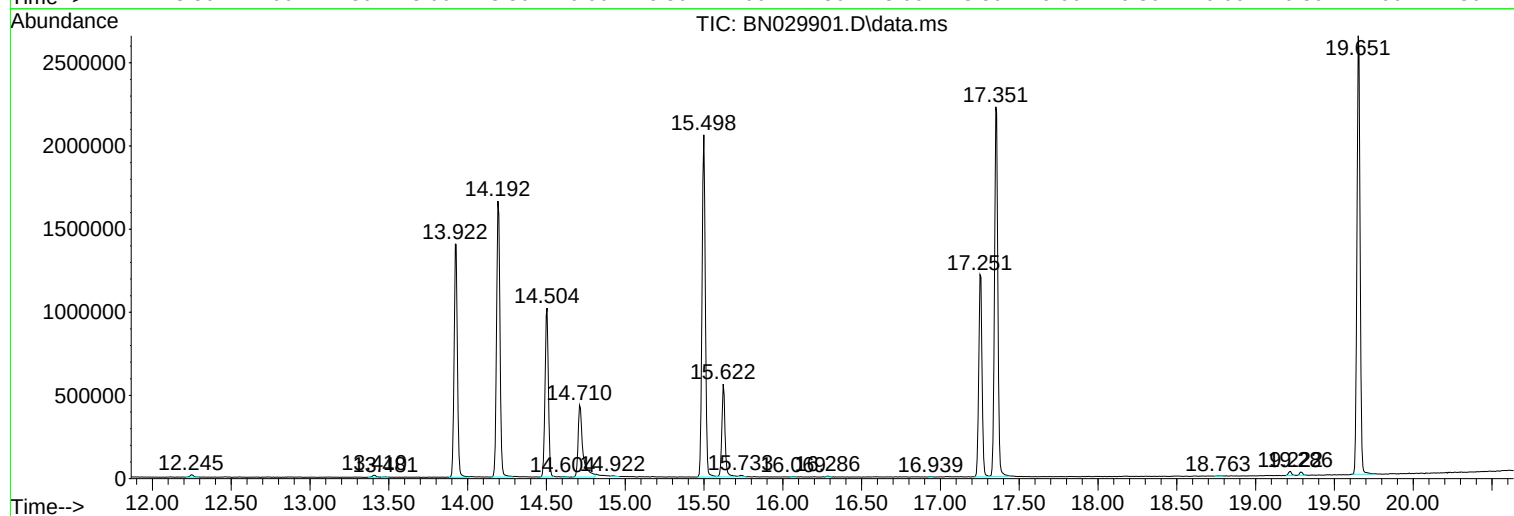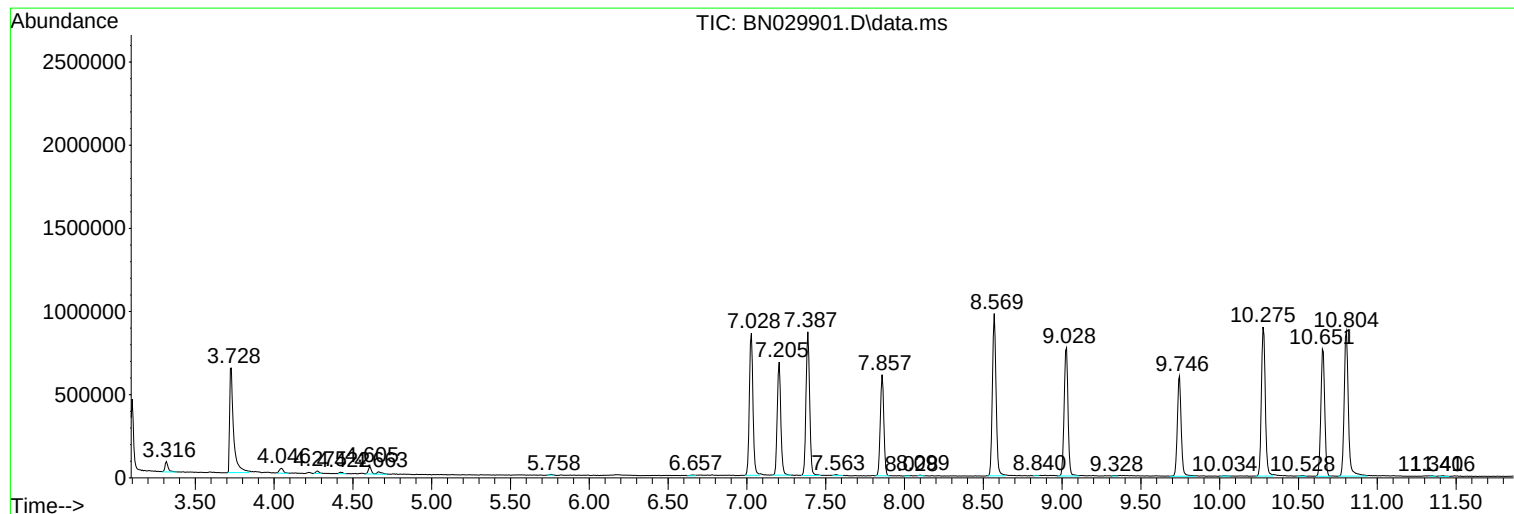

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029901.D
Acq On : 21 Feb 2024 22:14
Operator : MA/JU
Sample : PB159094BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029901.D
Acq On : 21 Feb 2024 22:14
Operator : MA/JU
Sample : PB159094BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc