

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029902.D
 Acq On : 21 Feb 2024 22:50
 Operator : MA/JU
 Sample : P1493-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	46	rVB	42370	55732	1.37%	0.145%
2	3.734	108	110	133	rVB	109381	230872	5.68%	0.601%
3	4.046	160	163	168	rVB3	11922	16534	0.41%	0.043%
4	5.516	409	413	420	rVB2	11689	18238	0.45%	0.047%
5	7.028	664	670	682	rVB	157272	255877	6.29%	0.666%
6	7.205	693	700	711	rBV	694442	1121159	27.57%	2.919%
7	7.387	724	731	743	rBV	673153	1060115	26.07%	2.760%
8	7.469	743	745	750	rVB6	5936	8811	0.22%	0.023%
9	7.858	804	811	820	rBV	567657	892909	21.96%	2.324%
10	8.569	926	932	947	rBV	440771	728998	17.93%	1.898%
11	9.022	1002	1009	1018	rBV	800198	1358008	33.40%	3.535%
12	9.746	1124	1132	1143	rBV	587648	1013572	24.93%	2.638%
13	10.275	1213	1222	1235	rBV	849049	1448158	35.61%	3.770%
14	10.652	1279	1286	1299	rBV	703445	1223764	30.10%	3.186%
15	10.804	1301	1312	1329	rBV	716318	1318341	32.42%	3.432%
16	11.204	1375	1380	1386	rBV2	15527	29423	0.72%	0.077%
17	11.269	1386	1391	1395	rVV	15137	25916	0.64%	0.067%
18	12.081	1524	1529	1535	rBV7	2778	4824	0.12%	0.013%
19	12.246	1553	1557	1563	rVB3	14770	23556	0.58%	0.061%
20	13.245	1723	1727	1731	rBV6	6934	9364	0.23%	0.024%
21	13.334	1738	1742	1745	rVB5	3540	4821	0.12%	0.013%
22	13.404	1748	1754	1762	rVV2	14382	22653	0.56%	0.059%
23	13.922	1836	1842	1854	rBV	1530166	2226548	54.76%	5.796%
24	14.193	1882	1888	1904	rBV	1744610	2676460	65.82%	6.967%
25	14.504	1934	1941	1950	rBV	932075	1413651	34.77%	3.680%
26	14.722	1971	1978	1993	rBV2	42725	122850	3.02%	0.320%
27	14.928	2010	2013	2016	rBV5	3396	5272	0.13%	0.014%
28	15.498	2103	2110	2125	rBV	2342465	3368916	82.85%	8.770%
29	15.622	2125	2131	2147	rVV	593568	870478	21.41%	2.266%
30	15.739	2147	2151	2155	rVB4	10990	15193	0.37%	0.040%
31	16.281	2238	2243	2249	rVB6	7550	10859	0.27%	0.028%
32	17.039	2369	2372	2378	rBV6	3559	6494	0.16%	0.017%
33	17.251	2401	2408	2418	rBV	1111741	1639566	40.32%	4.268%
34	17.357	2419	2426	2443	rVV	2457146	3683678	90.59%	9.589%
35	17.939	2521	2525	2527	rBV5	3613	4773	0.12%	0.012%
36	18.163	2558	2563	2572	rBV3	38898	61911	1.52%	0.161%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029902.D
Acq On : 21 Feb 2024 22:50
Operator : MA/JU
Sample : P1493-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.186	2732	2737	2738	rBV5	2466	4301	0.11%	0.011%
38	19.216	2738	2742	2749	rVB3	28629	40296	0.99%	0.105%
39	19.286	2749	2754	2758	rBV2	26409	39165	0.96%	0.102%
40	19.363	2765	2767	2771	rVB5	4752	4929	0.12%	0.013%
41	19.451	2779	2782	2789	rBV4	23097	34257	0.84%	0.089%
42	19.604	2805	2808	2810	rBV4	10866	13018	0.32%	0.034%
43	19.651	2810	2816	2825	rVV	2888039	4066249	100.00%	10.585%
44	20.027	2879	2880	2882	rBV2	5224	4303	0.11%	0.011%
45	21.451	3117	3122	3134	rBV	1185661	1629960	40.09%	4.243%
46	23.663	3491	3498	3511	rBV2	1956272	3885940	95.57%	10.116%
47	23.816	3518	3524	3537	rVB2	829429	1714840	42.17%	4.464%




Sum of corrected areas: 38415552

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029902.D
Acq On : 21 Feb 2024 22:50
Operator : MA/JU
Sample : P1493-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

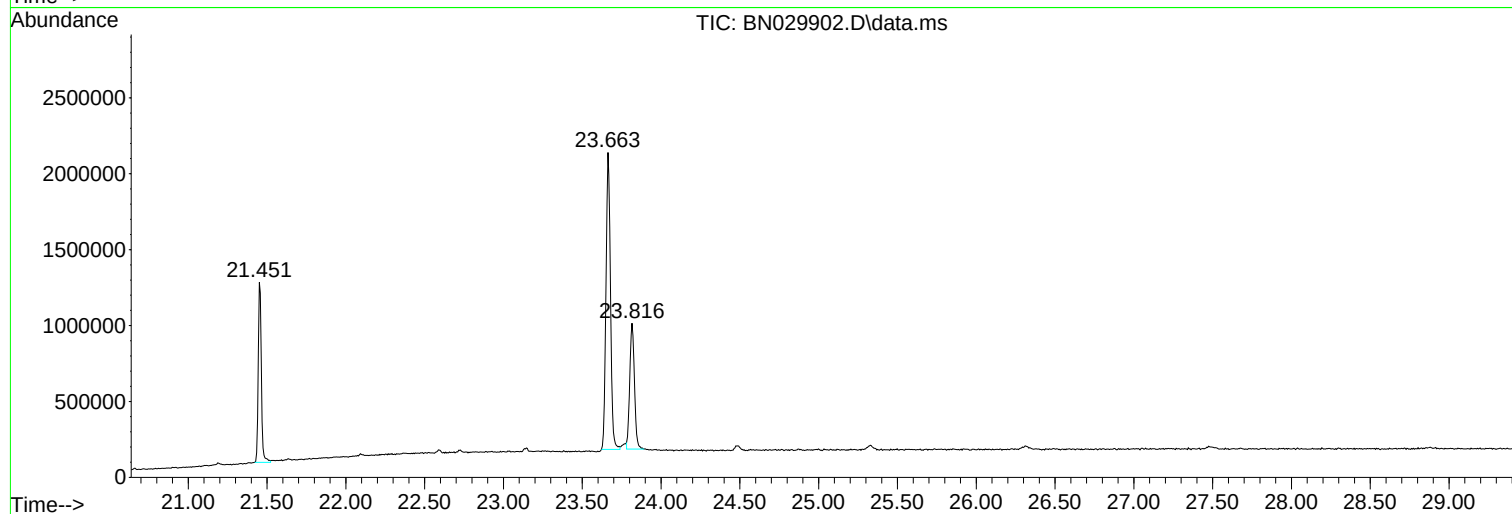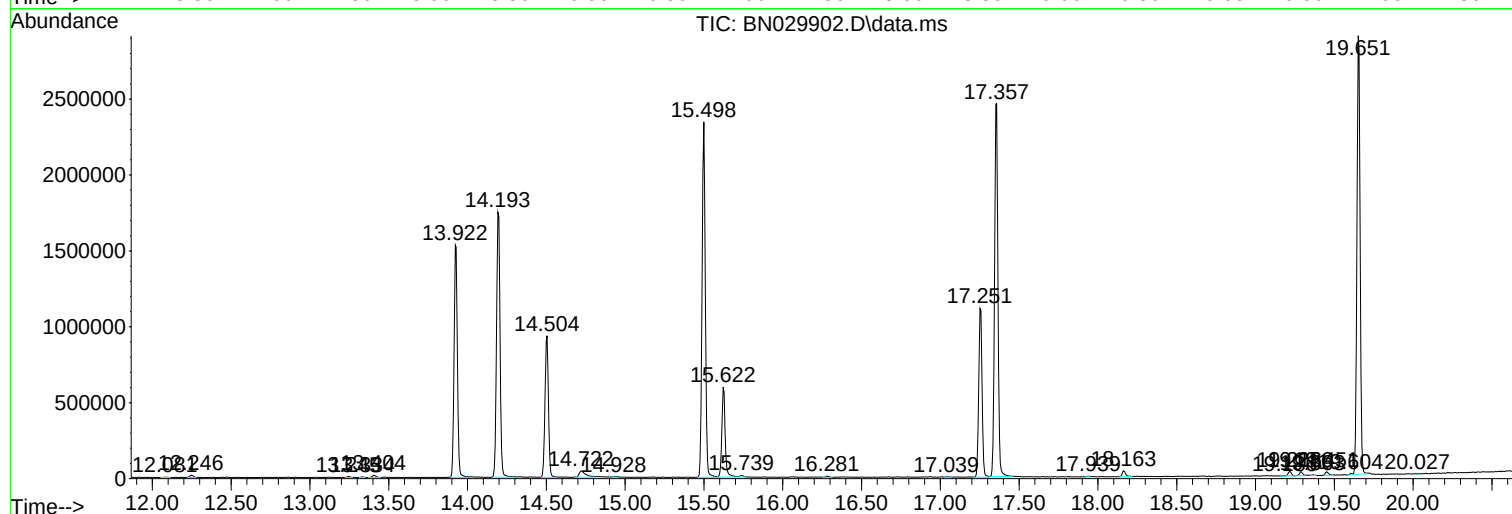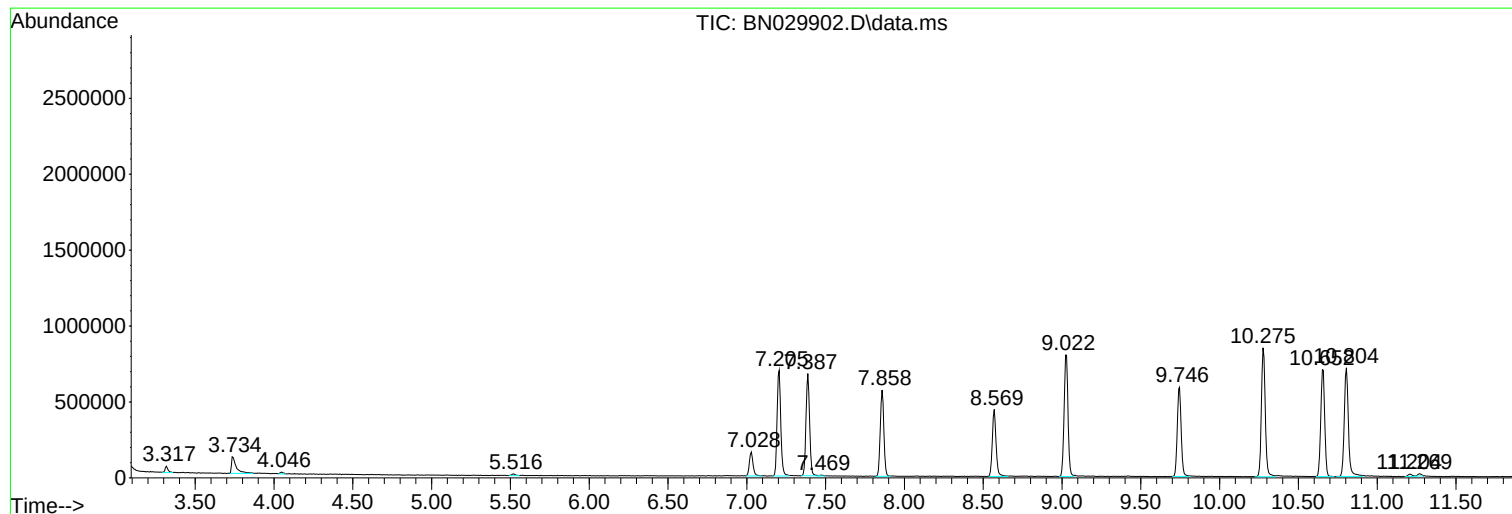

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029902.D
Acq On : 21 Feb 2024 22:50
Operator : MA/JU
Sample : P1493-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029902.D
Acq On : 21 Feb 2024 22:50
Operator : MA/JU
Sample : P1493-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------