

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029905.D
 Acq On : 22 Feb 2024 00:38
 Operator : MA/JU
 Sample : P1493-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	47	rVB	35579	47999	1.17%	0.125%
2	3.746	109	112	126	rBV	58556	126023	3.07%	0.327%
3	4.052	159	164	168	rBV2	11748	17015	0.42%	0.044%
4	5.522	409	414	417	rBV	12225	17876	0.44%	0.046%
5	6.858	638	641	646	rBV7	3089	5839	0.14%	0.015%
6	7.028	664	670	677	rBV	169166	270350	6.60%	0.702%
7	7.205	693	700	715	rBV	715410	1166174	28.45%	3.030%
8	7.387	724	731	743	rBV	708914	1112464	27.14%	2.891%
9	7.469	743	745	749	rVB5	4363	5550	0.14%	0.014%
10	7.857	805	811	821	rBV	558550	873132	21.30%	2.269%
11	8.569	925	932	942	rBV	485288	791535	19.31%	2.057%
12	9.022	1001	1009	1020	rBV	839445	1414742	34.52%	3.676%
13	9.410	1073	1075	1081	rVB5	5286	7632	0.19%	0.020%
14	9.746	1124	1132	1145	rBV	629651	1064337	25.97%	2.766%
15	10.275	1215	1222	1237	rBV	882519	1520625	37.10%	3.951%
16	10.440	1249	1250	1258	rVB7	3059	4163	0.10%	0.011%
17	10.651	1279	1286	1295	rBV	707858	1205650	29.42%	3.133%
18	10.804	1304	1312	1326	rBV	591350	1119863	27.32%	2.910%
19	12.075	1524	1528	1534	rVB7	5517	8102	0.20%	0.021%
20	12.251	1553	1558	1565	rVB2	14979	28002	0.68%	0.073%
21	13.404	1749	1754	1758	rBV4	5984	9906	0.24%	0.026%
22	13.922	1836	1842	1857	rBV	1517475	2205641	53.82%	5.731%
23	14.192	1881	1888	1904	rBV2	1811103	2754601	67.21%	7.157%
24	14.498	1934	1940	1949	rBV	939426	1418242	34.60%	3.685%
25	14.722	1970	1978	1988	rBV2	45102	120182	2.93%	0.312%
26	15.304	2073	2077	2079	rBV5	3395	4116	0.10%	0.011%
27	15.498	2103	2110	2123	rBV	2336640	3363035	82.05%	8.738%
28	15.622	2125	2131	2147	rVV	584797	873412	21.31%	2.269%
29	15.734	2147	2150	2160	rVB7	10713	22776	0.56%	0.059%
30	16.286	2241	2244	2247	rVV4	6576	8475	0.21%	0.022%
31	17.045	2368	2373	2376	rBV6	2863	5428	0.13%	0.014%
32	17.251	2402	2408	2417	rBV	1156213	1676864	40.91%	4.357%
33	17.351	2419	2425	2446	rVB2	2525925	3697714	90.22%	9.608%
34	17.933	2519	2524	2529	rVB8	3917	6394	0.16%	0.017%
35	18.163	2557	2563	2571	rBV3	15047	24427	0.60%	0.063%
36	18.645	2643	2645	2650	rBV6	3009	4359	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.216	2738	2742	2750	rVB2	27222	37197	0.91%	0.097%
38	19.286	2750	2754	2759	rBV	23662	34285	0.84%	0.089%
39	19.451	2776	2782	2786	rBV8	14111	24661	0.60%	0.064%
40	19.604	2805	2808	2811	rBV5	8454	13122	0.32%	0.034%
41	19.651	2811	2816	2825	rVV	2971209	4098543	100.00%	10.650%
42	20.657	2985	2987	2991	rBV5	8261	9100	0.22%	0.024%
43	21.451	3117	3122	3135	rBV2	1177503	1677636	40.93%	4.359%
44	23.668	3491	3499	3510	rBV2	1920604	3874691	94.54%	10.068%
45	23.815	3518	3524	3539	rVB2	814701	1713726	41.81%	4.453%




Sum of corrected areas: 38485606

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

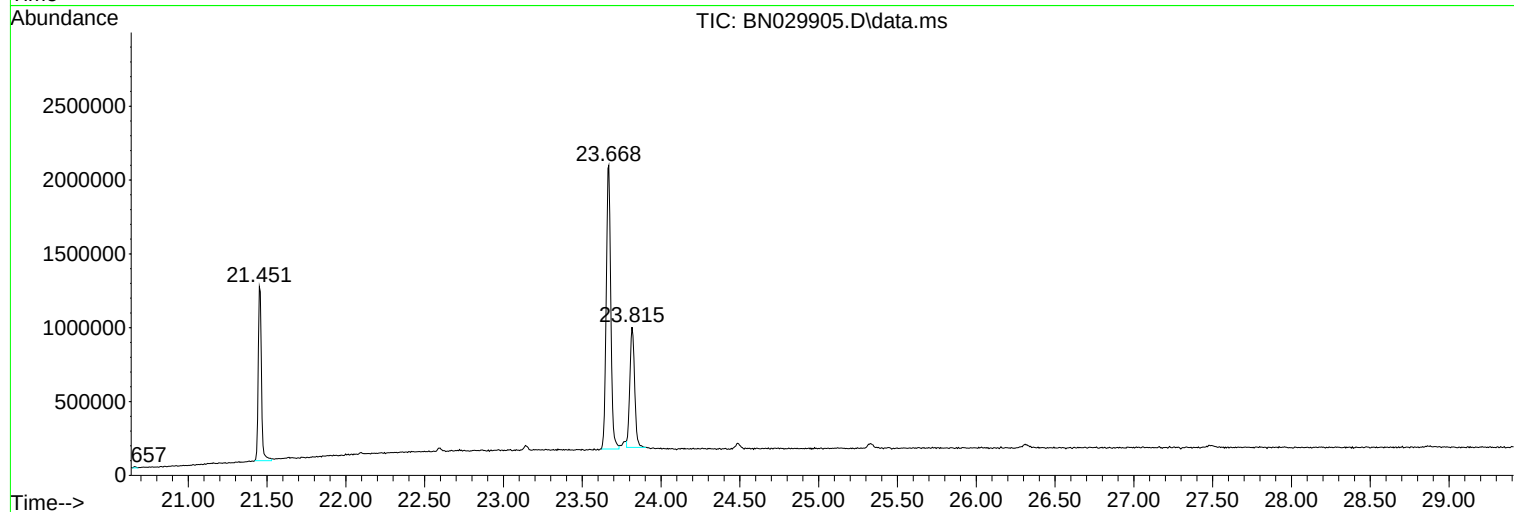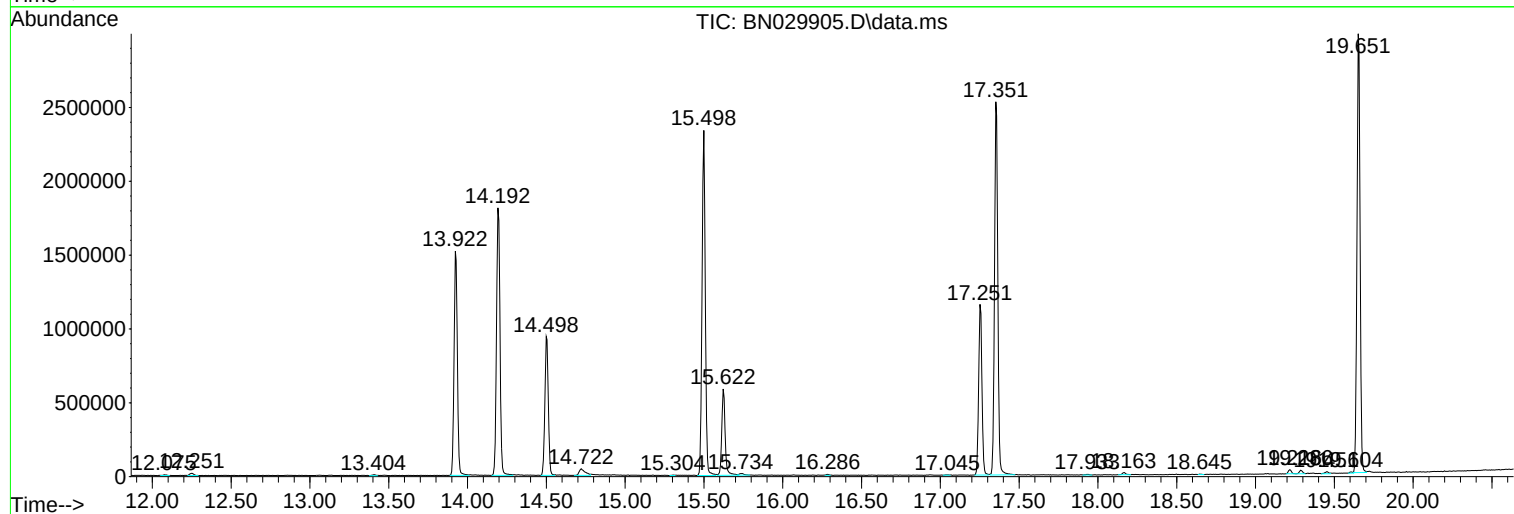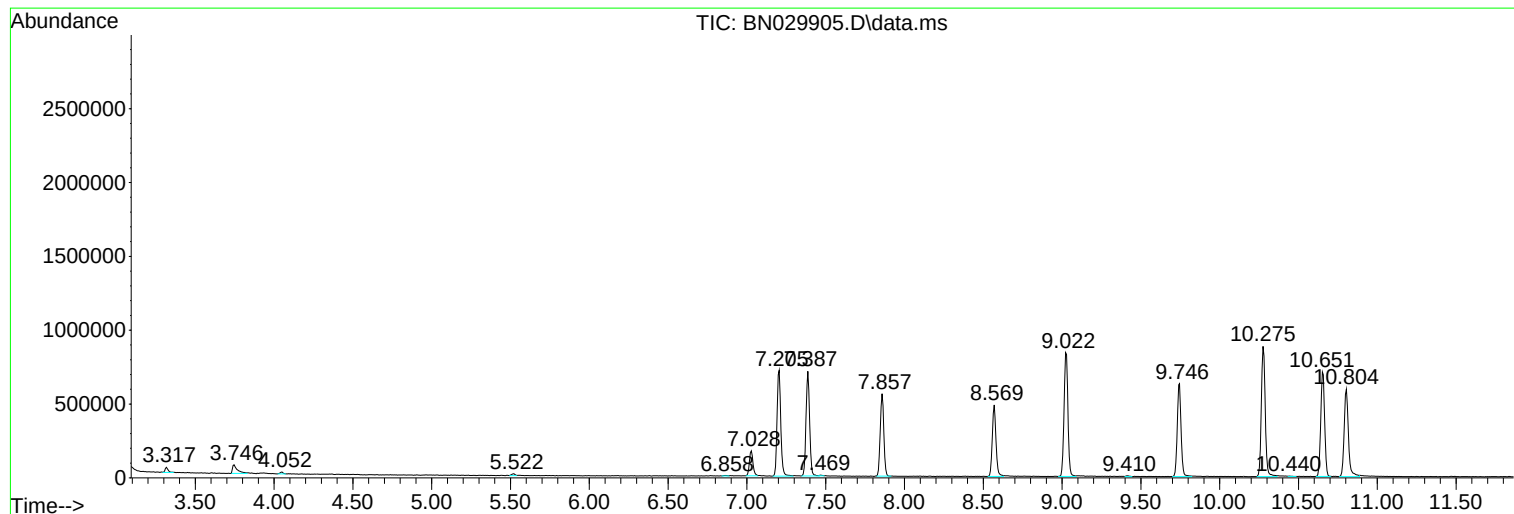

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029905.D
Acq On : 22 Feb 2024 00:38
Operator : MA/JU
Sample : P1493-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------