

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029908.D
 Acq On : 22 Feb 2024 02:26
 Operator : MA/JU
 Sample : P1493-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3X0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	47	rVB	43862	56879	1.09%	0.117%
2	3.728	106	109	126	rBV	258447	471157	9.05%	0.971%
3	4.046	159	163	173	rBV2	13811	22441	0.43%	0.046%
4	5.517	410	413	418	rVB3	17986	24087	0.46%	0.050%
5	7.028	664	670	681	rVB	232542	379051	7.28%	0.781%
6	7.205	693	700	712	rBV	947095	1499662	28.79%	3.091%
7	7.387	724	731	741	rBV	926454	1463510	28.10%	3.016%
8	7.469	743	745	751	rVB5	7211	11411	0.22%	0.024%
9	7.858	804	811	821	rBV	600931	941618	18.08%	1.941%
10	8.569	925	932	944	rBV	651989	1057079	20.30%	2.179%
11	9.022	1001	1009	1018	rBV	1083912	1836580	35.26%	3.785%
12	9.422	1072	1077	1078	rBV4	4395	5850	0.11%	0.012%
13	9.740	1122	1131	1148	rBV	821062	1409923	27.07%	2.906%
14	10.275	1213	1222	1235	rBV	1168829	1987437	38.16%	4.096%
15	10.652	1279	1286	1294	rBV	761250	1290735	24.78%	2.660%
16	10.804	1304	1312	1331	rBV	1055197	1936244	37.17%	3.990%
17	11.469	1421	1425	1429	rBV6	3050	5430	0.10%	0.011%
18	12.251	1552	1558	1564	rBV2	19153	35327	0.68%	0.073%
19	13.404	1750	1754	1760	rVB3	15351	24161	0.46%	0.050%
20	13.928	1835	1843	1856	rBV	1969251	2839265	54.51%	5.852%
21	14.193	1881	1888	1902	rBV	2329456	3543535	68.03%	7.303%
22	14.498	1932	1940	1948	rBV	996583	1508793	28.97%	3.110%
23	14.716	1971	1977	1990	rBV	75060	193329	3.71%	0.398%
24	15.498	2103	2110	2125	rBV	2881737	4271164	82.00%	8.803%
25	15.622	2125	2131	2145	rVV	832052	1170072	22.46%	2.411%
26	15.740	2147	2151	2156	rVB5	16065	25879	0.50%	0.053%
27	15.916	2177	2181	2187	rBV8	3702	6309	0.12%	0.013%
28	16.069	2203	2207	2211	rBV7	4399	7089	0.14%	0.015%
29	16.287	2240	2244	2249	rVB4	9419	13583	0.26%	0.028%
30	16.928	2351	2353	2358	rVB6	4364	5395	0.10%	0.011%
31	16.986	2358	2363	2365	rBV5	4551	6248	0.12%	0.013%
32	17.028	2368	2370	2374	rVV5	4080	5601	0.11%	0.012%
33	17.251	2402	2408	2419	rBV	1223609	1775622	34.09%	3.659%
34	17.357	2419	2426	2442	rVV	3028417	4597928	88.28%	9.476%
35	17.763	2489	2495	2498	rBV6	5527	9550	0.18%	0.020%
36	17.934	2521	2524	2532	rVB7	7243	11515	0.22%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029908.D
Acq On : 22 Feb 2024 02:26
Operator : MA/JU
Sample : P1493-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	18.163	2559	2563	2569	rBV3	19992	31342	0.60%	0.065%
38	18.651	2642	2646	2650	rVB7	4464	5807	0.11%	0.012%
39	18.928	2688	2693	2698	rBV7	5910	13215	0.25%	0.027%
40	19.098	2719	2722	2724	rBV4	5153	5663	0.11%	0.012%
41	19.216	2738	2742	2747	rBV2	36382	50688	0.97%	0.104%
42	19.286	2750	2754	2759	rBV	32028	47242	0.91%	0.097%
43	19.451	2778	2782	2788	rBV6	12853	18979	0.36%	0.039%
44	19.604	2805	2808	2810	rBV4	10559	10910	0.21%	0.022%
45	19.651	2810	2816	2833	rVV	3789832	5208465	100.00%	10.734%
46	19.933	2862	2864	2865	rBV2	7334	6302	0.12%	0.013%
47	21.451	3117	3122	3137	rBV	1358175	1800885	34.58%	3.711%
48	23.663	3490	3498	3512	rBV2	2475163	5044920	96.86%	10.397%
49	23.816	3517	3524	3533	rVB	893985	1827990	35.10%	3.767%




Sum of corrected areas: 48521867

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029908.D
Acq On : 22 Feb 2024 02:26
Operator : MA/JU
Sample : P1493-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

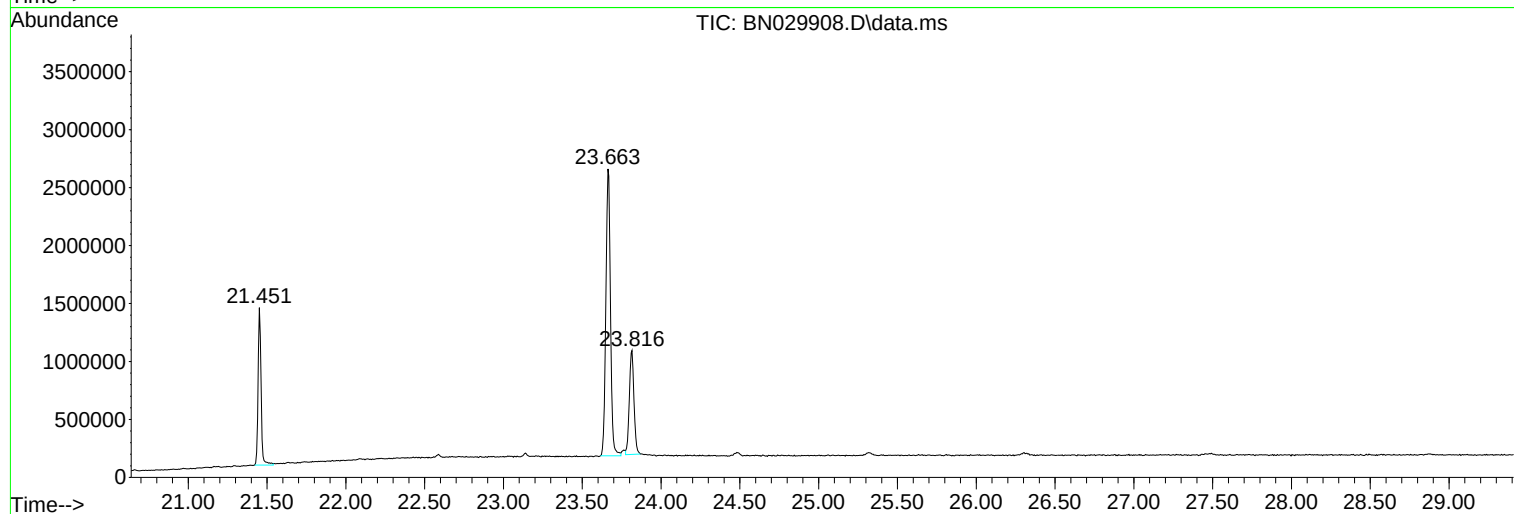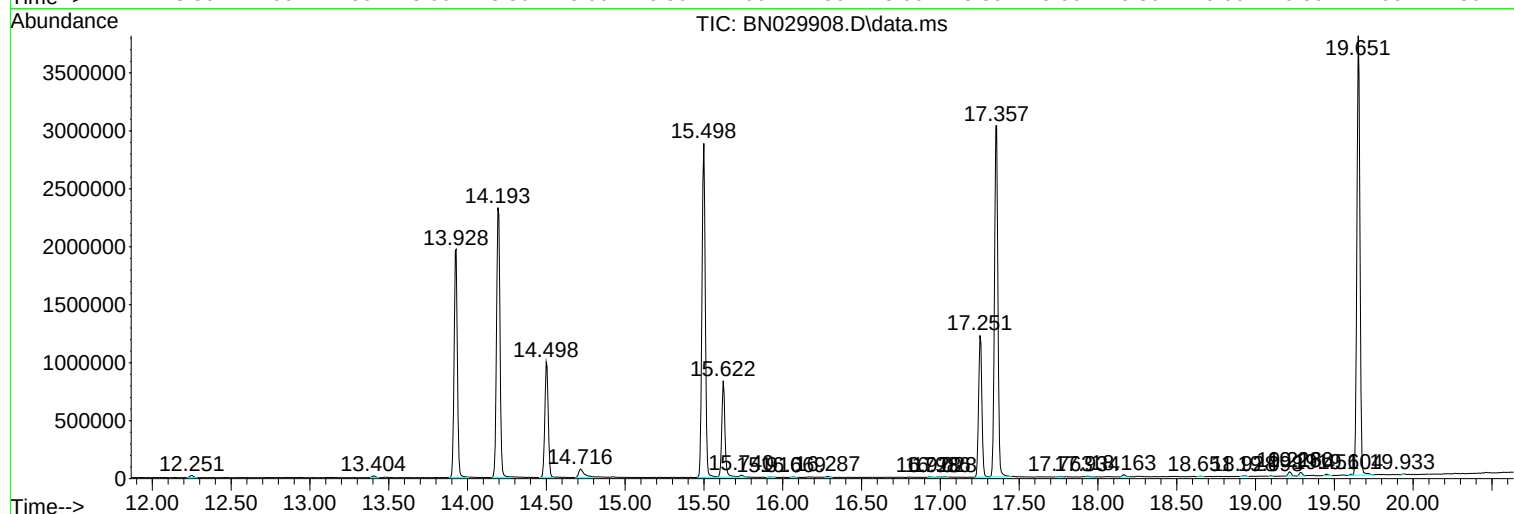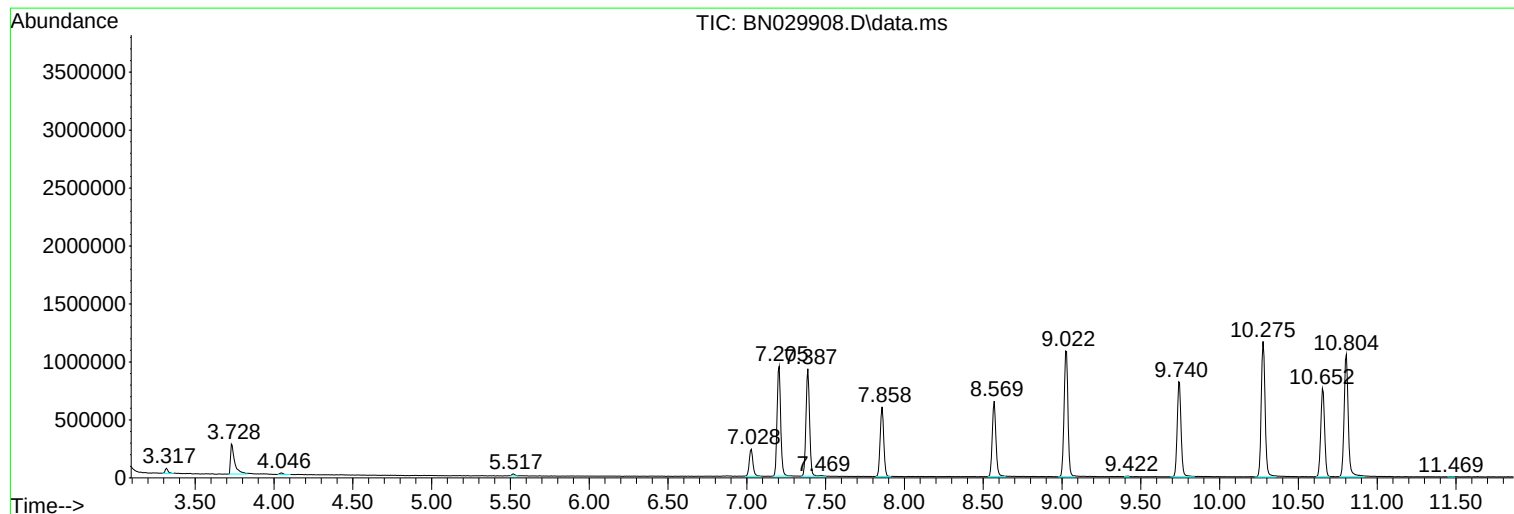

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029908.D
Acq On : 22 Feb 2024 02:26
Operator : MA/JU
Sample : P1493-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029908.D
Acq On : 22 Feb 2024 02:26
Operator : MA/JU
Sample : P1493-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc