

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029909.D
 Acq On : 22 Feb 2024 03:02
 Operator : MA/JU
 Sample : P1493-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	36	39	46	rVB	41189	54598	1.25%	0.129%
2	3.734	106	110	126	rBV	210868	402154	9.18%	0.953%
3	4.052	160	164	168	rVB	11353	16513	0.38%	0.039%
4	5.522	409	414	418	rBV2	14007	23249	0.53%	0.055%
5	7.028	663	670	680	rBV	180713	301105	6.87%	0.713%
6	7.205	692	700	713	rBV	795573	1295793	29.58%	3.070%
7	7.387	724	731	742	rBV	771791	1219501	27.84%	2.889%
8	7.463	742	744	750	rVB6	4843	6891	0.16%	0.016%
9	7.857	804	811	819	rBV	589840	929337	21.22%	2.202%
10	8.569	925	932	949	rBV	526968	874079	19.95%	2.071%
11	9.022	1000	1009	1022	rBV	932331	1560536	35.63%	3.697%
12	9.357	1061	1066	1074	rBV3	31330	63126	1.44%	0.150%
13	9.416	1074	1076	1084	rVB9	7878	12052	0.28%	0.029%
14	9.740	1124	1131	1146	rBV	678655	1171670	26.75%	2.776%
15	10.275	1214	1222	1239	rBV	957654	1648837	37.64%	3.906%
16	10.651	1279	1286	1295	rVB	762127	1271227	29.02%	3.012%
17	10.798	1304	1311	1326	rBV	896226	1683681	38.44%	3.989%
18	11.322	1394	1400	1405	rBV4	13211	26160	0.60%	0.062%
19	12.245	1552	1557	1567	rBV2	18268	34073	0.78%	0.081%
20	13.410	1748	1755	1761	rVB4	10986	18868	0.43%	0.045%
21	13.463	1761	1764	1770	rBV6	2479	5943	0.14%	0.014%
22	13.922	1834	1842	1857	rBV	1718454	2443906	55.79%	5.790%
23	14.034	1857	1861	1866	rVB7	10365	16394	0.37%	0.039%
24	14.192	1880	1888	1904	rBV2	2016764	3010590	68.73%	7.132%
25	14.498	1934	1940	1951	rBV	960083	1517717	34.65%	3.595%
26	14.722	1971	1978	1993	rBV3	48284	152828	3.49%	0.362%
27	15.498	2103	2110	2124	rBV	2495948	3612013	82.46%	8.557%
28	15.622	2125	2131	2143	rVV	628929	900436	20.56%	2.133%
29	15.734	2145	2150	2156	rVB5	19694	40131	0.92%	0.095%
30	16.286	2240	2244	2248	rVB5	7239	8672	0.20%	0.021%
31	16.339	2248	2253	2257	rBV2	10656	15169	0.35%	0.036%
32	16.398	2259	2263	2269	rBV3	9534	17834	0.41%	0.042%
33	16.463	2269	2274	2277	rBV5	9757	15037	0.34%	0.036%
34	16.504	2279	2281	2285	rVB4	7093	7676	0.18%	0.018%
35	16.657	2302	2307	2313	rBV6	7302	14734	0.34%	0.035%
36	16.728	2316	2319	2326	rVV	12583	22113	0.50%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029909.D
 Acq On : 22 Feb 2024 03:02
 Operator : MA/JU
 Sample : P1493-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.804	2329	2332	2336	rVB5	5794	9057	0.21%	0.021%
38	16.933	2350	2354	2357	rBV4	4583	5903	0.13%	0.014%
39	17.251	2402	2408	2419	rBV	1132265	1673645	38.21%	3.965%
40	17.351	2419	2425	2441	rVV2	2647139	3946494	90.10%	9.349%
41	17.457	2441	2443	2450	rVB7	10738	15878	0.36%	0.038%
42	18.163	2558	2563	2571	rBV3	23908	41688	0.95%	0.099%
43	18.710	2653	2656	2660	rVB5	4650	5147	0.12%	0.012%
44	19.216	2738	2742	2747	rBV	31025	45028	1.03%	0.107%
45	19.286	2748	2754	2759	rVV2	25871	39798	0.91%	0.094%
46	19.445	2779	2781	2789	rBV6	10788	18109	0.41%	0.043%
47	19.604	2805	2808	2810	rBV4	9111	9670	0.22%	0.023%
48	19.651	2810	2816	2827	rVV	3308484	4380337	100.00%	10.377%
49	21.451	3117	3122	3129	rBV	1189696	1633375	37.29%	3.869%
50	23.668	3491	3499	3510	rBV2	2065764	4153470	94.82%	9.840%
51	23.815	3517	3524	3542	rVB	839453	1819761	41.54%	4.311%




Sum of corrected areas: 42212003

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029909.D
Acq On : 22 Feb 2024 03:02
Operator : MA/JU
Sample : P1493-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

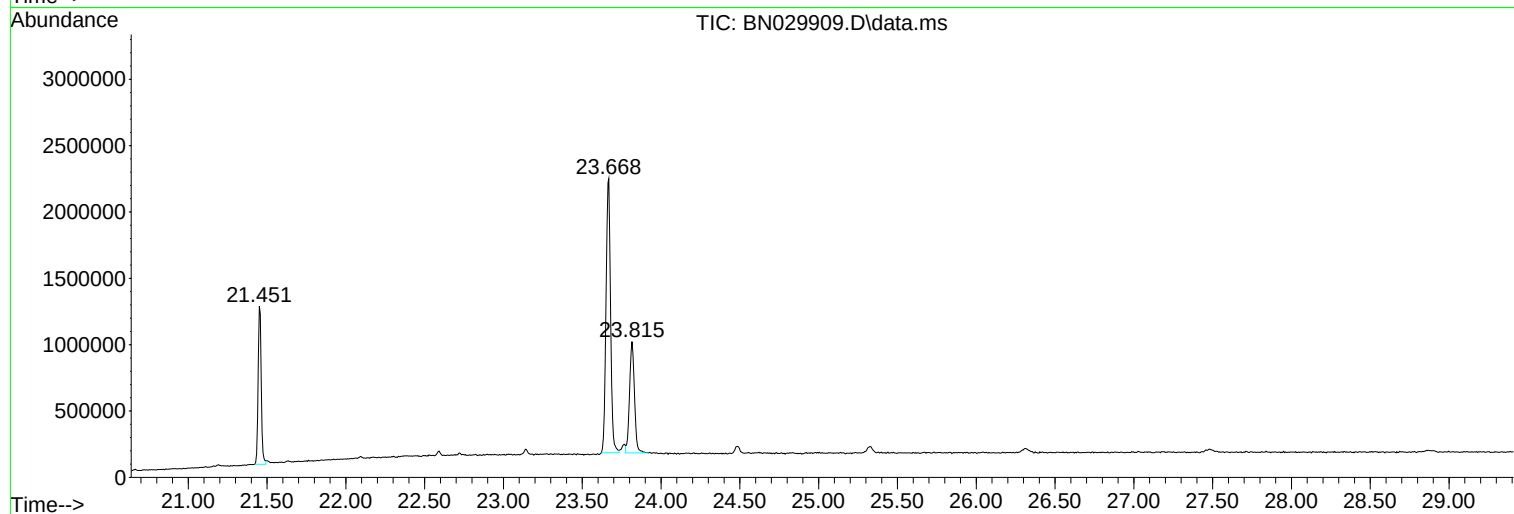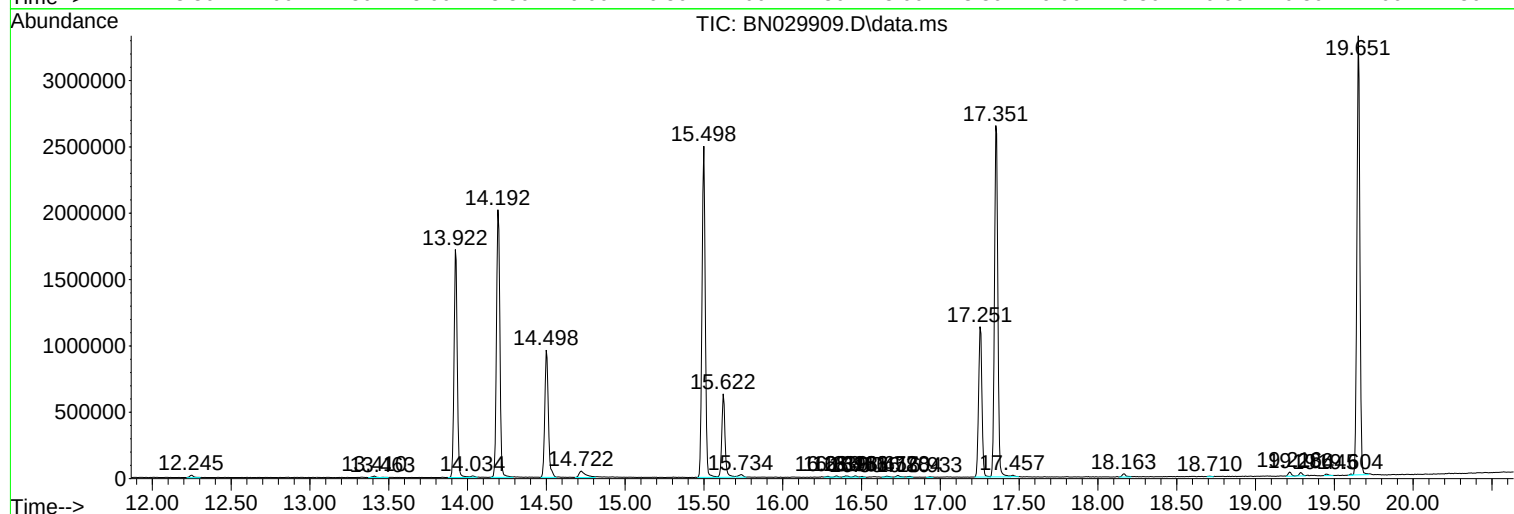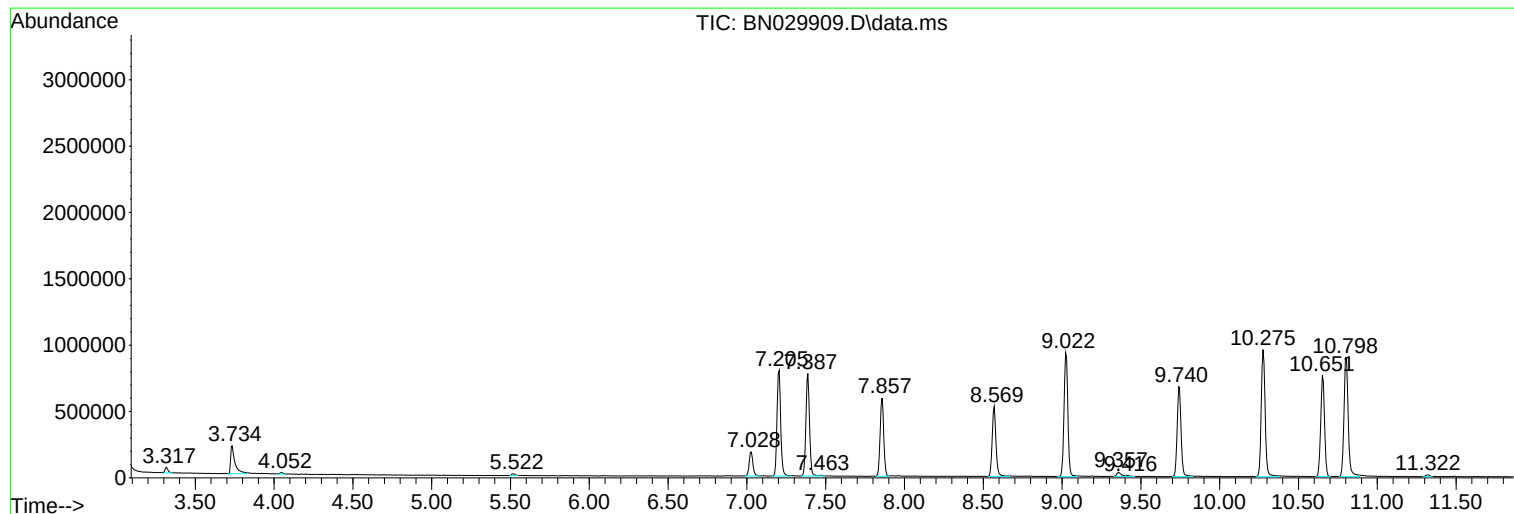

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029909.D
Acq On : 22 Feb 2024 03:02
Operator : MA/JU
Sample : P1493-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029909.D
Acq On : 22 Feb 2024 03:02
Operator : MA/JU
Sample : P1493-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------