

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029910.D
 Acq On : 22 Feb 2024 03:38
 Operator : MA/JU
 Sample : P1493-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	37	rBV	273574	369299	11.10%	1.057%
2	3.317	37	39	49	rVB	44698	64736	1.95%	0.185%
3	3.734	107	110	124	rBV	116146	222885	6.70%	0.638%
4	4.046	160	163	167	rVB	15579	17609	0.53%	0.050%
5	4.505	238	241	247	rBV7	4224	6419	0.19%	0.018%
6	5.517	409	413	417	rBV	12635	17332	0.52%	0.050%
7	6.540	580	587	589	rBV8	2221	4668	0.14%	0.013%
8	6.834	635	637	640	rBV4	2723	3703	0.11%	0.011%
9	6.881	640	645	647	rVV5	3057	5689	0.17%	0.016%
10	7.028	663	670	682	rVB	122825	215449	6.48%	0.616%
11	7.199	693	699	712	rBV	634774	1048539	31.52%	3.000%
12	7.387	724	731	741	rBV	579799	934294	28.08%	2.673%
13	7.858	804	811	820	rBV	585977	913790	27.47%	2.615%
14	7.928	820	823	826	rVV5	2888	3645	0.11%	0.010%
15	8.416	902	906	911	rVB6	1879	3436	0.10%	0.010%
16	8.569	925	932	945	rBV	375218	626706	18.84%	1.793%
17	8.658	945	947	953	rVV7	3502	6012	0.18%	0.017%
18	9.022	1002	1009	1023	rBV	743033	1241748	37.32%	3.553%
19	9.411	1070	1075	1076	rBV4	5063	5162	0.16%	0.015%
20	9.740	1124	1131	1143	rBV	534591	909828	27.35%	2.603%
21	10.275	1215	1222	1241	rBV	759847	1306612	39.27%	3.739%
22	10.399	1241	1243	1247	rVB5	3157	4477	0.13%	0.013%
23	10.652	1277	1286	1297	rVB	753926	1245641	37.44%	3.564%
24	10.799	1304	1311	1339	rBV	808974	1551811	46.64%	4.440%
25	12.081	1527	1529	1534	rBV4	3442	4743	0.14%	0.014%
26	12.246	1552	1557	1564	rBV2	13380	20995	0.63%	0.060%
27	12.993	1680	1684	1689	rVB7	2700	3991	0.12%	0.011%
28	13.116	1700	1705	1708	rVB6	3368	5032	0.15%	0.014%
29	13.328	1736	1741	1748	rBV7	6572	9575	0.29%	0.027%
30	13.404	1748	1754	1760	rVB3	11680	20734	0.62%	0.059%
31	13.469	1763	1765	1767	rBV3	3512	3985	0.12%	0.011%
32	13.922	1835	1842	1858	rBV	1378375	1970644	59.23%	5.639%
33	14.034	1858	1861	1864	rVV5	3667	5536	0.17%	0.016%
34	14.193	1879	1888	1901	rBV	1619794	2394475	71.97%	6.851%
35	14.410	1921	1925	1929	rBV7	2072	3376	0.10%	0.010%
36	14.498	1934	1940	1952	rBV	970976	1455824	43.76%	4.166%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029910.D
 Acq On : 22 Feb 2024 03:38
 Operator : MA/JU
 Sample : P1493-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	14.722	1972	1978	1992	rBV	29673	85050	2.56%	0.243%
38	15.316	2073	2079	2082	rVB8	3196	4638	0.14%	0.013%
39	15.428	2095	2098	2101	rBV4	2397	3507	0.11%	0.010%
40	15.498	2101	2110	2125	rBV	1980896	2870011	86.27%	8.212%
41	15.622	2125	2131	2143	rVV	463559	686833	20.64%	1.965%
42	15.740	2147	2151	2155	rVB6	10334	14407	0.43%	0.041%
43	15.840	2165	2168	2173	rVB5	2082	3368	0.10%	0.010%
44	15.969	2186	2190	2194	rVB6	2275	3471	0.10%	0.010%
45	16.069	2202	2207	2208	rBV4	3300	3941	0.12%	0.011%
46	16.281	2239	2243	2246	rBV5	6954	7664	0.23%	0.022%
47	16.663	2304	2308	2312	rBV5	3844	6207	0.19%	0.018%
48	17.040	2368	2372	2377	rBV6	3868	6467	0.19%	0.019%
49	17.251	2402	2408	2418	rBV	1120208	1642420	49.37%	4.699%
50	17.351	2419	2425	2437	rVV2	2059728	2974442	89.40%	8.511%
51	17.551	2457	2459	2464	rVB5	2492	3912	0.12%	0.011%
52	17.769	2493	2496	2499	rBV5	2537	3392	0.10%	0.010%
53	17.934	2522	2524	2529	rVB6	3371	4841	0.15%	0.014%
54	18.163	2558	2563	2570	rBV3	47591	68726	2.07%	0.197%
55	18.463	2611	2614	2617	rBV5	3282	4731	0.14%	0.014%
56	18.651	2642	2646	2648	rBV5	3827	4358	0.13%	0.012%
57	19.216	2737	2742	2748	rBV2	24655	35177	1.06%	0.101%
58	19.286	2750	2754	2758	rBV	21113	29846	0.90%	0.085%
59	19.334	2758	2762	2765	rVB6	8543	10450	0.31%	0.030%
60	19.451	2777	2782	2789	rBV6	21486	38844	1.17%	0.111%
61	19.604	2804	2808	2810	rBV4	9620	12218	0.37%	0.035%
62	19.651	2810	2816	2824	rVV	2451349	3326934	100.00%	9.519%
63	21.192	3074	3078	3087	rBV6	23457	42916	1.29%	0.123%
64	21.451	3117	3122	3135	rBV	1226081	1660057	49.90%	4.750%
65	23.663	3491	3498	3510	rBV	1543709	3111367	93.52%	8.902%
66	23.816	3518	3524	3534	rVB2	815112	1650833	49.62%	4.723%




Sum of corrected areas: 34949428

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

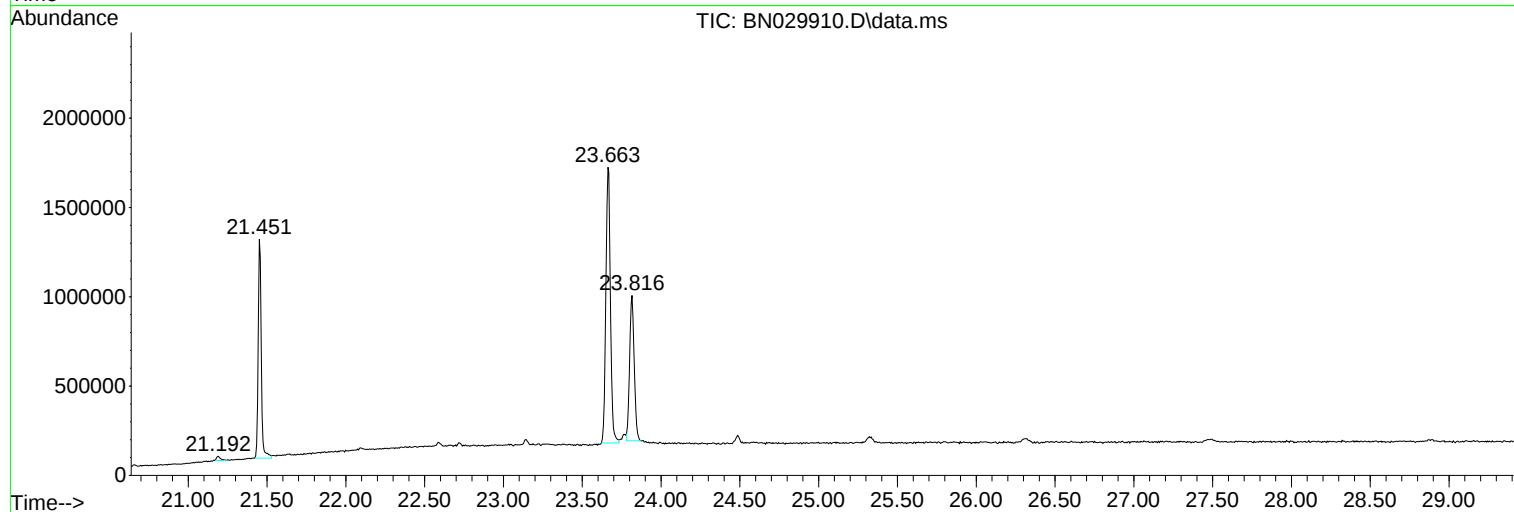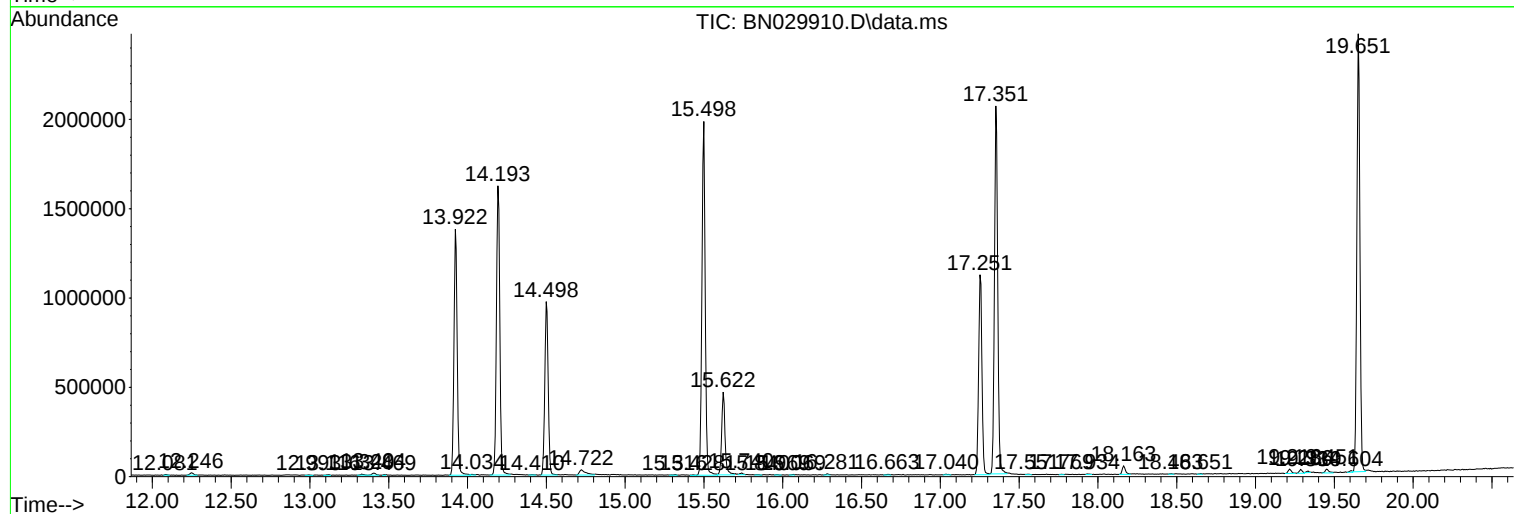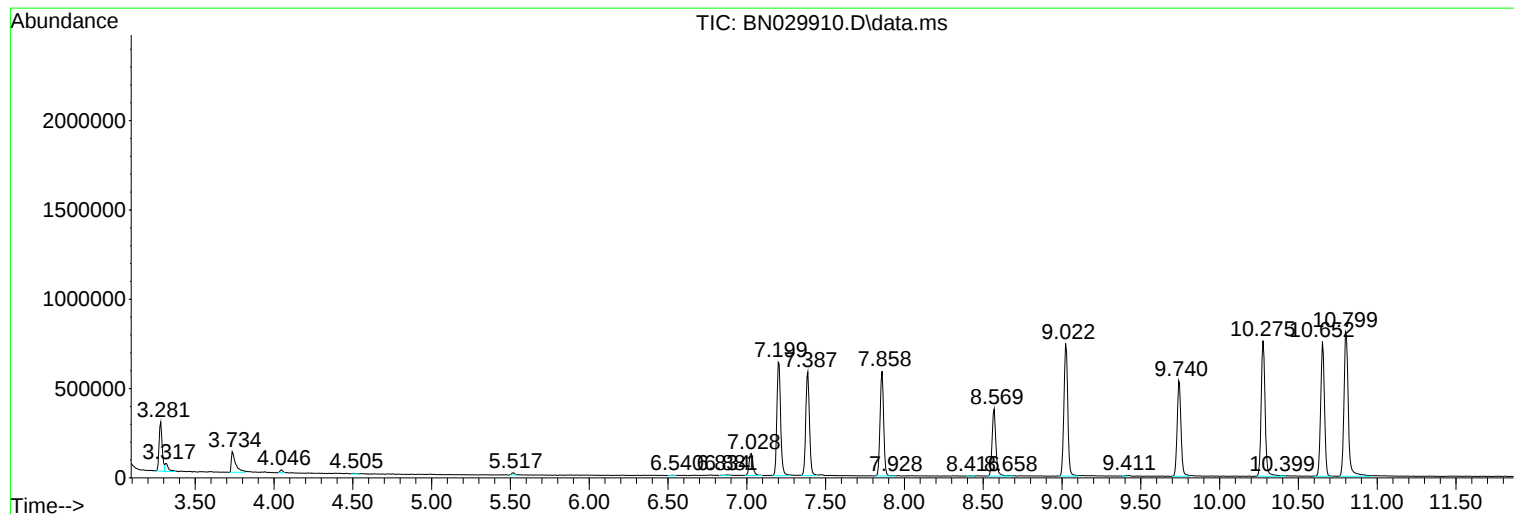

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029910.D
Acq On : 22 Feb 2024 03:38
Operator : MA/JU
Sample : P1493-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------