

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029911.D
 Acq On : 22 Feb 2024 04:14
 Operator : MA/JU
 Sample : P1493-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	43	rBV	34431	39277	0.91%	0.098%
2	3.734	107	110	124	rBV	126876	241402	5.61%	0.601%
3	4.046	160	163	168	rVB	11738	13533	0.31%	0.034%
4	5.517	409	413	419	rBV2	16047	20790	0.48%	0.052%
5	6.169	518	524	527	rBV7	2208	4662	0.11%	0.012%
6	7.028	664	670	681	rVB	156502	257412	5.98%	0.641%
7	7.199	691	699	710	rBV	692371	1127061	26.17%	2.805%
8	7.387	724	731	741	rBV	666042	1060031	24.62%	2.638%
9	7.858	804	811	822	rBV	568728	910607	21.15%	2.266%
10	8.569	924	932	944	rBV	453522	755023	17.53%	1.879%
11	9.022	1001	1009	1021	rBV	831281	1391930	32.33%	3.464%
12	9.187	1034	1037	1041	rVV5	4612	6975	0.16%	0.017%
13	9.416	1072	1076	1082	rVB3	7380	10928	0.25%	0.027%
14	9.740	1122	1131	1145	rBV	598579	1032761	23.98%	2.570%
15	10.275	1215	1222	1233	rBV	868143	1480254	34.38%	3.683%
16	10.652	1278	1286	1294	rVB	759968	1258101	29.22%	3.131%
17	10.804	1304	1312	1329	rBV	737743	1389945	32.28%	3.459%
18	12.246	1552	1557	1568	rVB2	16187	27598	0.64%	0.069%
19	13.334	1737	1742	1747	rVB3	8382	12909	0.30%	0.032%
20	13.404	1747	1754	1763	rBV3	15959	27537	0.64%	0.069%
21	13.922	1835	1842	1852	rBV	1626653	2312892	53.71%	5.755%
22	14.193	1881	1888	1904	rBV2	1942135	2823367	65.57%	7.026%
23	14.404	1923	1924	1930	rVB6	3859	4987	0.12%	0.012%
24	14.498	1933	1940	1950	rVV	980798	1480245	34.38%	3.683%
25	14.716	1971	1977	1989	rBV3	43599	120899	2.81%	0.301%
26	14.922	2008	2012	2021	rVB10	4911	12084	0.28%	0.030%
27	15.298	2073	2076	2080	rBV4	2950	5806	0.13%	0.014%
28	15.498	2103	2110	2124	rBV	2460219	3501069	81.31%	8.712%
29	15.622	2125	2131	2146	rVV	614424	893180	20.74%	2.223%
30	15.740	2146	2151	2155	rVB5	12373	18275	0.42%	0.045%
31	16.287	2239	2244	2248	rBV7	7646	12309	0.29%	0.031%
32	16.669	2305	2309	2313	rBV5	3362	4799	0.11%	0.012%
33	16.934	2350	2354	2357	rVB6	3938	6099	0.14%	0.015%
34	17.028	2365	2370	2374	rBV8	3525	6887	0.16%	0.017%
35	17.251	2402	2408	2418	rBV	1206913	1727317	40.11%	4.298%
36	17.351	2418	2425	2442	rVV2	2681781	3863003	89.71%	9.613%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029911.D
Acq On : 22 Feb 2024 04:14
Operator : MA/JU
Sample : P1493-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	17.557	2455	2460	2462	rBV6	2807	4328	0.10%	0.011%
38	18.163	2558	2563	2572	rBV2	58664	89778	2.08%	0.223%
39	18.316	2587	2589	2594	rBV6	3372	4612	0.11%	0.011%
40	19.216	2737	2742	2748	rBV3	32039	44208	1.03%	0.110%
41	19.286	2750	2754	2758	rBV2	26666	35137	0.82%	0.087%
42	19.451	2777	2782	2789	rBV5	27981	42691	0.99%	0.106%
43	19.604	2806	2808	2810	rBV2	8976	7255	0.17%	0.018%
44	19.651	2810	2816	2824	rVV	3171334	4306042	100.00%	10.715%
45	21.186	3074	3077	3087	rBV6	36958	58452	1.36%	0.145%
46	21.451	3117	3122	3132	rBV2	1239022	1745614	40.54%	4.344%
47	23.663	3491	3498	3509	rBV2	2089700	4170186	96.84%	10.377%
48	23.816	3517	3524	3533	rVB	908544	1816652	42.19%	4.521%




Sum of corrected areas: 40186909

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029911.D
Acq On : 22 Feb 2024 04:14
Operator : MA/JU
Sample : P1493-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

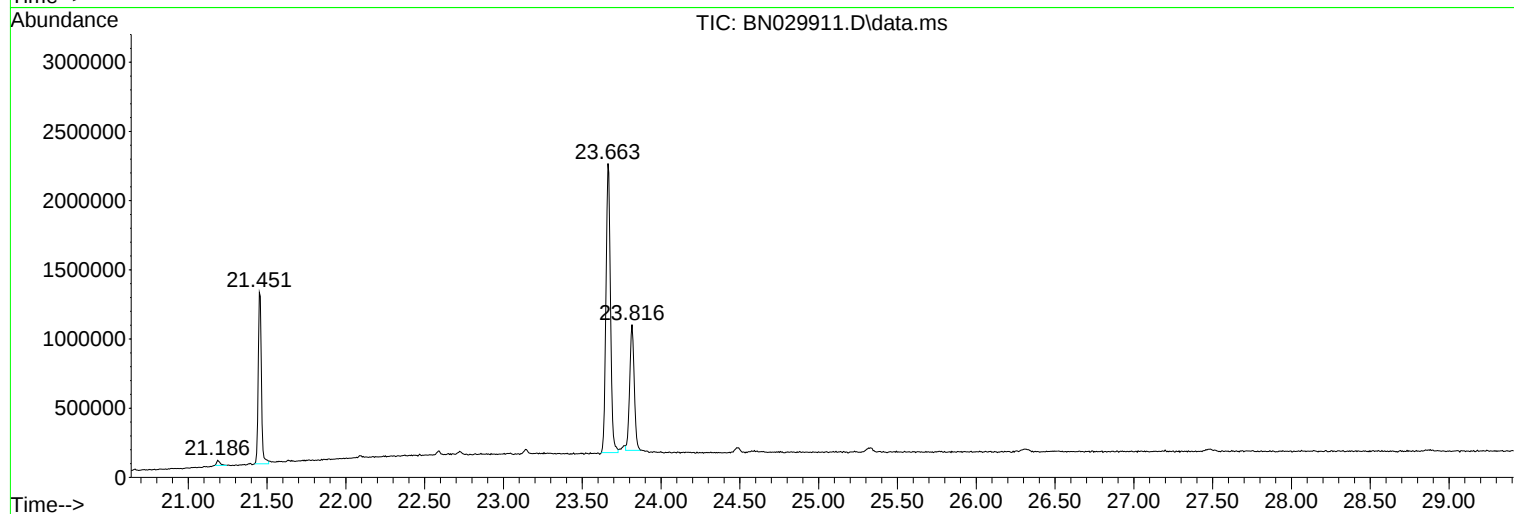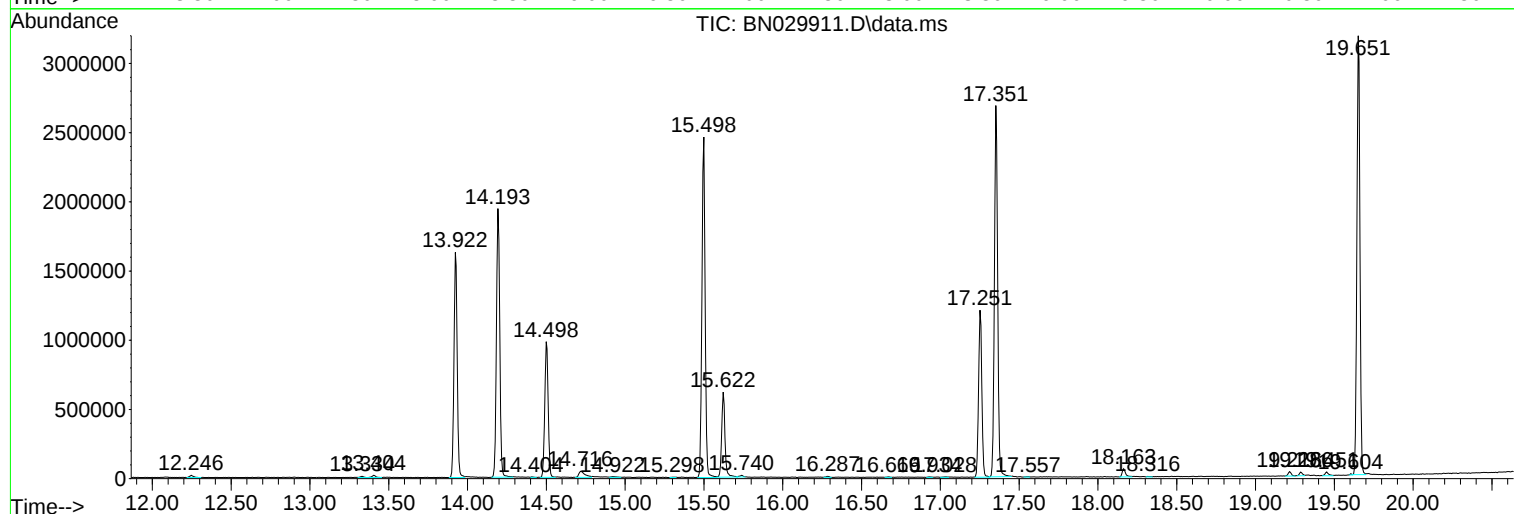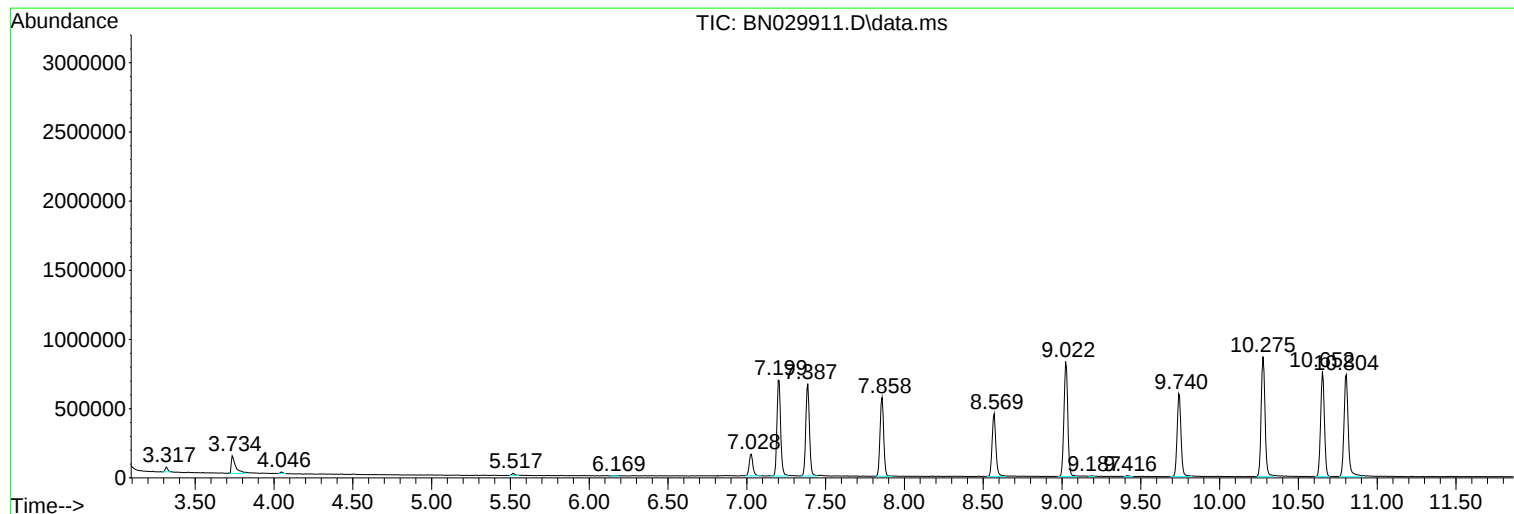

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029911.D
Acq On : 22 Feb 2024 04:14
Operator : MA/JU
Sample : P1493-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029911.D
Acq On : 22 Feb 2024 04:14
Operator : MA/JU
Sample : P1493-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------