

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029912.D
 Acq On : 22 Feb 2024 04:50
 Operator : MA/JU
 Sample : P1493-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	36	39	46	rVB	41287	54314	1.25%	0.126%
2	3.734	107	110	127	rBV	169694	326983	7.52%	0.756%
3	4.052	160	164	166	rVB	12587	15788	0.36%	0.036%
4	5.516	409	413	417	rBV	13943	18364	0.42%	0.042%
5	5.846	466	469	473	rVB5	3561	5033	0.12%	0.012%
6	5.905	475	479	484	rVB6	6473	10383	0.24%	0.024%
7	6.852	639	640	647	rBV6	2834	5187	0.12%	0.012%
8	7.028	663	670	683	rVB	178483	301102	6.93%	0.696%
9	7.199	693	699	716	rBV	818546	1347374	30.99%	3.114%
10	7.387	724	731	742	rBV	761744	1228882	28.26%	2.840%
11	7.857	804	811	819	rBV	638415	1006154	23.14%	2.325%
12	8.087	848	850	855	rVB5	3693	4382	0.10%	0.010%
13	8.569	925	932	943	rBV	517814	850974	19.57%	1.967%
14	9.022	1002	1009	1022	rBV	983093	1625418	37.38%	3.756%
15	9.134	1024	1028	1034	rVB3	16412	28896	0.66%	0.067%
16	9.252	1046	1048	1054	rVB6	2382	4375	0.10%	0.010%
17	9.416	1071	1076	1082	rVB5	5192	9243	0.21%	0.021%
18	9.740	1124	1131	1151	rBV	723010	1209435	27.82%	2.795%
19	10.275	1214	1222	1240	rBV	999095	1700208	39.10%	3.929%
20	10.651	1278	1286	1296	rVB	804932	1376870	31.67%	3.182%
21	10.804	1303	1312	1325	rBV	861882	1622562	37.32%	3.750%
22	12.245	1553	1557	1564	rBV2	17880	28135	0.65%	0.065%
23	13.404	1750	1754	1760	rBV2	11272	16994	0.39%	0.039%
24	13.922	1836	1842	1858	rBV	1796862	2530084	58.19%	5.847%
25	14.192	1881	1888	1901	rBV	2145225	3117626	71.70%	7.205%
26	14.498	1932	1940	1950	rBV	1092463	1596986	36.73%	3.691%
27	14.610	1957	1959	1965	rVB7	2940	5462	0.13%	0.013%
28	14.722	1971	1978	1989	rBV3	41450	121512	2.79%	0.281%
29	14.928	2012	2013	2020	rVB6	4622	5413	0.12%	0.013%
30	15.310	2073	2078	2082	rBV	11715	17069	0.39%	0.039%
31	15.357	2084	2086	2092	rVB5	2977	4482	0.10%	0.010%
32	15.498	2102	2110	2121	rBV	2539764	3744160	86.11%	8.653%
33	15.622	2125	2131	2146	rVV	659246	939679	21.61%	2.172%
34	15.734	2146	2150	2157	rVB5	12999	24297	0.56%	0.056%
35	16.281	2239	2243	2249	rVB4	8526	12976	0.30%	0.030%
36	16.933	2350	2354	2358	rBV7	3813	5801	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029912.D
Acq On : 22 Feb 2024 04:50
Operator : MA/JU
Sample : P1493-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	17.251	2402	2408	2416	rBV	1302538	1823891	41.95%	4.215%
38	17.351	2419	2425	2443	rVB	2815811	3982846	91.60%	9.204%
39	17.933	2518	2524	2525	rBV6	3592	5781	0.13%	0.013%
40	18.163	2558	2563	2569	rBV2	21757	33231	0.76%	0.077%
41	19.216	2737	2742	2747	rBV3	29785	42223	0.97%	0.098%
42	19.286	2748	2754	2758	rBV	27601	39652	0.91%	0.092%
43	19.357	2764	2766	2771	rBV6	3206	5069	0.12%	0.012%
44	19.451	2779	2782	2788	rBV5	19067	27290	0.63%	0.063%
45	19.610	2805	2809	2810	rBV3	10288	11452	0.26%	0.026%
46	19.651	2810	2816	2825	rVV	3185943	4347988	100.00%	10.048%
47	21.451	3117	3122	3137	rBV	1349017	1853067	42.62%	4.282%
48	23.668	3491	3499	3512	rBV2	2069586	4248626	97.71%	9.819%
49	23.815	3518	3524	3535	rVB	982231	1927636	44.33%	4.455%




Sum of corrected areas: 43271355

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029912.D
Acq On : 22 Feb 2024 04:50
Operator : MA/JU
Sample : P1493-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

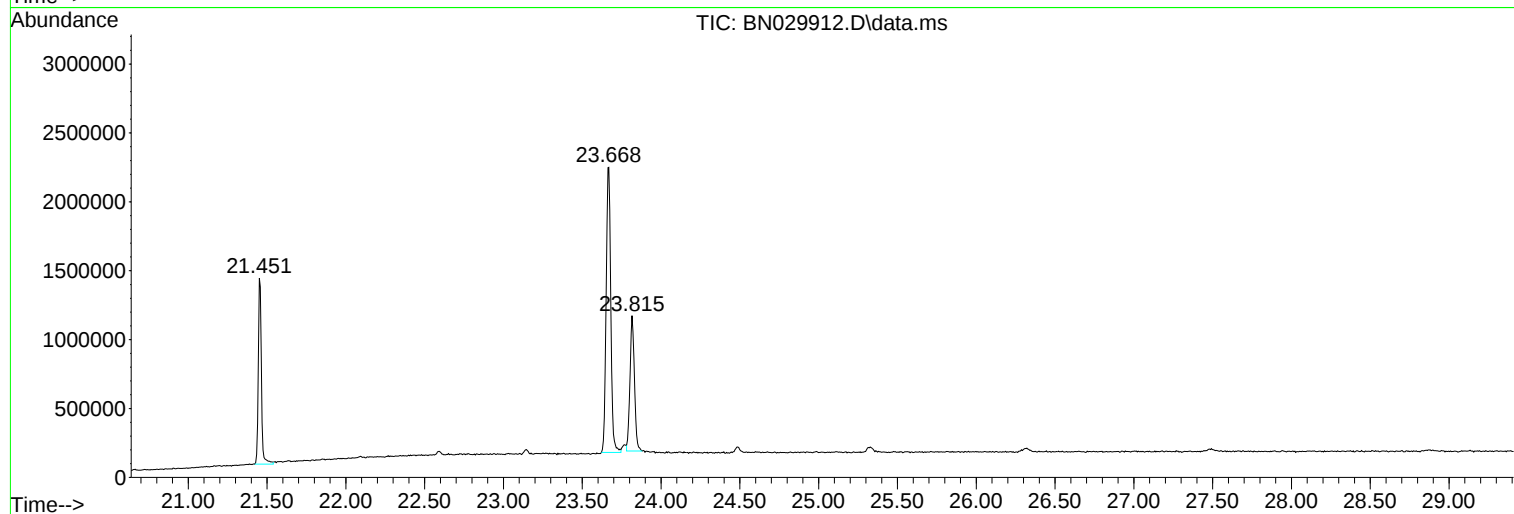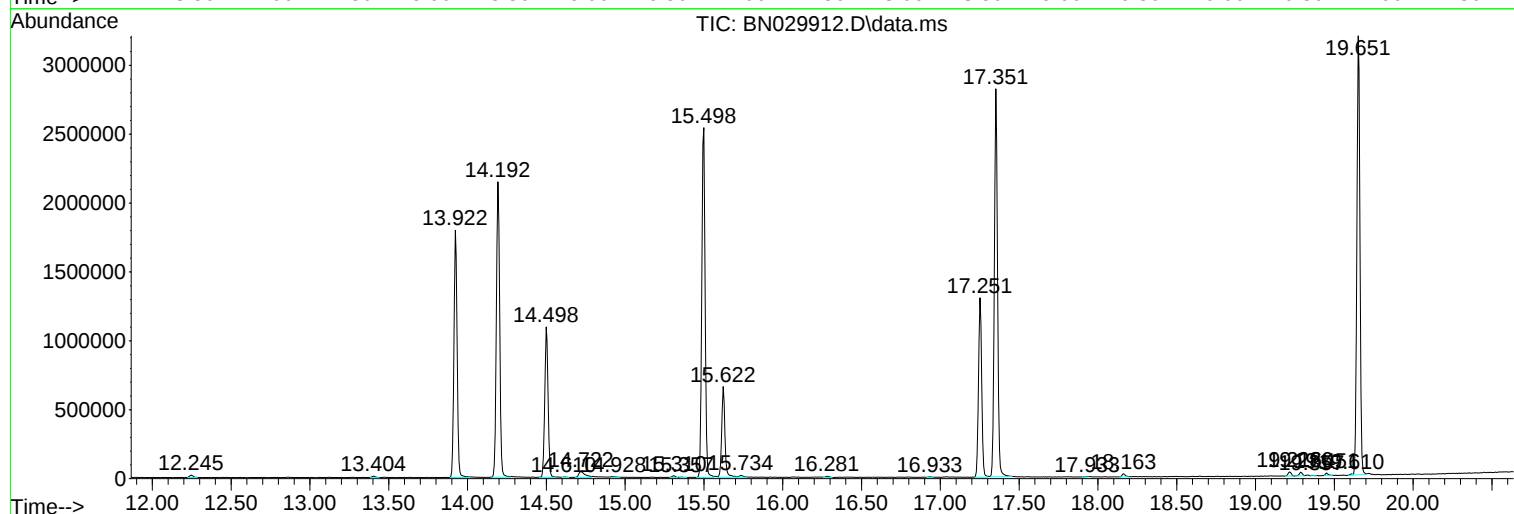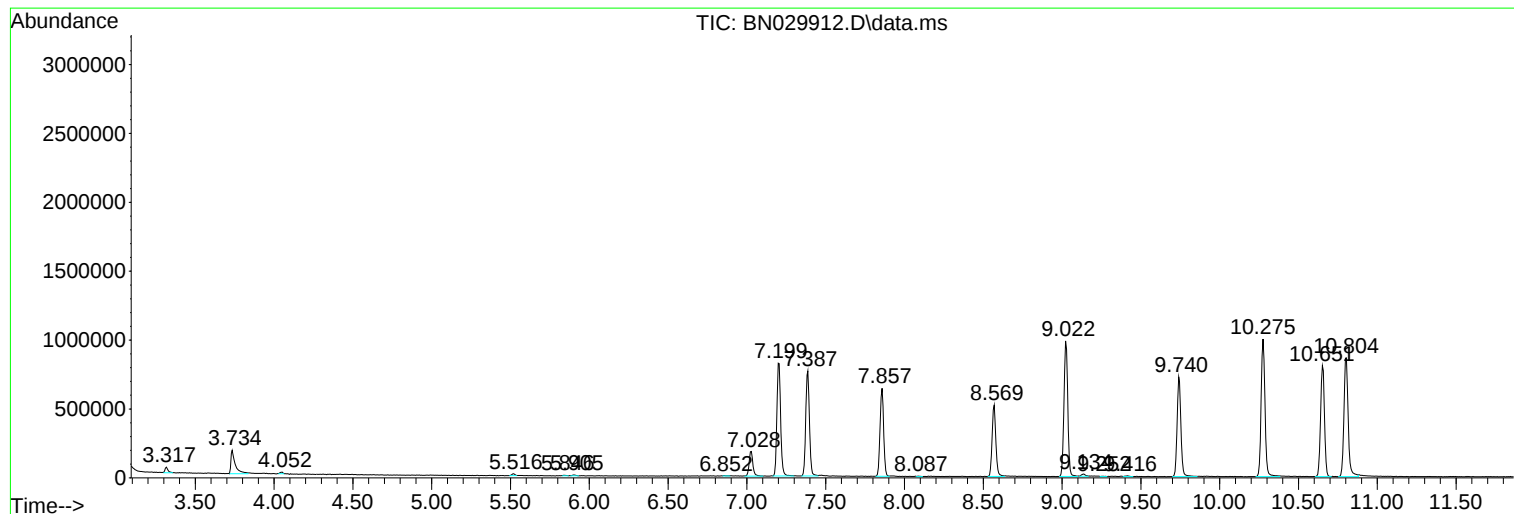

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029912.D
Acq On : 22 Feb 2024 04:50
Operator : MA/JU
Sample : P1493-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029912.D
Acq On : 22 Feb 2024 04:50
Operator : MA/JU
Sample : P1493-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc