

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029919.D
 Acq On : 22 Feb 2024 09:37
 Operator : MA/JU
 Sample : PB159098BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	45	rBV	71815	92048	2.10%	0.192%
2	3.722	105	108	127	rBV	829294	1351478	30.88%	2.822%
3	4.046	158	163	170	rVB3	31382	55037	1.26%	0.115%
4	4.217	189	192	198	rVB6	6795	12207	0.28%	0.025%
5	4.275	198	202	207	rBV3	23514	34318	0.78%	0.072%
6	4.422	224	227	232	rVB4	13234	20997	0.48%	0.044%
7	4.552	247	249	253	rVV4	4460	5413	0.12%	0.011%
8	4.605	253	258	263	rVV	50467	72172	1.65%	0.151%
9	4.658	264	267	276	rVB2	16903	37244	0.85%	0.078%
10	5.758	451	454	460	rVB7	6572	8992	0.21%	0.019%
11	6.181	522	526	530	rBV7	5408	9334	0.21%	0.019%
12	6.652	602	606	609	rBV6	5045	7767	0.18%	0.016%
13	6.693	609	613	617	rVV7	2707	6110	0.14%	0.013%
14	7.022	662	669	685	rBV	1056304	1721488	39.34%	3.594%
15	7.205	693	700	713	rBV	826888	1340319	30.63%	2.798%
16	7.387	724	731	741	rBV	1058005	1713804	39.16%	3.578%
17	7.569	757	762	766	rVB6	8220	14971	0.34%	0.031%
18	7.858	804	811	818	rVB	555356	880283	20.12%	1.838%
19	8.105	847	853	857	rVB5	5482	8670	0.20%	0.018%
20	8.569	924	932	946	rBV	1231076	1995738	45.61%	4.167%
21	8.834	972	977	982	rBV7	5996	12031	0.27%	0.025%
22	9.022	1002	1009	1021	rBV	974498	1613939	36.88%	3.370%
23	9.369	1064	1068	1071	rBV6	3234	4828	0.11%	0.010%
24	9.740	1124	1131	1145	rBV	765564	1283136	29.32%	2.679%
25	10.022	1172	1179	1182	rBV8	2989	5857	0.13%	0.012%
26	10.275	1214	1222	1240	rBV	1152603	1955783	44.69%	4.083%
27	10.516	1261	1263	1268	rVB6	3702	5862	0.13%	0.012%
28	10.652	1279	1286	1295	rBV	728594	1226556	28.03%	2.561%
29	10.799	1303	1311	1325	rBV	1093733	1996267	45.62%	4.168%
30	11.040	1347	1352	1358	rBV10	2903	6714	0.15%	0.014%
31	11.422	1411	1417	1419	rBV7	4398	7766	0.18%	0.016%
32	12.246	1550	1557	1564	rBV3	17708	31995	0.73%	0.067%
33	13.404	1748	1754	1760	rBV5	13092	23617	0.54%	0.049%
34	13.475	1760	1766	1771	rVB8	3411	5960	0.14%	0.012%
35	13.922	1833	1842	1855	rBV	1740745	2515446	57.48%	5.252%
36	14.193	1880	1888	1902	rBV	2126737	3100810	70.86%	6.474%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029919.D
 Acq On : 22 Feb 2024 09:37
 Operator : MA/JU
 Sample : PB159098BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	14.498	1933	1940	1950	rBV	943868	1419595	32.44%	2.964%
38	14.710	1967	1976	2000	rBV	582074	1171451	26.77%	2.446%
39	15.498	2103	2110	2122	rBV	2543292	3694227	84.42%	7.713%
40	15.622	2124	2131	2140	rBV	676881	945190	21.60%	1.973%
41	15.739	2147	2151	2158	rVB5	13798	25719	0.59%	0.054%
42	16.063	2203	2206	2212	rBV6	2581	4884	0.11%	0.010%
43	16.287	2238	2244	2247	rVB5	7774	11075	0.25%	0.023%
44	16.934	2348	2354	2358	rBV6	3453	4550	0.10%	0.009%
45	17.251	2400	2408	2416	rBV	1129307	1621913	37.06%	3.386%
46	17.351	2419	2425	2441	rVV2	2743596	3917596	89.53%	8.179%
47	17.675	2476	2480	2484	rVB7	2606	5248	0.12%	0.011%
48	18.169	2560	2564	2570	rBV7	4092	7816	0.18%	0.016%
49	19.216	2738	2742	2749	rVB5	31816	46280	1.06%	0.097%
50	19.286	2749	2754	2758	rBV2	30791	44022	1.01%	0.092%
51	19.610	2806	2809	2810	rBV3	6636	6504	0.15%	0.014%
52	19.657	2810	2817	2824	rVV	3232739	4375899	100.00%	9.136%
53	21.457	3117	3123	3133	rBV	1191503	1624203	37.12%	3.391%
54	23.668	3491	3499	3510	rBV2	2025876	4138031	94.56%	8.639%
55	23.816	3518	3524	3538	rVB	797120	1647652	37.65%	3.440%




Sum of corrected areas: 47896812

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029919.D
Acq On : 22 Feb 2024 09:37
Operator : MA/JU
Sample : PB159098BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

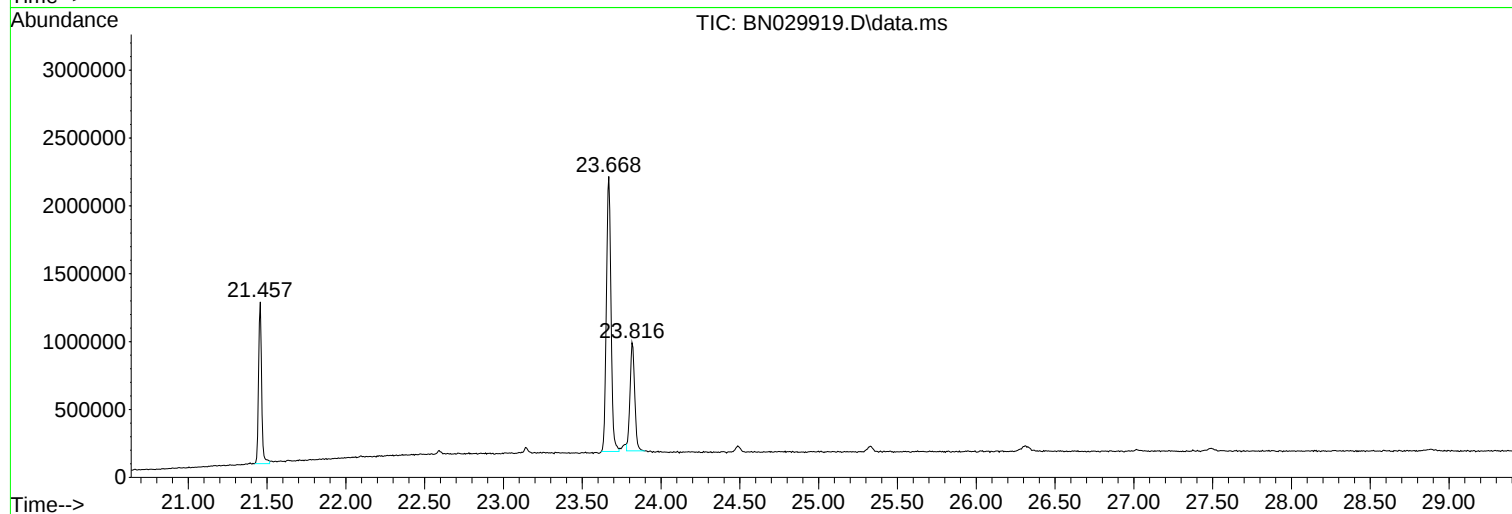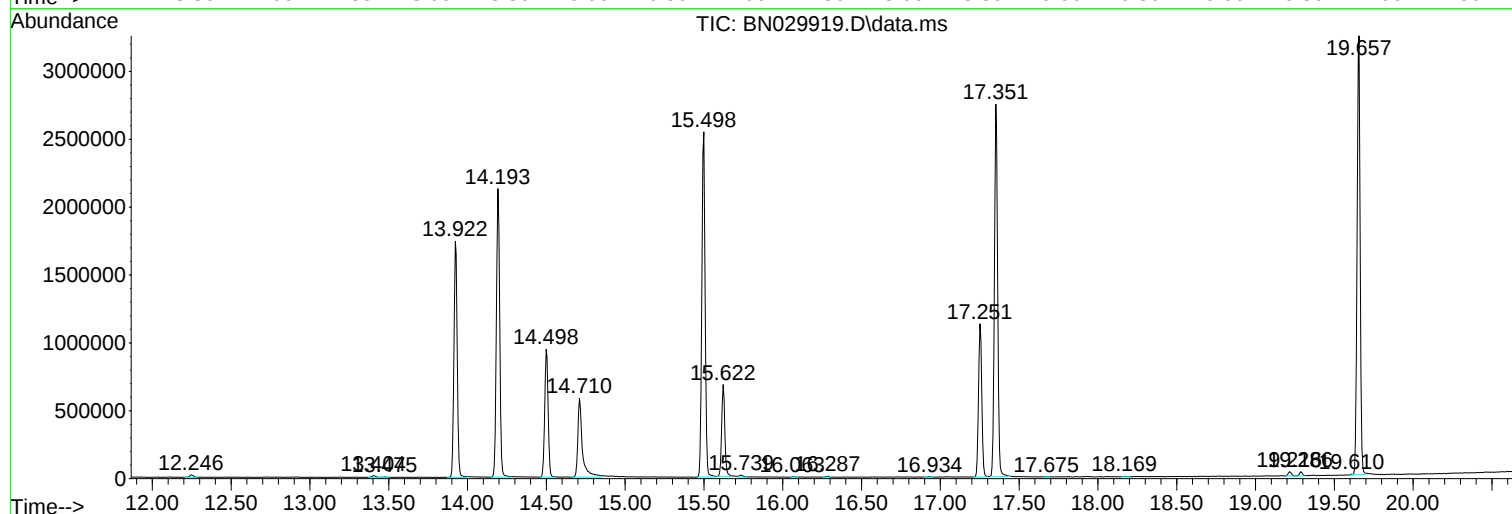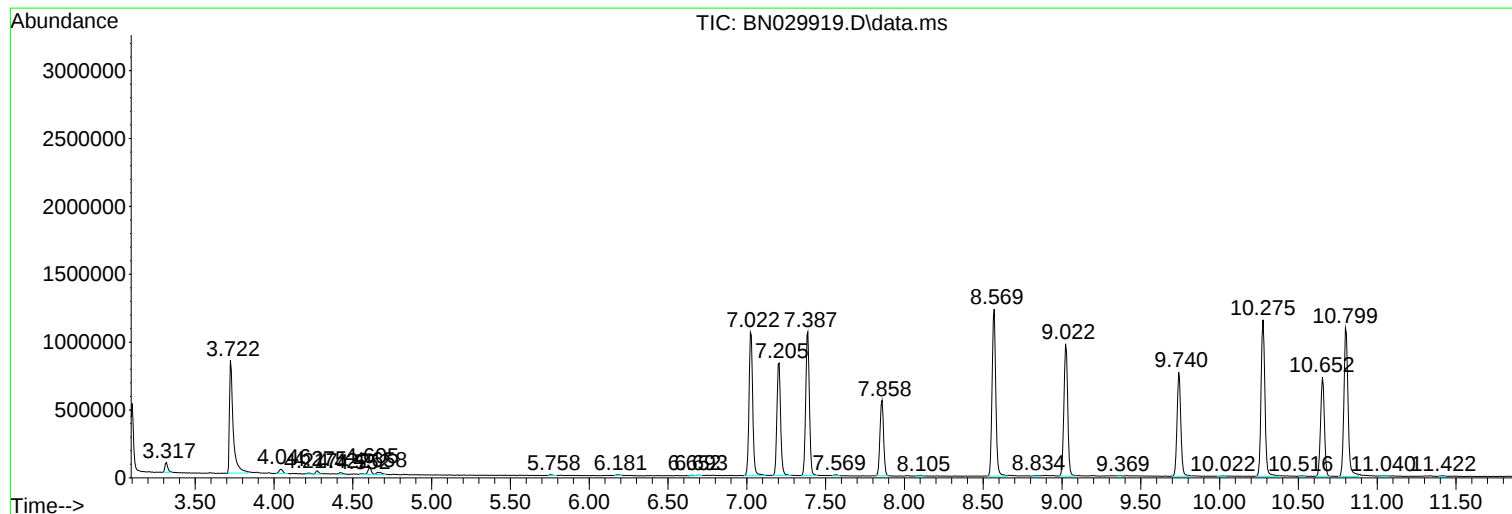

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029919.D
Acq On : 22 Feb 2024 09:37
Operator : MA/JU
Sample : PB159098BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029919.D
Acq On : 22 Feb 2024 09:37
Operator : MA/JU
Sample : PB159098BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc