

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029920.D
 Acq On : 22 Feb 2024 10:13
 Operator : MA/JU
 Sample : P1493-15
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	35	39	44	rBV	39213	51610	1.16%	0.120%
2	3.734	106	110	123	rBV	186764	344142	7.71%	0.799%
3	4.046	160	163	169	rVB3	13589	19561	0.44%	0.045%
4	5.516	409	413	420	rBV	16598	26444	0.59%	0.061%
5	6.869	641	643	648	rVB6	3270	4940	0.11%	0.011%
6	7.028	664	670	681	rVB	199588	328079	7.35%	0.761%
7	7.205	693	700	710	rBV	823353	1333080	29.87%	3.094%
8	7.387	724	731	742	rBV	791620	1277809	28.63%	2.966%
9	7.475	742	746	751	rVB5	5189	8281	0.19%	0.019%
10	7.857	804	811	820	rVB	603773	935476	20.96%	2.171%
11	8.569	925	932	942	rBV	564350	909960	20.39%	2.112%
12	9.022	1002	1009	1022	rBV	973682	1605704	35.98%	3.727%
13	9.134	1025	1028	1033	rVB6	7376	11613	0.26%	0.027%
14	9.193	1033	1038	1041	rBV5	5366	6543	0.15%	0.015%
15	9.416	1071	1076	1079	rBV4	3156	4775	0.11%	0.011%
16	9.457	1079	1083	1088	rVB7	5788	11028	0.25%	0.026%
17	9.740	1123	1131	1139	rBV	720729	1214115	27.21%	2.818%
18	10.075	1186	1188	1192	rBV4	4532	5529	0.12%	0.013%
19	10.275	1215	1222	1235	rBV	1022633	1717014	38.47%	3.985%
20	10.651	1279	1286	1293	rBV	777320	1288879	28.88%	2.991%
21	10.804	1303	1312	1325	rBV	812377	1536446	34.43%	3.566%
22	11.063	1350	1356	1364	rVB	6229	16443	0.37%	0.038%
23	11.216	1378	1382	1384	rBV5	3360	4642	0.10%	0.011%
24	11.457	1420	1423	1426	rBV4	5741	10632	0.24%	0.025%
25	11.481	1426	1427	1432	rVV4	7529	7699	0.17%	0.018%
26	12.087	1525	1530	1537	rVB7	5085	9163	0.21%	0.021%
27	12.251	1550	1558	1565	rVB3	17663	32360	0.73%	0.075%
28	13.334	1735	1742	1745	rBV4	10692	16275	0.36%	0.038%
29	13.404	1748	1754	1760	rVB6	9283	16199	0.36%	0.038%
30	13.481	1760	1767	1769	rBV7	2426	4620	0.10%	0.011%
31	13.922	1835	1842	1857	rBV	1740359	2518438	56.43%	5.845%
32	14.192	1881	1888	1904	rBV	2082021	3081231	69.04%	7.151%
33	14.410	1921	1925	1930	rVB4	12210	17229	0.39%	0.040%
34	14.498	1934	1940	1950	rBV	972189	1493518	33.47%	3.466%
35	14.716	1971	1977	1985	rBV2	56905	138403	3.10%	0.321%
36	14.916	2008	2011	2014	rBV5	4952	7264	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029920.D
 Acq On : 22 Feb 2024 10:13
 Operator : MA/JU
 Sample : P1493-15
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	14.939	2014	2015	2021	rVV6	3391	4667	0.10%	0.011%
38	15.022	2025	2029	2034	rVB7	3770	5312	0.12%	0.012%
39	15.310	2074	2078	2082	rBV5	4898	7233	0.16%	0.017%
40	15.363	2082	2087	2093	rVB3	18238	25434	0.57%	0.059%
41	15.498	2102	2110	2125	rBV	2538638	3751155	84.06%	8.706%
42	15.622	2125	2131	2145	rVV	639997	931290	20.87%	2.161%
43	15.733	2148	2150	2156	rVV6	8587	12064	0.27%	0.028%
44	15.928	2179	2183	2186	rVB5	3426	4912	0.11%	0.011%
45	15.981	2189	2192	2197	rVB7	3737	6577	0.15%	0.015%
46	16.063	2199	2206	2210	rBV8	4028	8541	0.19%	0.020%
47	16.228	2230	2234	2241	rBV3	23735	35628	0.80%	0.083%
48	16.286	2241	2244	2248	rVB6	8437	10839	0.24%	0.025%
49	16.733	2318	2320	2325	rVB6	5164	6938	0.16%	0.016%
50	16.810	2325	2333	2335	rBV10	4042	8796	0.20%	0.020%
51	16.933	2351	2354	2359	rBV7	3298	5088	0.11%	0.012%
52	17.022	2366	2369	2375	rBV4	21333	32486	0.73%	0.075%
53	17.080	2375	2379	2383	rVB7	4903	7908	0.18%	0.018%
54	17.251	2402	2408	2418	rBV	1152510	1695849	38.00%	3.936%
55	17.351	2419	2425	2439	rVV	2718322	3951485	88.55%	9.171%
56	17.563	2456	2461	2465	rVB7	4496	7701	0.17%	0.018%
57	17.769	2492	2496	2503	rBV3	18584	32425	0.73%	0.075%
58	18.045	2538	2543	2545	rBV6	4500	7756	0.17%	0.018%
59	18.163	2558	2563	2572	rBV3	68186	98149	2.20%	0.228%
60	18.463	2610	2614	2618	rBV3	11806	16728	0.37%	0.039%
61	19.069	2715	2717	2719	rBV3	5458	6070	0.14%	0.014%
62	19.104	2719	2723	2729	rVB6	11855	19990	0.45%	0.046%
63	19.216	2738	2742	2747	rBV2	32687	46198	1.04%	0.107%
64	19.286	2748	2754	2758	rBV	29778	44271	0.99%	0.103%
65	19.333	2758	2762	2764	rBV5	8027	10396	0.23%	0.024%
66	19.451	2779	2782	2787	rBV2	32397	41888	0.94%	0.097%
67	19.604	2805	2808	2810	rBV3	13392	14401	0.32%	0.033%
68	19.657	2810	2817	2826	rVV	3210005	4462684	100.00%	10.357%
69	21.186	3075	3077	3087	rVB8	29245	48906	1.10%	0.114%
70	21.457	3117	3123	3133	rBV	1256950	1724965	38.65%	4.003%
71	23.668	3491	3499	3510	rBV2	2162176	4253228	95.31%	9.871%
72	23.821	3518	3525	3535	rVB	866596	1724501	38.64%	4.002%




Sum of corrected areas: 43087603

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029920.D
Acq On : 22 Feb 2024 10:13
Operator : MA/JU
Sample : P1493-15
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

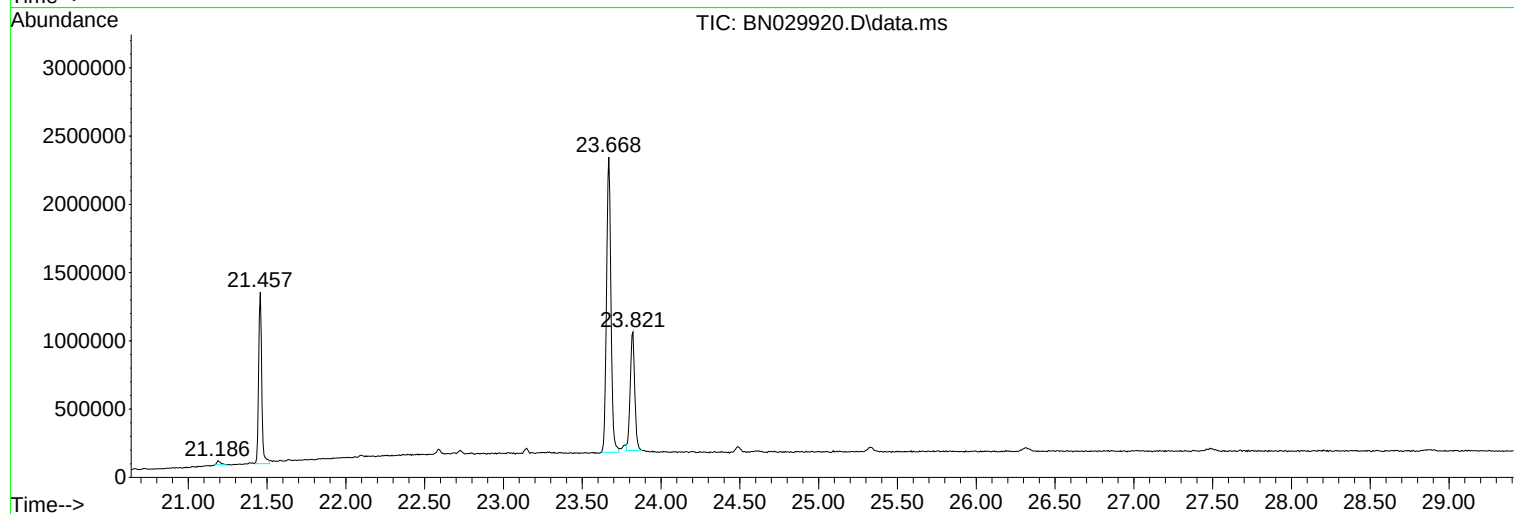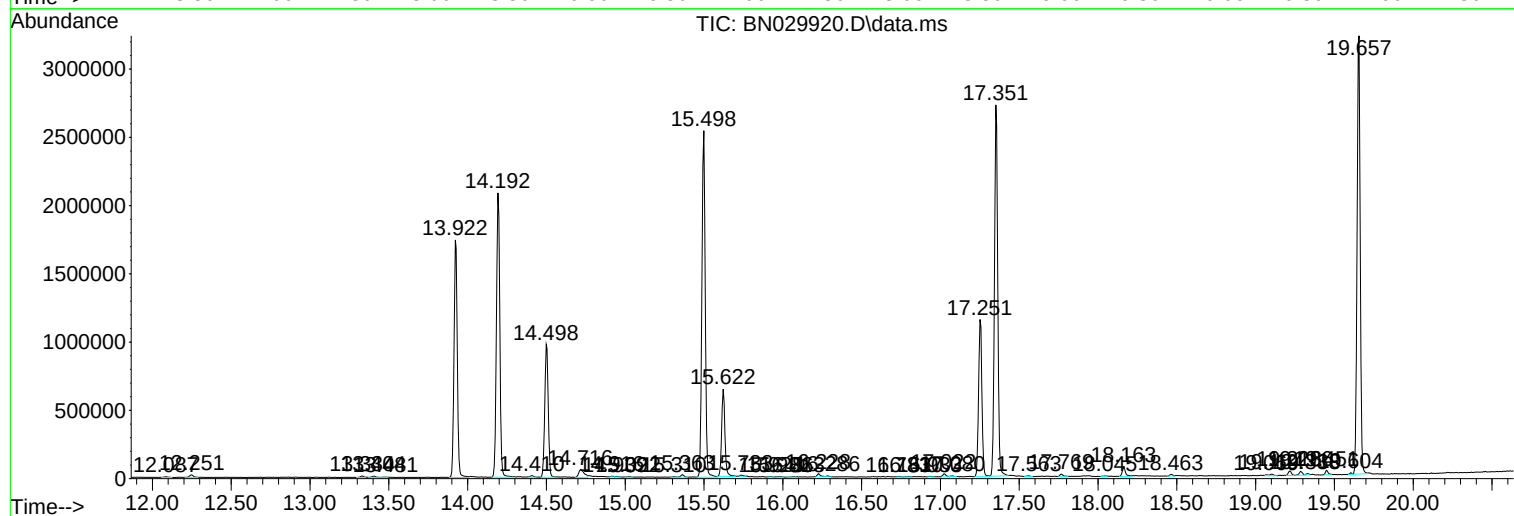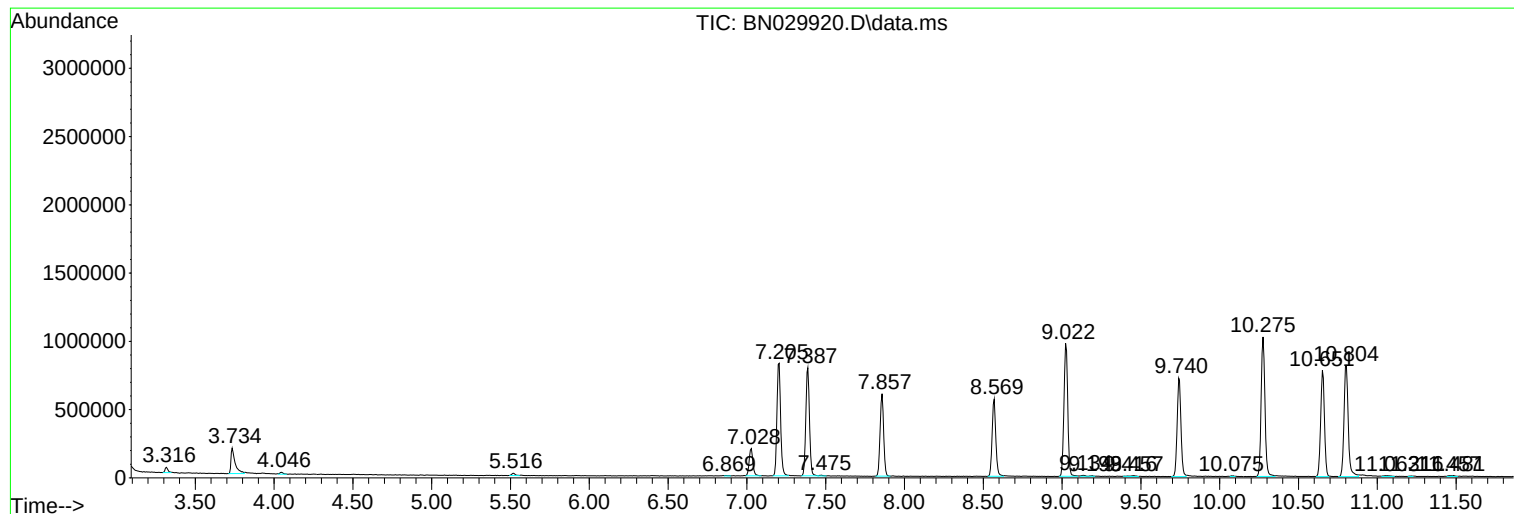

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029920.D
Acq On : 22 Feb 2024 10:13
Operator : MA/JU
Sample : P1493-15
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029920.D
Acq On : 22 Feb 2024 10:13
Operator : MA/JU
Sample : P1493-15
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc