

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029924.D
 Acq On : 22 Feb 2024 12:38
 Operator : MA/JU
 Sample : P1493-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	36	rBV4	11861	11686	0.24%	0.026%
2	3.317	36	39	45	rVB	43282	51189	1.07%	0.112%
3	3.734	106	110	126	rBV	224731	425351	8.88%	0.934%
4	4.046	160	163	166	rBV2	11496	14355	0.30%	0.032%
5	5.516	409	413	418	rBV	15975	20722	0.43%	0.045%
6	7.022	663	669	683	rVB	223039	374313	7.81%	0.822%
7	7.199	693	699	718	rVB	873261	1422126	29.68%	3.122%
8	7.387	723	731	743	rVV	859391	1368322	28.55%	3.004%
9	7.469	743	745	751	rVB6	6240	9238	0.19%	0.020%
10	7.858	802	811	821	rBV	596189	951719	19.86%	2.090%
11	8.569	923	932	946	rBV	621706	1024174	21.37%	2.249%
12	9.022	1001	1009	1022	rBV	1027346	1706714	35.61%	3.747%
13	9.187	1035	1037	1041	rVB5	4585	5556	0.12%	0.012%
14	9.410	1070	1075	1081	rVB3	7053	13260	0.28%	0.029%
15	9.740	1123	1131	1143	rBV	764059	1283471	26.78%	2.818%
16	10.275	1213	1222	1233	rBV	1073719	1830555	38.20%	4.019%
17	10.651	1278	1286	1297	rBV	760250	1289063	26.90%	2.830%
18	10.799	1304	1311	1329	rBV	957789	1798643	37.53%	3.949%
19	11.463	1418	1424	1433	rVB	6601	15503	0.32%	0.034%
20	12.246	1552	1557	1565	rVB2	17874	32276	0.67%	0.071%
21	13.334	1735	1742	1745	rBV6	8919	15154	0.32%	0.033%
22	13.404	1749	1754	1759	rVV3	14274	25766	0.54%	0.057%
23	13.922	1836	1842	1852	rBV	1860596	2663562	55.58%	5.848%
24	14.192	1881	1888	1902	rBV	2232154	3278347	68.41%	7.198%
25	14.498	1933	1940	1952	rBV	975309	1463060	30.53%	3.212%
26	14.716	1971	1977	1994	rBV	65247	170553	3.56%	0.374%
27	14.928	2007	2013	2020	rVB8	10529	22749	0.47%	0.050%
28	15.498	2102	2110	2125	rBV	2700734	3946002	82.34%	8.664%
29	15.622	2125	2131	2144	rVV	745121	1064094	22.20%	2.336%
30	15.739	2147	2151	2156	rVB3	12561	18500	0.39%	0.041%
31	16.281	2240	2243	2249	rVB5	7471	10029	0.21%	0.022%
32	16.663	2305	2308	2313	rVB3	12084	14474	0.30%	0.032%
33	17.039	2367	2372	2374	rBV5	4163	7525	0.16%	0.017%
34	17.251	2401	2408	2419	rBV	1166208	1646816	34.36%	3.616%
35	17.351	2419	2425	2438	rBV2	2930537	4265293	89.00%	9.365%
36	17.939	2521	2525	2531	rVB8	7644	12579	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029924.D
 Acq On : 22 Feb 2024 12:38
 Operator : MA/JU
 Sample : P1493-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z4

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	18.033	2537	2541	2545	rBV5	8281	9436	0.20%	0.021%
38	18.163	2557	2563	2571	rBV	111616	158683	3.31%	0.348%
39	19.216	2738	2742	2746	rBV4	34336	48451	1.01%	0.106%
40	19.286	2750	2754	2758	rBV2	28235	39933	0.83%	0.088%
41	19.327	2758	2761	2766	rVB6	12500	17400	0.36%	0.038%
42	19.451	2778	2782	2787	rBV3	34470	46745	0.98%	0.103%
43	19.604	2805	2808	2810	rBV3	11079	11816	0.25%	0.026%
44	19.651	2810	2816	2825	rVV	3588608	4792226	100.00%	10.522%
45	21.192	3074	3078	3084	rBV4	56057	95189	1.99%	0.209%
46	21.457	3117	3123	3135	rBV	1232575	1673908	34.93%	3.675%
47	23.668	3491	3499	3511	rBV2	2311735	4650898	97.05%	10.212%
48	23.815	3518	3524	3537	rVB	834571	1728175	36.06%	3.794%




Sum of corrected areas: 45545599

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

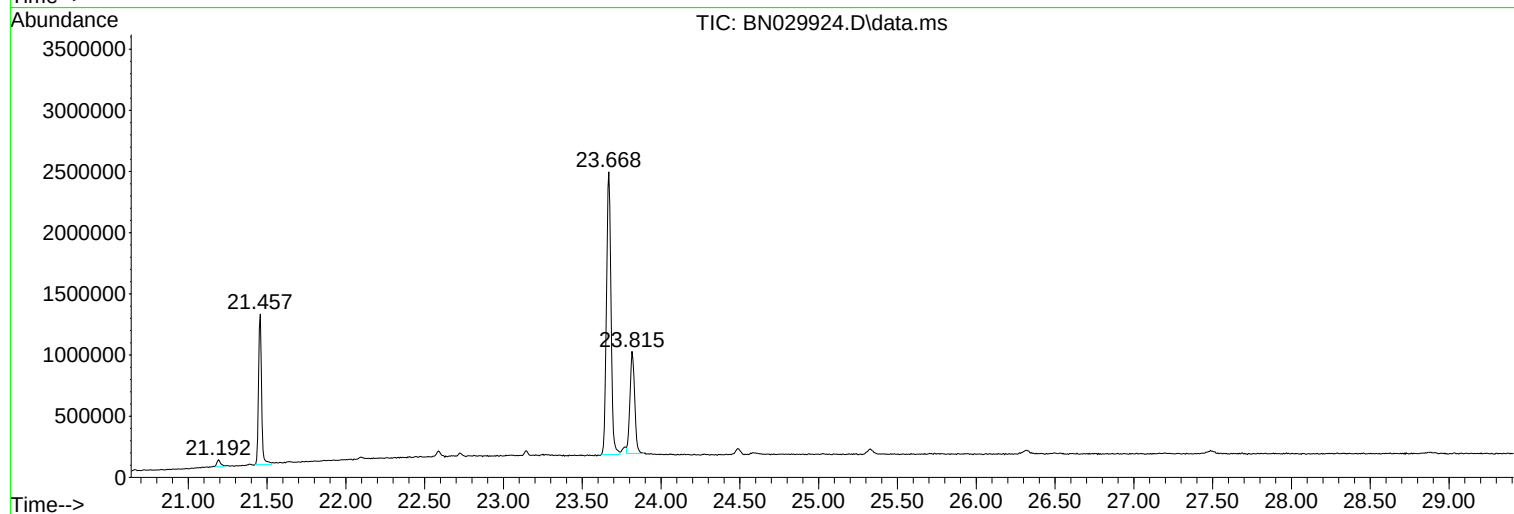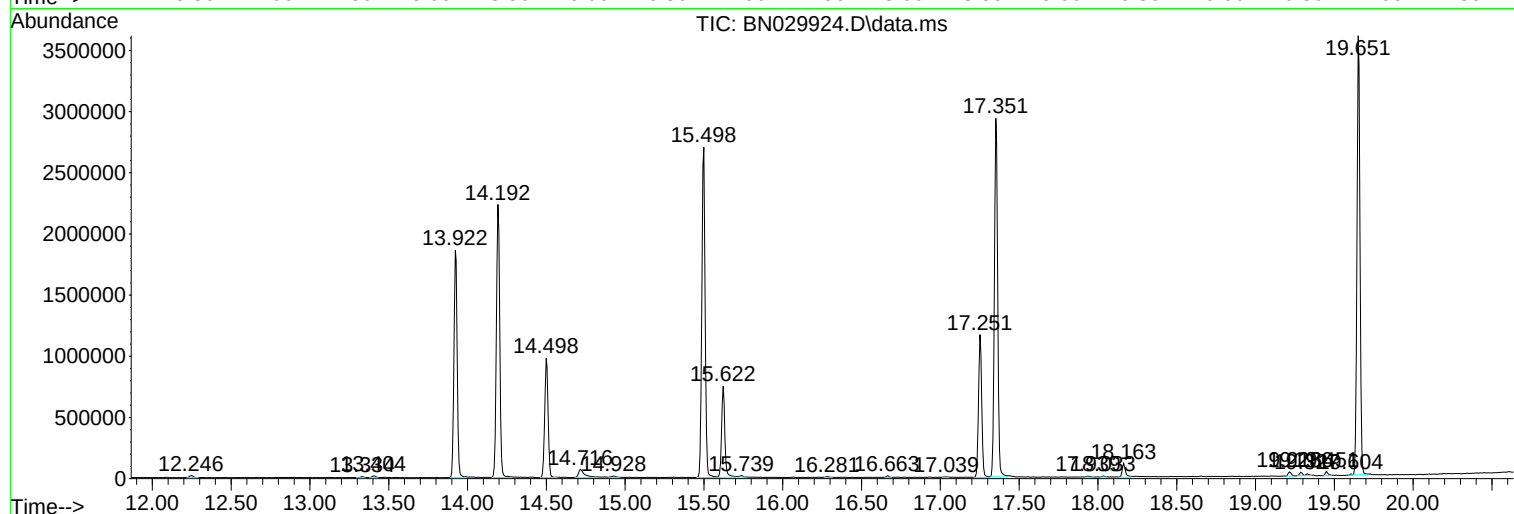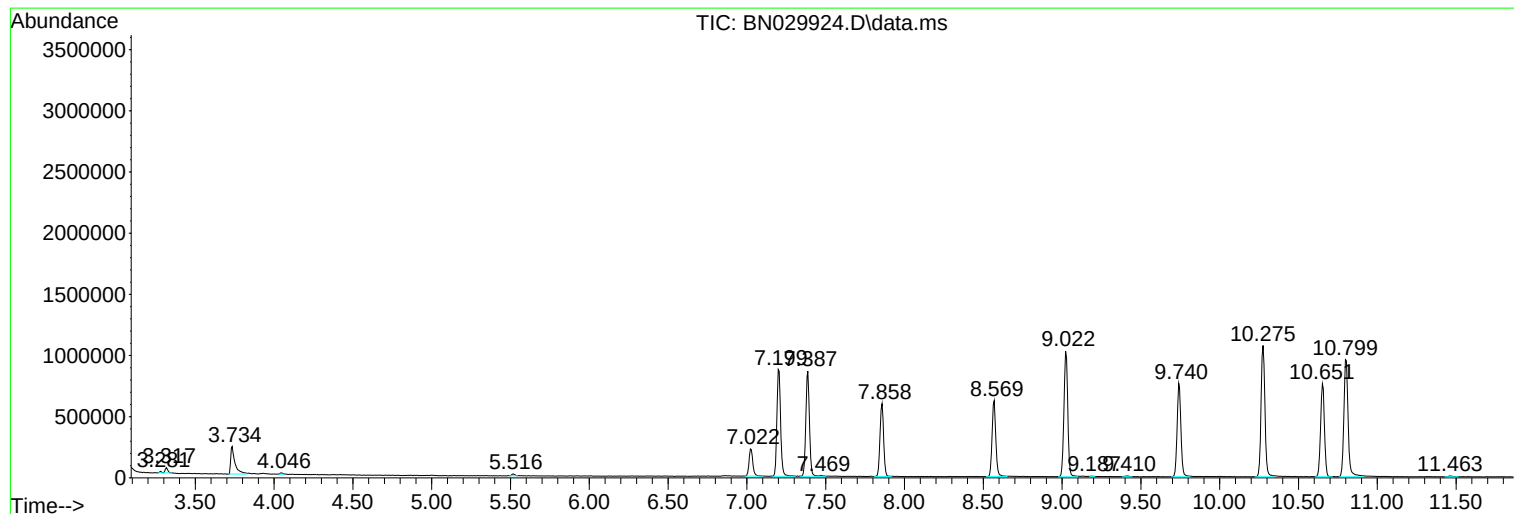

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029924.D
Acq On : 22 Feb 2024 12:38
Operator : MA/JU
Sample : P1493-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------