

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029925.D
 Acq On : 22 Feb 2024 13:14
 Operator : MA/JU
 Sample : P1493-20
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3W7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	45	rBV	43067	55497	1.16%	0.124%
2	3.734	107	110	125	rBV	133428	260706	5.43%	0.581%
3	4.046	160	163	168	rVB2	13005	16338	0.34%	0.036%
4	5.516	408	413	420	rBV	18470	29734	0.62%	0.066%
5	7.022	664	669	678	rBV	222391	359894	7.50%	0.802%
6	7.199	693	699	709	rBV	910937	1478155	30.79%	3.295%
7	7.387	722	731	742	rBV	884869	1425842	29.70%	3.178%
8	7.469	742	745	753	rVB9	6718	14395	0.30%	0.032%
9	7.858	802	811	819	rBV	567053	912179	19.00%	2.033%
10	8.569	925	932	947	rBV	618907	1035583	21.57%	2.308%
11	9.022	1002	1009	1020	rBV	1081916	1776206	37.00%	3.959%
12	9.193	1035	1038	1044	rVB7	3594	5246	0.11%	0.012%
13	9.416	1072	1076	1083	rVB7	6668	11350	0.24%	0.025%
14	9.740	1124	1131	1148	rBV	798343	1332485	27.76%	2.970%
15	10.275	1214	1222	1237	rBV	1116741	1885120	39.27%	4.202%
16	10.651	1279	1286	1296	rVB	745738	1224971	25.52%	2.730%
17	10.799	1301	1311	1332	rBV	870281	1633878	34.04%	3.642%
18	12.246	1552	1557	1563	rBV2	18365	32249	0.67%	0.072%
19	13.328	1737	1741	1745	rBV6	4143	5998	0.12%	0.013%
20	13.404	1747	1754	1760	rBV2	17577	27001	0.56%	0.060%
21	13.922	1835	1842	1856	rBV	1966369	2728239	56.83%	6.081%
22	14.192	1879	1888	1905	rBV	2250311	3331932	69.41%	7.426%
23	14.498	1933	1940	1950	rBV	960254	1384850	28.85%	3.087%
24	14.716	1971	1977	1990	rBV2	55551	148494	3.09%	0.331%
25	15.304	2075	2077	2081	rBV5	2915	4847	0.10%	0.011%
26	15.498	2103	2110	2125	rBV	2724748	3997335	83.27%	8.909%
27	15.622	2125	2131	2145	rVV	738711	1073393	22.36%	2.392%
28	15.734	2147	2150	2155	rVB5	14172	21389	0.45%	0.048%
29	16.069	2200	2207	2208	rBV6	4387	6732	0.14%	0.015%
30	16.286	2240	2244	2247	rVB4	8421	10164	0.21%	0.023%
31	17.251	2402	2408	2416	rBV	1104641	1544493	32.17%	3.442%
32	17.351	2419	2425	2439	rVV2	2953874	4290838	89.38%	9.563%
33	18.163	2556	2563	2567	rBV3	27270	40137	0.84%	0.089%
34	18.651	2642	2646	2650	rBV7	3685	6336	0.13%	0.014%
35	19.216	2737	2742	2750	rBV2	35126	49434	1.03%	0.110%
36	19.286	2750	2754	2761	rBV	30509	42070	0.88%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029925.D
Acq On : 22 Feb 2024 13:14
Operator : MA/JU
Sample : P1493-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.451	2778	2782	2785	rBV5	13609	16090	0.34%	0.036%
38	19.563	2799	2801	2804	rBV4	4023	4859	0.10%	0.011%
39	19.604	2804	2808	2810	rVV4	11192	14377	0.30%	0.032%
40	19.651	2810	2816	2836	rVB	3476755	4800486	100.00%	10.699%
41	20.216	2910	2912	2914	rBV3	5995	5842	0.12%	0.013%
42	21.457	3117	3123	3135	rBV	1108674	1546084	32.21%	3.446%
43	23.668	3491	3499	3510	rBV	2299529	4616833	96.17%	10.290%
44	23.816	3518	3524	3542	rVB	772267	1659046	34.56%	3.698%




Sum of corrected areas: 44867127

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029925.D
Acq On : 22 Feb 2024 13:14
Operator : MA/JU
Sample : P1493-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

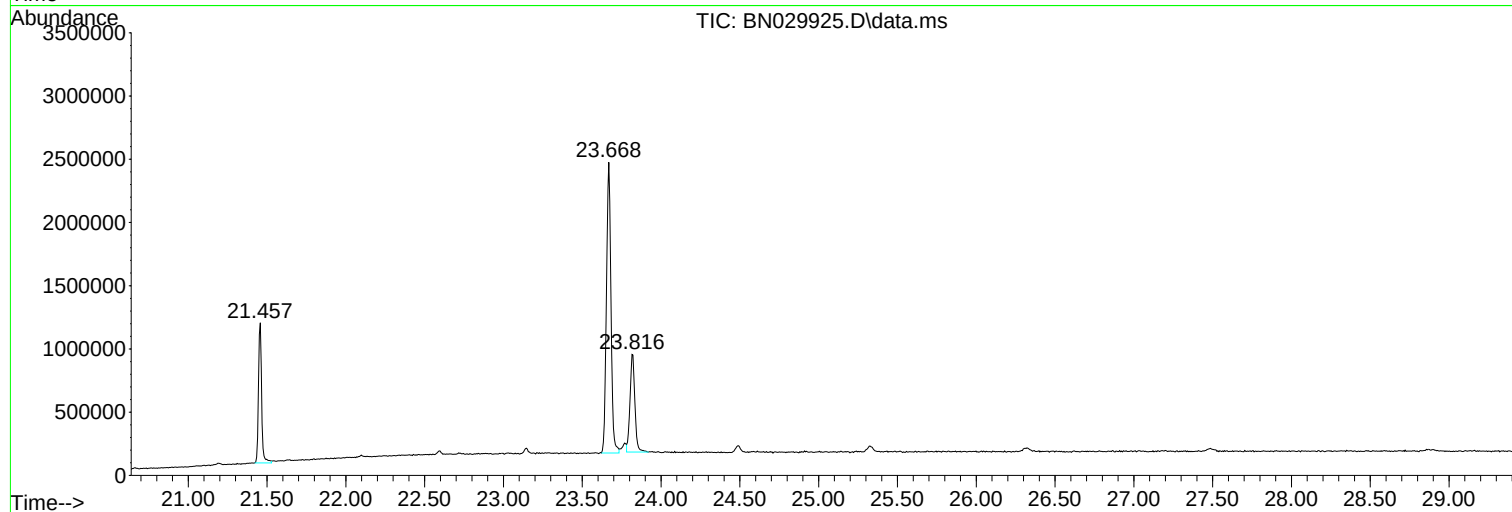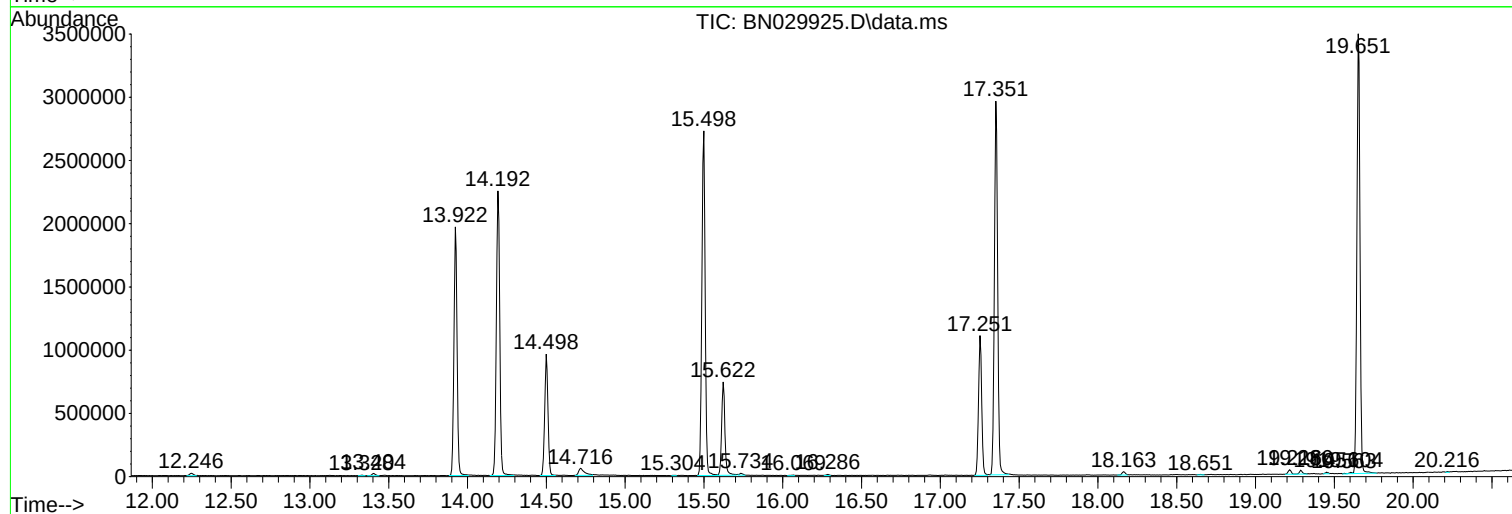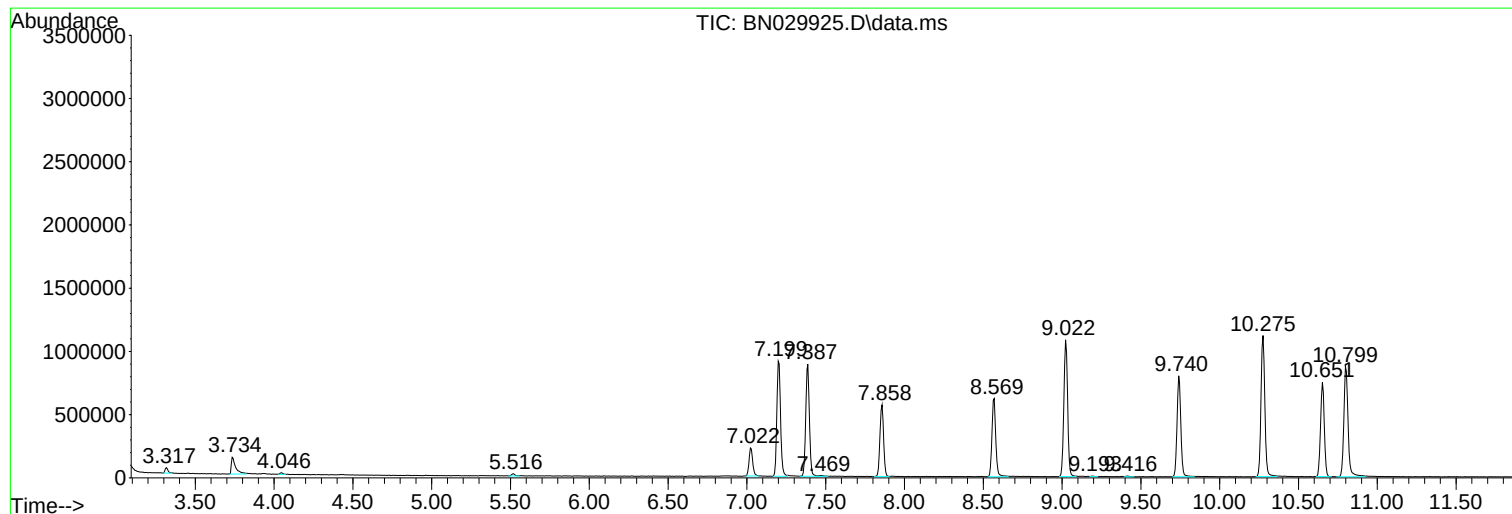

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029925.D
Acq On : 22 Feb 2024 13:14
Operator : MA/JU
Sample : P1493-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029925.D
Acq On : 22 Feb 2024 13:14
Operator : MA/JU
Sample : P1493-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc