

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029928.D
 Acq On : 22 Feb 2024 15:03
 Operator : MA/JU
 Sample : P1494-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	50	rVB	40836	55407	1.05%	0.125%
2	3.734	107	110	131	rBV	154021	304697	5.80%	0.687%
3	4.046	159	163	167	rVB	15075	18543	0.35%	0.042%
4	7.022	664	669	683	rBV	199180	328298	6.25%	0.740%
5	7.199	693	699	711	rBV	744755	1213044	23.10%	2.735%
6	7.387	723	731	741	rBV	723098	1187693	22.61%	2.678%
7	7.858	804	811	818	rBV	579683	932944	17.76%	2.103%
8	8.563	925	931	947	rBV	515885	894291	17.03%	2.016%
9	9.022	1002	1009	1024	rBV	893107	1481924	28.22%	3.341%
10	9.187	1033	1037	1042	rVB7	5252	6784	0.13%	0.015%
11	9.410	1071	1075	1081	rVB5	4790	7501	0.14%	0.017%
12	9.740	1124	1131	1143	rBV	670167	1119458	21.31%	2.524%
13	10.275	1215	1222	1234	rBV	930494	1591208	30.30%	3.588%
14	10.651	1278	1286	1298	rVB	776810	1303036	24.81%	2.938%
15	10.799	1303	1311	1326	rBV	836225	1543831	29.39%	3.481%
16	12.246	1550	1557	1563	rBV2	14837	26705	0.51%	0.060%
17	13.410	1747	1755	1760	rBV3	14720	25817	0.49%	0.058%
18	13.922	1835	1842	1854	rBV	1707434	2374683	45.21%	5.354%
19	14.192	1881	1888	1904	rBV	2012661	2942529	56.03%	6.634%
20	14.498	1933	1940	1952	rBV	1043257	1526342	29.06%	3.441%
21	14.716	1971	1977	1991	rBV2	60963	166879	3.18%	0.376%
22	14.928	2008	2013	2015	rBV6	3902	6552	0.12%	0.015%
23	15.498	2103	2110	2125	rBV	2436862	3591258	68.38%	8.097%
24	15.622	2125	2131	2147	rVV	810920	1168722	22.25%	2.635%
25	15.734	2147	2150	2155	rVB3	12204	17891	0.34%	0.040%
26	16.286	2240	2244	2249	rVB6	7179	11563	0.22%	0.026%
27	16.669	2304	2309	2315	rVB6	4687	7169	0.14%	0.016%
28	17.251	2402	2408	2418	rBV	1256589	1767204	33.65%	3.984%
29	17.351	2419	2425	2439	rVV2	3252015	4661307	88.75%	10.510%
30	18.033	2537	2541	2547	rBV7	8544	12116	0.23%	0.027%
31	18.163	2558	2563	2570	rBV2	49175	71377	1.36%	0.161%
32	19.216	2737	2742	2748	rBV3	36050	52476	1.00%	0.118%
33	19.286	2750	2754	2758	rVV	32742	47522	0.90%	0.107%
34	19.333	2758	2762	2765	rVV5	12850	21511	0.41%	0.049%
35	19.363	2765	2767	2772	rVB6	6630	9660	0.18%	0.022%
36	19.451	2778	2782	2788	rBV5	22477	31649	0.60%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029928.D
Acq On : 22 Feb 2024 15:03
Operator : MA/JU
Sample : P1494-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.604	2805	2808	2811	rBV3	13082	17953	0.34%	0.040%
38	19.651	2811	2816	2826	rVV	3743777	5252023	100.00%	11.842%
39	20.663	2985	2988	2991	rBV5	14829	20051	0.38%	0.045%
40	21.457	3118	3123	3135	rBV	1321732	1742444	33.18%	3.929%
41	23.668	3492	3499	3511	rBV2	2505396	5005199	95.30%	11.285%
42	23.821	3519	3525	3535	rVB	877300	1784859	33.98%	4.024%




Sum of corrected areas: 44352120

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029928.D
Acq On : 22 Feb 2024 15:03
Operator : MA/JU
Sample : P1494-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

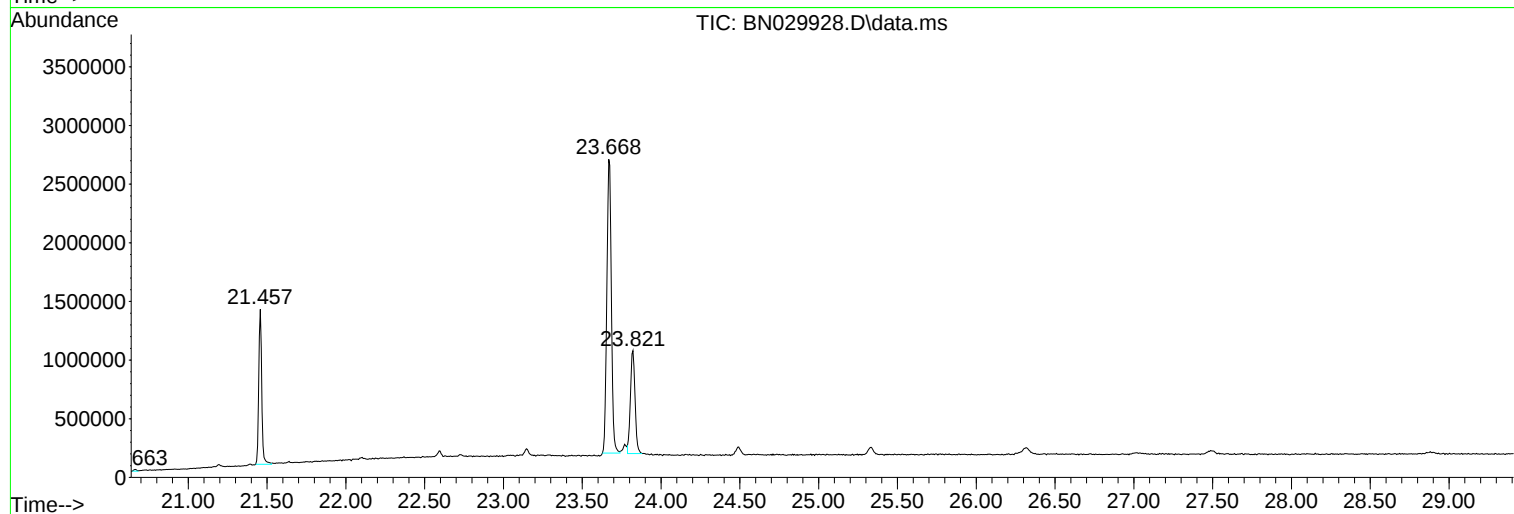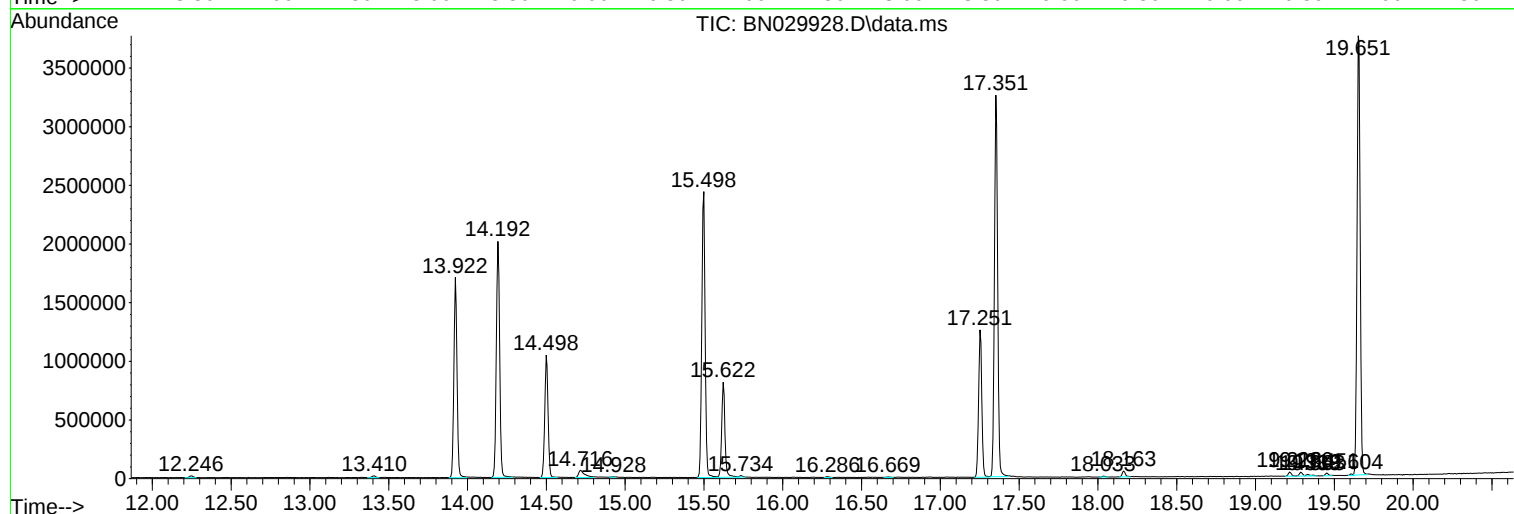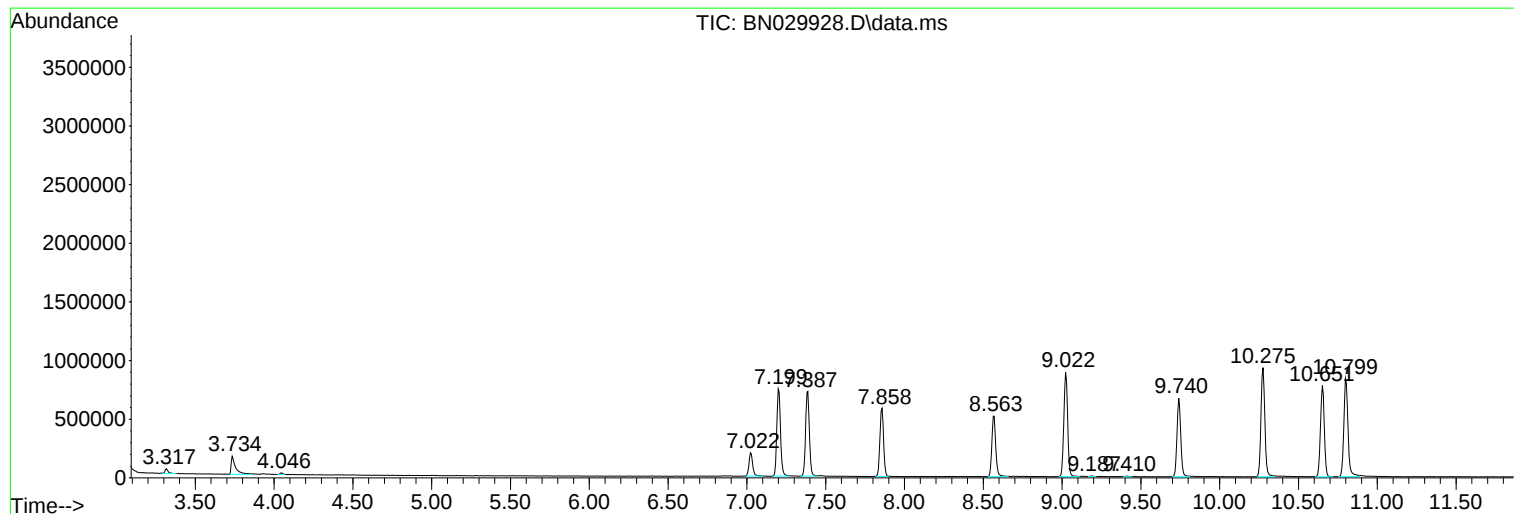

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029928.D
Acq On : 22 Feb 2024 15:03
Operator : MA/JU
Sample : P1494-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029928.D
Acq On : 22 Feb 2024 15:03
Operator : MA/JU
Sample : P1494-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc